


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF071118\
 Data File : BF107318.D
 Acq On : 11 Jul 2018 23:46
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jul 11 16:39:37 2018

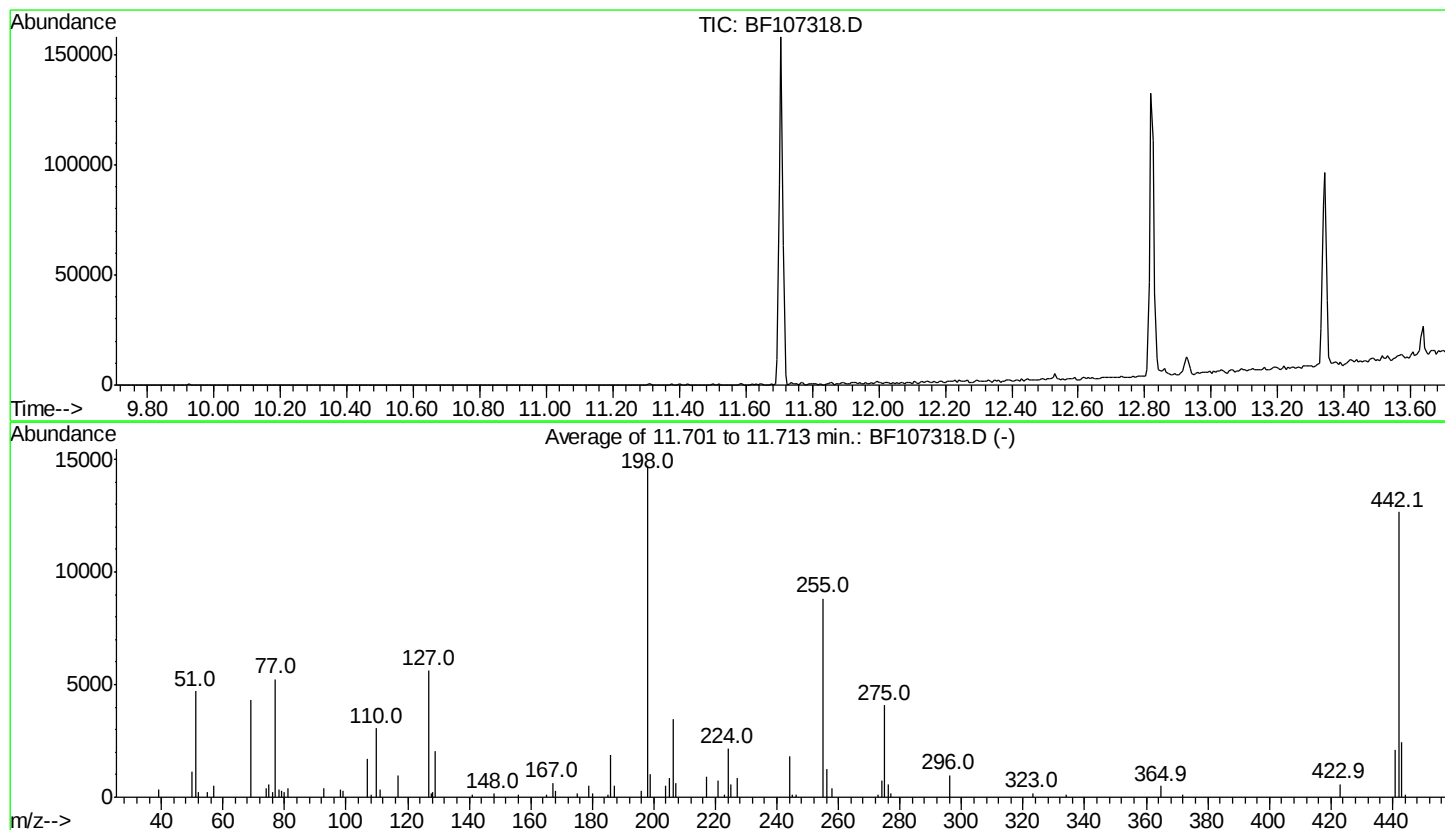

AutoFind: Scans 1592, 1593, 1594; Background Corrected with Scan 1588

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.0	4706	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	29.2	4297	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	38.2	5618	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	14711	PASS
199	198	5	9	7.0	1032	PASS
275	198	10	60	27.6	4065	PASS
365	198	1	100	3.4	503	PASS
441	198	0.01	100	14.1	2077	PASS
442	198	50	100	86.1	12664	PASS
443	442	15	24	19.4	2455	PASS