

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF071216\
 Data File : BF088944.D
 Acq On : 13 Jul 2016 4:52
 Operator : UM/SJ
 Sample : H3987-02
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 COMP-WALL-W-070816

Quant Time: Jul 13 06:52:31 2016
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 11 18:13:32 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.71	152	58759	20.00	ng	0.00
21) Naphthalene-d8	7.99	136	240918	20.00	ng	-0.01
38) Acenaphthene-d10	9.74	164	96758	20.00	ng	-0.01
63) Phenanthrene-d10	11.21	188	141622	20.00	ng	-0.01
75) Chrysene-d12	13.84	240	125482	20.00	ng	-0.01
86) Perylene-d12	15.21	264	109441	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.30	112	338656	86.38	ng	0.01
7) Phenol-d6	6.35	99	486795	96.09	ng	0.00
23) Nitrobenzene-d5	7.27	82	292028	63.52	ng	-0.01
41) 2,4,6-Tribromophenol	10.52	330	69356	77.19	ng	-0.01
44) 2-Fluorobiphenyl	9.07	172	563857	92.05	ng	0.00
78) Terphenyl-d14	12.80	244	364211	64.65	ng	0.00
Target Compounds						
19) n-Nitroso-di-n-propylamine	7.27	70	40001	11.76	ng	# 74
25) Isophorone	7.27	82	227749	26.74	ng	# 65
49) Dimethylphthalate	9.46	163	108615	15.76	ng	99
56) 2,4-Dinitrotoluene	9.74	165	12316	6.17	ng	# 36
66) 4-Bromophenyl-phenylether	10.52	248	4658	3.26	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF071216\
Data File : BF088944.D
Acq On : 13 Jul 2016 4:52
Operator : UM/SJ
Sample : H3987-02
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
COMP-WALL-W-070816

Quant Time: Jul 13 06:52:31 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 11 18:13:32 2016
Response via : Initial Calibration

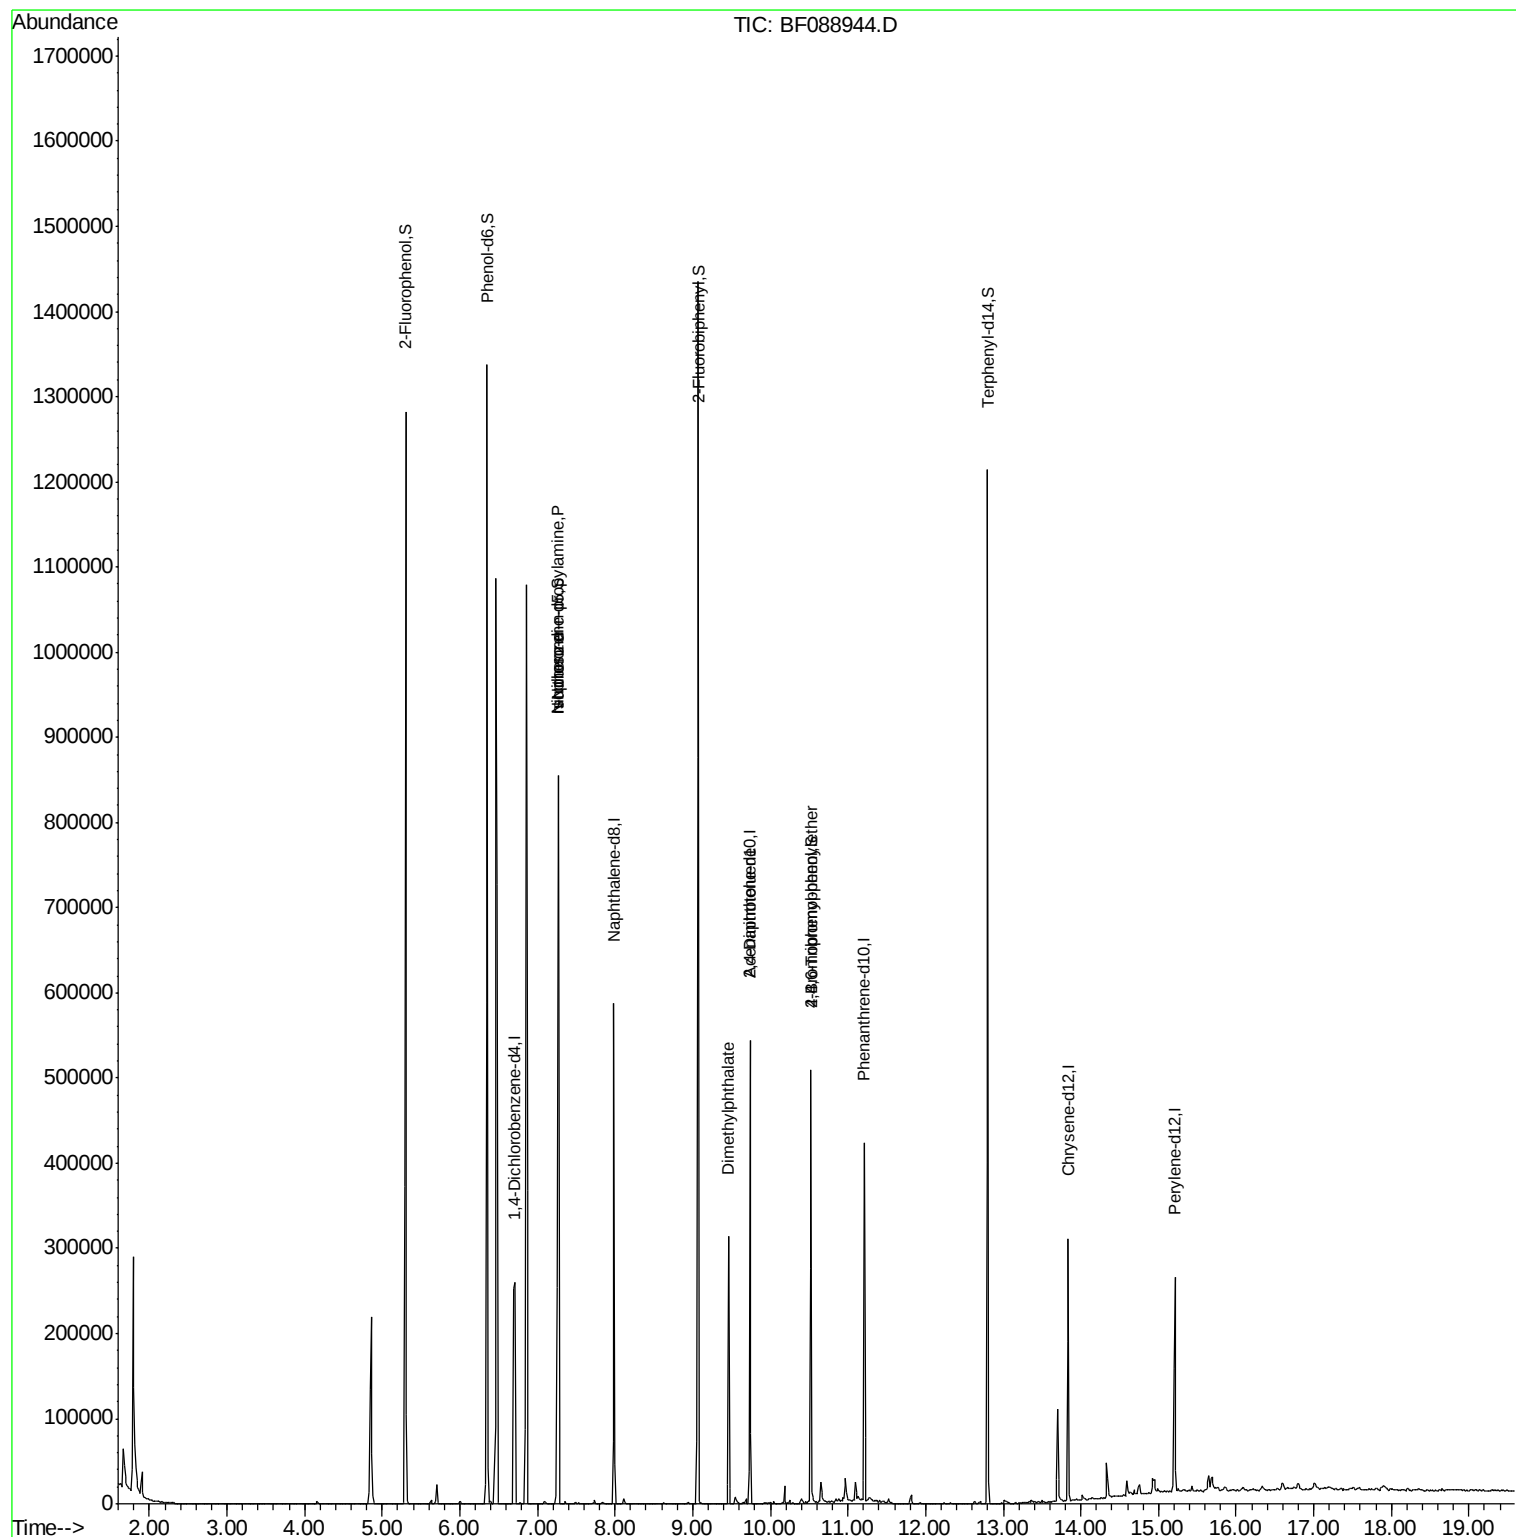

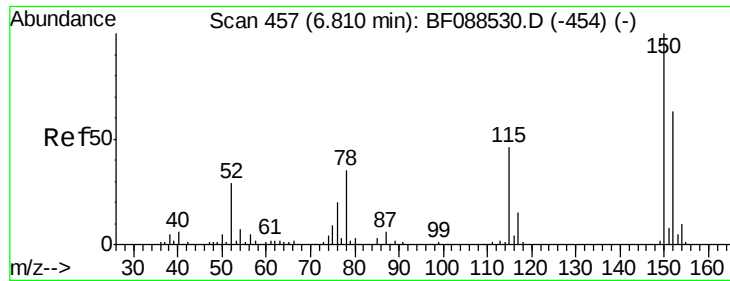

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.71 min Scan# 448

Delta R.T. -0.00 min

Lab File: BF088944.D

Acq: 13 Jul 2016 4:52

Instrument :

BNA_F

ClientSampleId :

COMP-WALL-W-070816


Tgt Ion:152 Resp: 58759

Ion Ratio Lower Upper

152 100

150 152.0 123.8 185.6



115 53.9 39.6 59.4

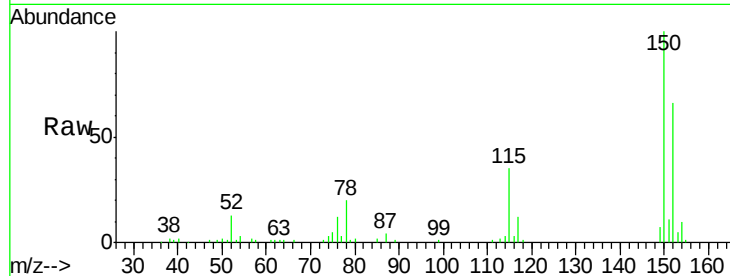

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

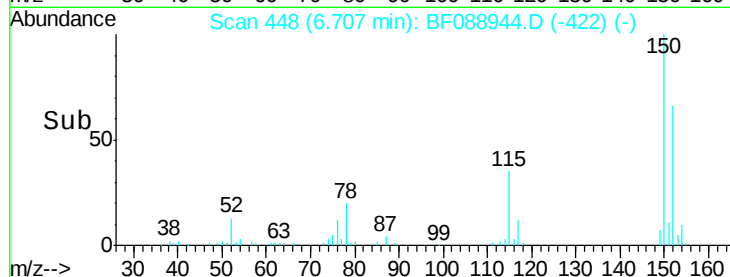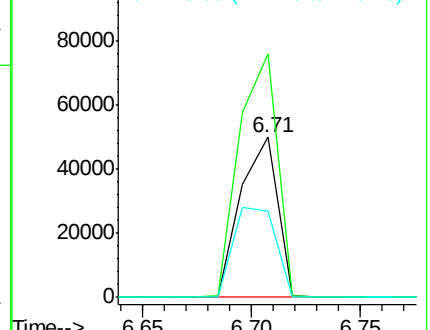

#5

2-Fluorophenol

Concen: 86.38 ng

RT: 5.30 min Scan# 325

Delta R.T. 0.01 min

Lab File: BF088944.D

Acq: 13 Jul 2016 4:52


Tgt Ion:112 Resp: 338656

Ion Ratio Lower Upper

112 100

64 60.2 42.2 63.2



63 32.0 21.8 32.8


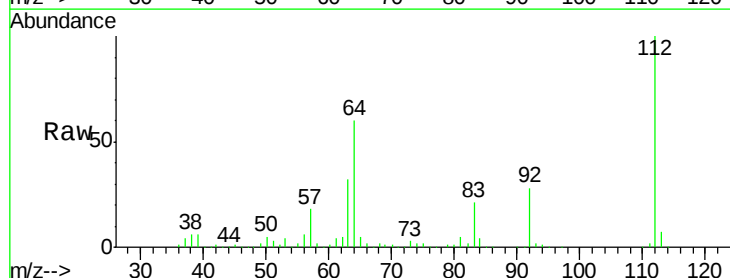


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

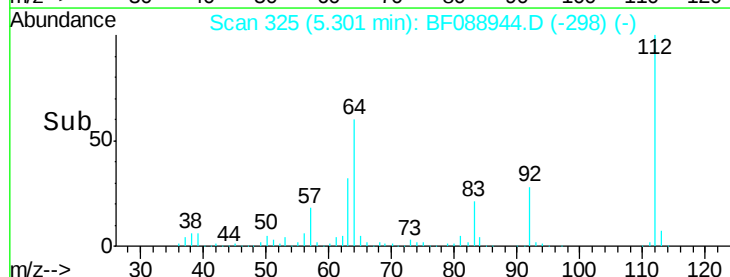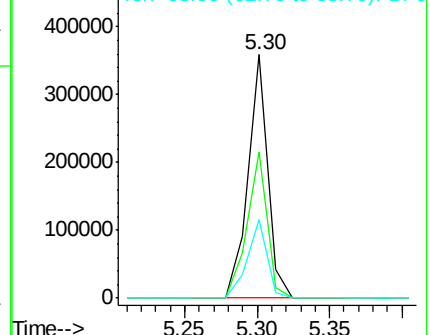

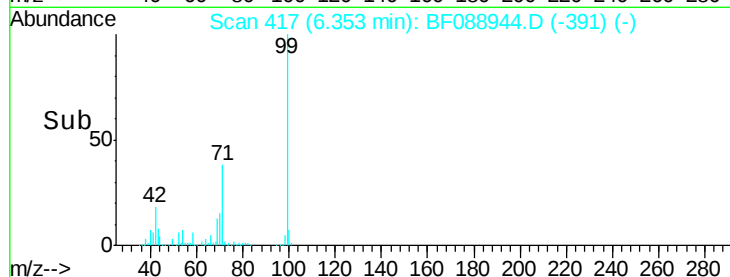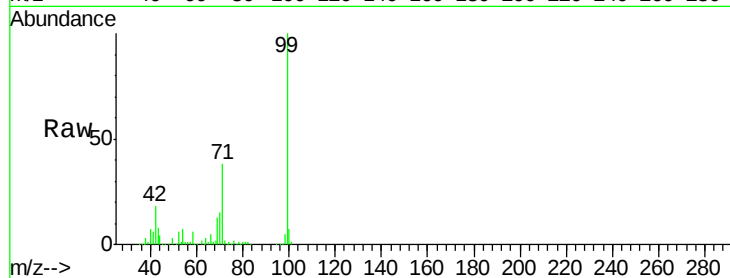

#7

Phenol-d6

Concen: 96.09 ng

RT: 6.35 min Scan# 417

Delta R.T. -0.00 min

Lab File: BF088944.D

Acq: 13 Jul 2016 4:52

Instrument :

BNA_F

ClientSampleId :

COMP-WALL-W-070816





Tgt Ion: 99 Resp: 486795

Ion Ratio Lower Upper

99 100

42 17.8 12.2 18.2

71 37.6 23.4 35.0#

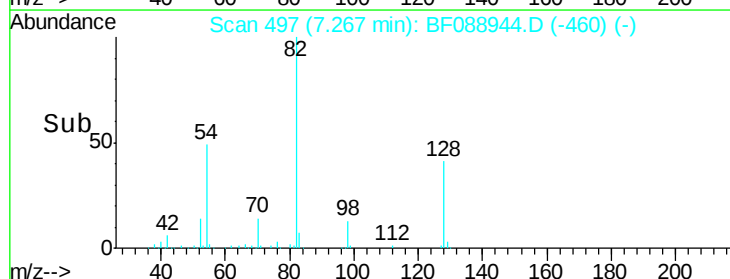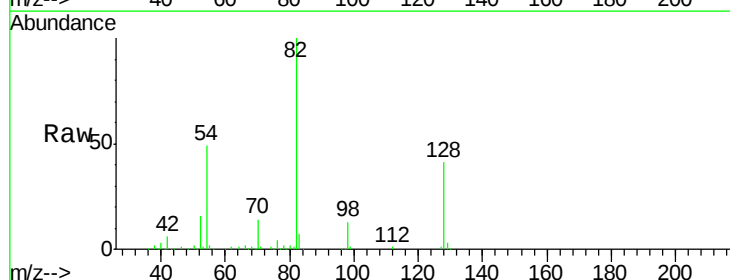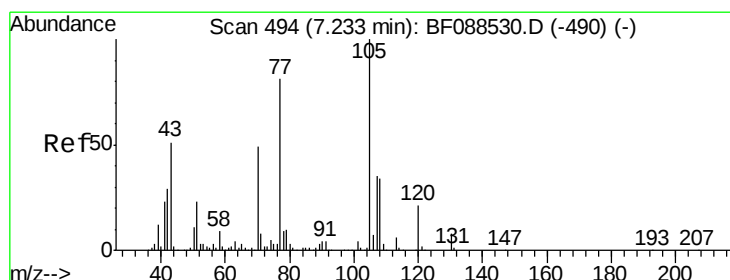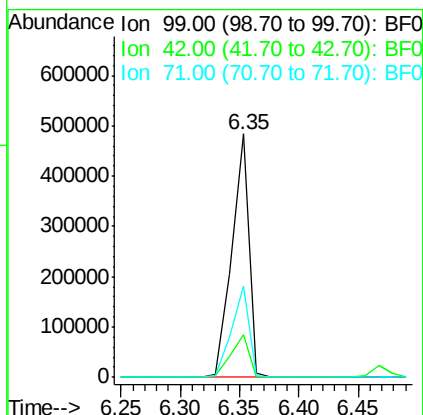

#19

n-Nitroso-di-n-propylamine

Concen: 11.76 ng

RT: 7.27 min Scan# 497

Delta R.T. 0.13 min

Lab File: BF088944.D

Acq: 13 Jul 2016 4:52

Tgt Ion: 70 Resp: 40001


Ion Ratio Lower Upper

70 100

42 45.1 49.6 74.4#

101 0.0 7.1 10.7#

130 1.9 15.4 23.2#

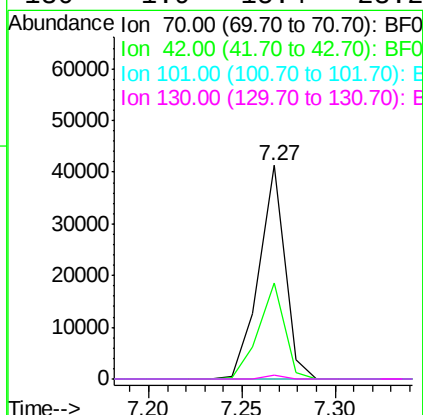



#21

Naphthalene-d8

Concen: 20.00 ng

RT: 7.99 min Scan# 560

Delta R.T. -0.01 min

Lab File: BF088944.D

Acq: 13 Jul 2016 4:52

Instrument :

BNA_F

ClientSampleId :

COMP-WALL-W-070816

Tgt Ion: 136 Resp: 240918


Ion Ratio Lower Upper

136 100

137 10.7 9.1 13.7

54 7.5 6.6 10.0

68 6.1 5.1 7.7





Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

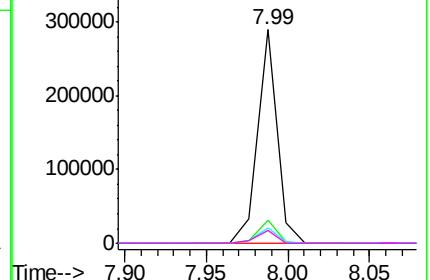

#23

Nitrobenzene-d5

Concen: 63.52 ng

RT: 7.27 min Scan# 497

Delta R.T. -0.01 min

Lab File: BF088944.D

Acq: 13 Jul 2016 4:52


Tgt Ion: 82 Resp: 292028

Ion Ratio Lower Upper

82 100

128 40.7 35.9 53.9



54 49.0 40.9 61.3




Abundance Ion 82.00 (81.70 to 82.70): BF0

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF0

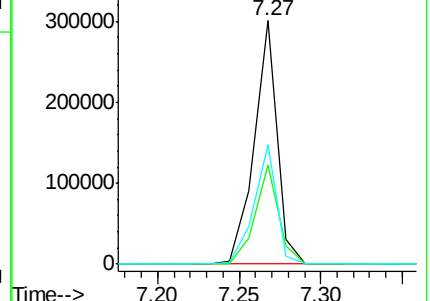

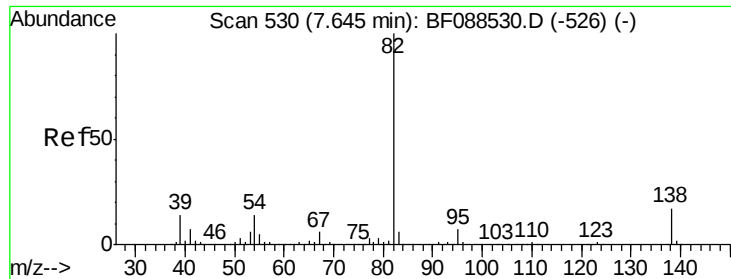

#25

Isophorone

Concen: 26.74 ng

RT: 7.27 min Scan# 497

Delta R.T. -0.27 min

Lab File: BF088944.D

Acq: 13 Jul 2016 4:52

Instrument :

BNA_F

ClientSampleId :

COMP-WALL-W-070816


Tgt Ion: 82 Resp: 227749

Ion Ratio Lower Upper

82 100

95 0.0 5.4 8.2#




138 0.0 14.6 21.8#

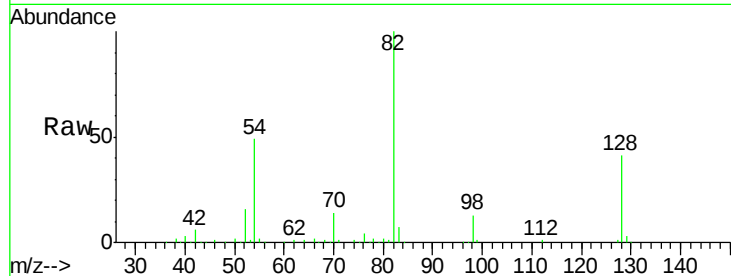

Abundance Ion 82.00 (81.70 to 82.70): BF0

Ion 95.00 (94.70 to 95.70): BF0

Ion 138.00 (137.70 to 138.70): BF0

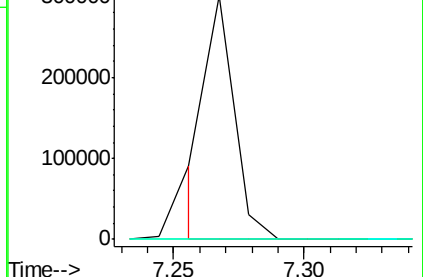

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 9.74 min Scan# 713

Delta R.T. -0.01 min

Lab File: BF088944.D

Acq: 13 Jul 2016 4:52


Tgt Ion: 164 Resp: 96758

Ion Ratio Lower Upper

164 100

162 105.3 85.4 128.2



160 47.1 39.5 59.3




Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E




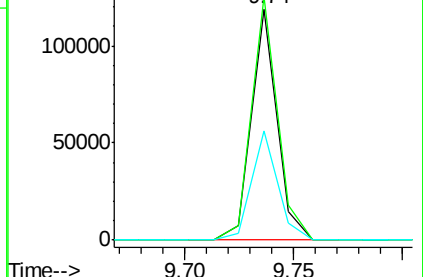


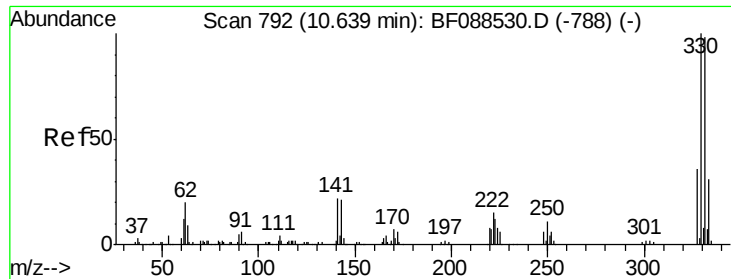

#41
 2,4,6-Tribromophenol
 Concen: 77.19 ng
 RT: 10.52 min Scan# 782
 Delta R.T. -0.01 min
 Lab File: BF088944.D
 Acq: 13 Jul 2016 4:52




Instrument :
 BNA_F
 ClientSampleId :
 COMP-WALL-W-070816


Tgt Ion	Ratio	Lower	Upper
330	100		
332	95.8	0.0	0.0#
141	36.4	0.0	0.0#

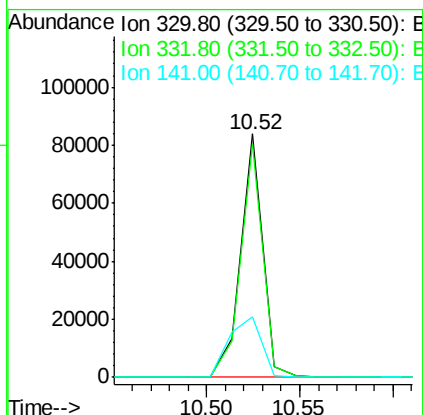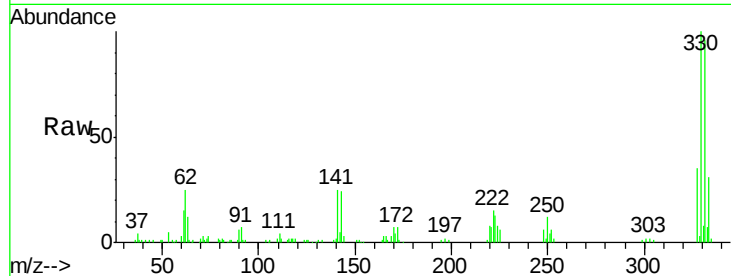

#44
 2-Fluorobiphenyl
 Concen: 92.05 ng
 RT: 9.07 min Scan# 655
 Delta R.T. -0.00 min
 Lab File: BF088944.D
 Acq: 13 Jul 2016 4:52

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.5	28.6	43.0
170	23.8	19.2	28.8

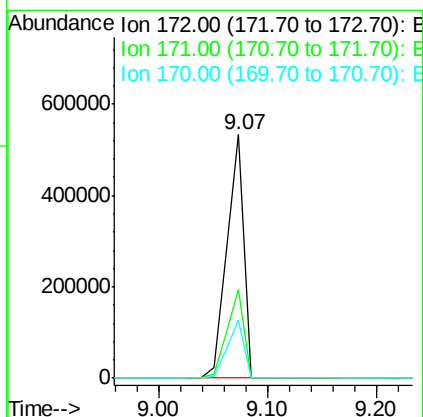

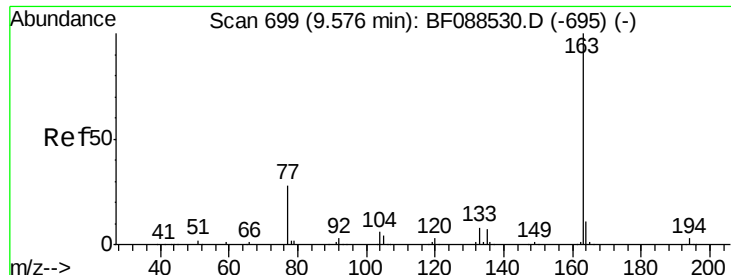

#49

Dimethylphthalate

Concen: 15.76 ng

RT: 9.46 min Scan# 689

Delta R.T. -0.02 min

Lab File: BF088944.D

Acq: 13 Jul 2016 4:52

Instrument :

BNA_F

ClientSampleId :

COMP-WALL-W-070816


Tgt Ion:163 Resp: 108615

Ion Ratio Lower Upper

163 100

194 3.2 2.8 4.2




164 10.2 8.3 12.5



Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

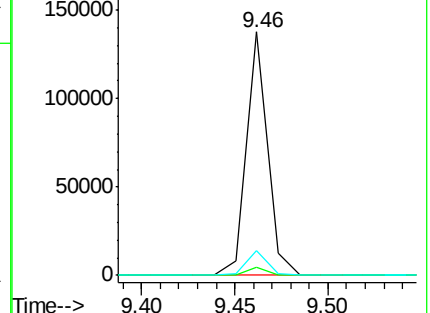

#56

2,4-Dinitrotoluene

Concen: 6.17 ng

RT: 9.74 min Scan# 713

Delta R.T. -0.21 min

Lab File: BF088944.D

Acq: 13 Jul 2016 4:52

Tgt Ion:165 Resp: 12316


Ion Ratio Lower Upper

165 100

63 0.0 22.0 33.0#

89 0.0 41.1 61.7#

182 0.0 2.0 3.0#





Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF0

Ion 89.00 (88.70 to 89.70): BF0

Ion 182.00 (181.70 to 182.70): E



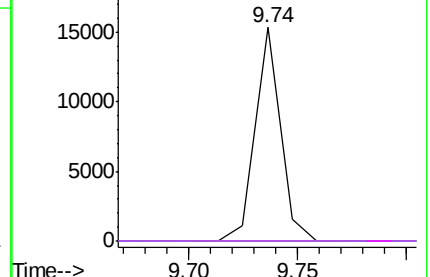





#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.21 min Scan# 842
Delta R.T. -0.01 min
Lab File: BF088944.D
Acq: 13 Jul 2016 4:52




Instrument :
BNA_F
ClientSampleId :
COMP-WALL-W-070816


Tgt Ion:188 Resp: 141622
Ion Ratio Lower Upper
188 100
94 11.2 9.0 13.6
80 12.6 10.0 15.0

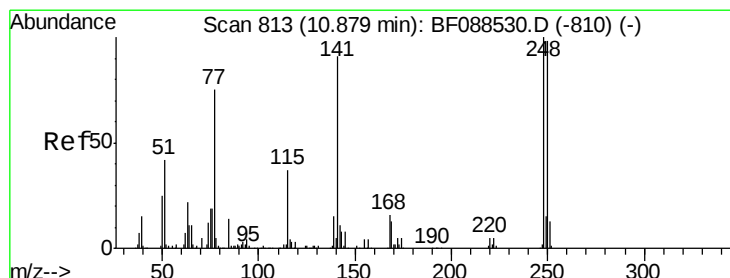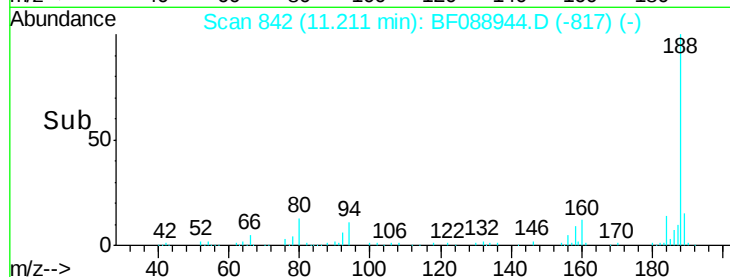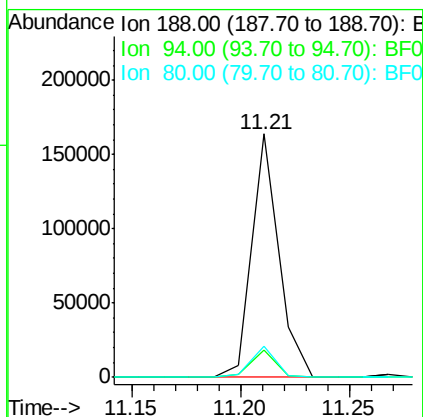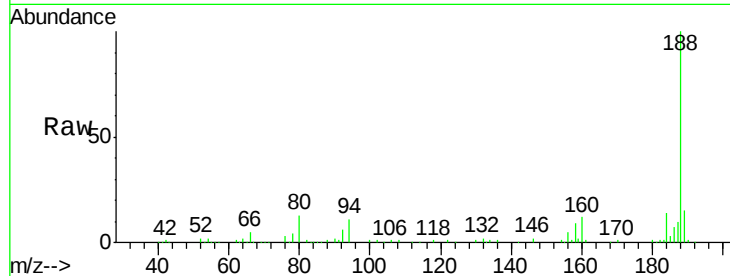

#66
4-Bromophenyl-phenylether
Concen: 3.26 ng
RT: 10.52 min Scan# 782
Delta R.T. -0.25 min
Lab File: BF088944.D
Acq: 13 Jul 2016 4:52

Tgt Ion:248 Resp: 4658
Ion Ratio Lower Upper
248 100
250 198.9 77.1 115.7#
141 401.9 50.6 76.0#

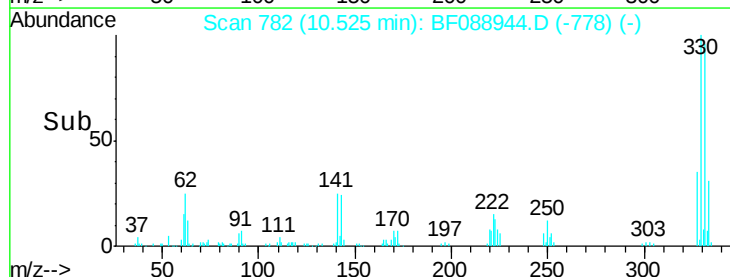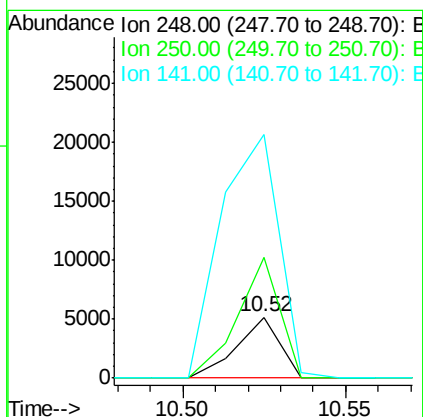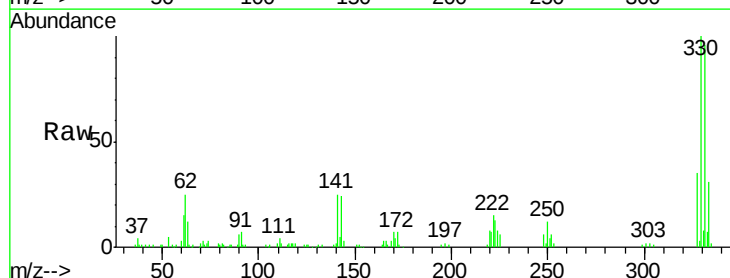

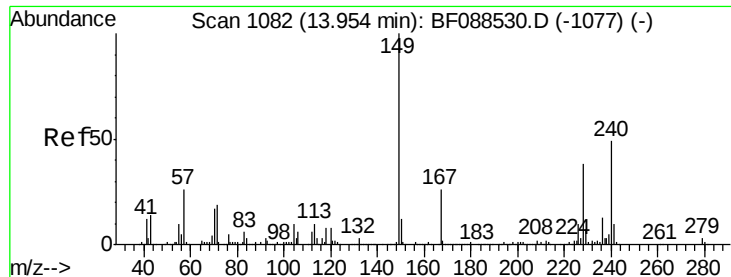

#75

Chrysene-d12

Concen: 20.00 ng

RT: 13.84 min Scan# 1072

Delta R.T. -0.01 min

Lab File: BF088944.D

Acq: 13 Jul 2016 4:52

Instrument :

BNA_F

ClientSampleId :

COMP-WALL-W-070816


Tgt Ion:240 Resp: 125482

Ion Ratio Lower Upper

240 100

120 7.9 6.8 10.2




236 25.4 20.2 30.2



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

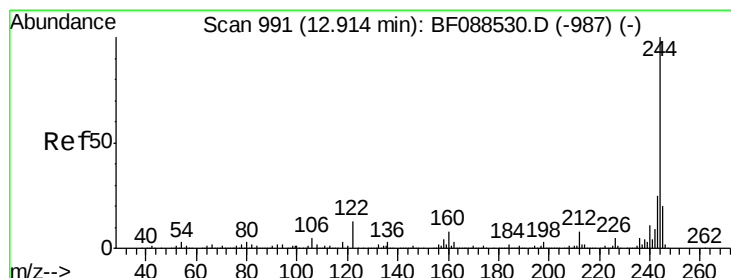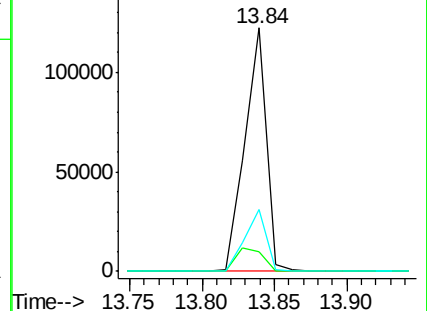

#78

Terphenyl-d14

Concen: 64.65 ng

RT: 12.80 min Scan# 981

Delta R.T. -0.00 min

Lab File: BF088944.D

Acq: 13 Jul 2016 4:52


Tgt Ion:244 Resp: 364211

Ion Ratio Lower Upper

244 100

212 7.4 6.0 9.0



122 10.8 11.2 16.8#




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

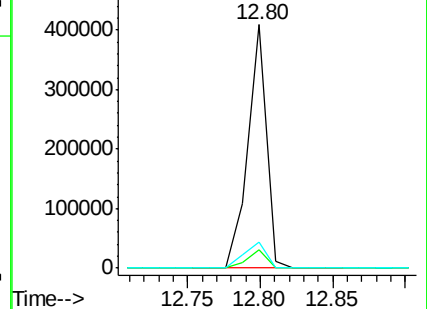

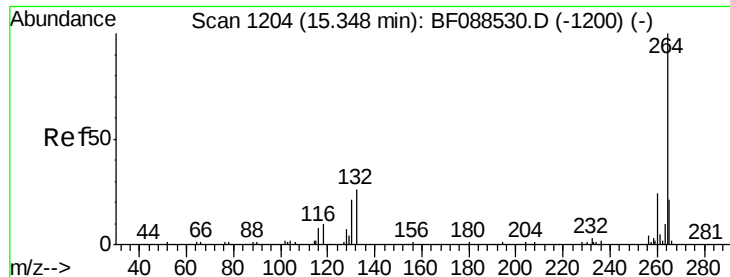

#86

Perylene-d12

Concen: 20.00 ng

RT: 15.21 min Scan# 1192

Delta R.T. -0.00 min

Lab File: BF088944.D

Acq: 13 Jul 2016 4:52

Instrument :

BNA_F

ClientSampleId :

COMP-WALL-W-070816


Tgt Ion:264 Resp: 109441

Ion Ratio Lower Upper

264 100

260 23.3 19.2 28.8

265 21.1 16.9 25.3

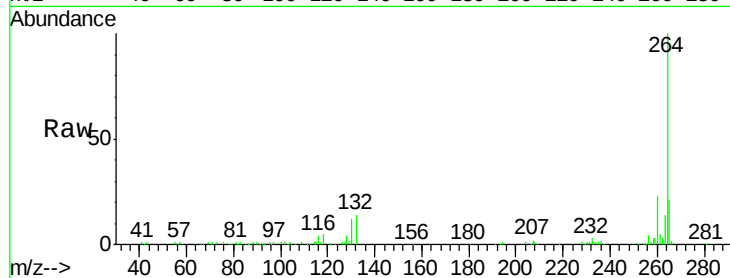

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

