


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF071216\
 Data File : BF088920.D
 Acq On : 12 Jul 2016 12:59
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jul 11 18:13:32 2016

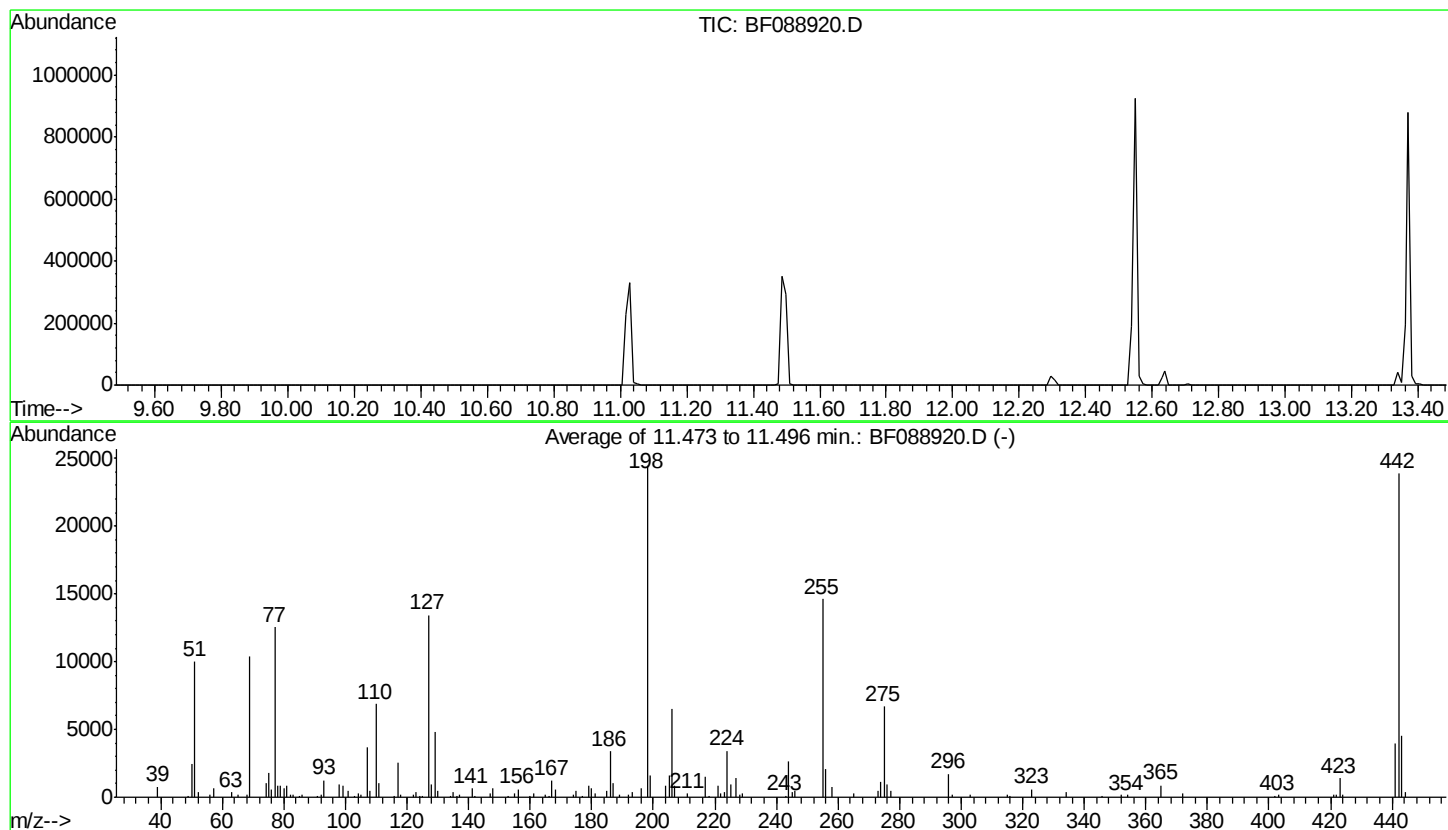

AutoFind: Scans 865, 866, 867; Background Corrected with Scan 862

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.9	10009	PASS
68	69	0.00	2	1.7	174	PASS
69	198	0.00	100	42.6	10412	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	54.9	13435	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	24464	PASS
199	198	5	9	6.5	1597	PASS
275	198	10	60	27.3	6673	PASS
365	198	1	100	3.6	891	PASS
441	442	0.01	24	16.5	3939	PASS
442	198	50	100	97.7	23893	PASS
443	442	15	24	19.0	4531	PASS