
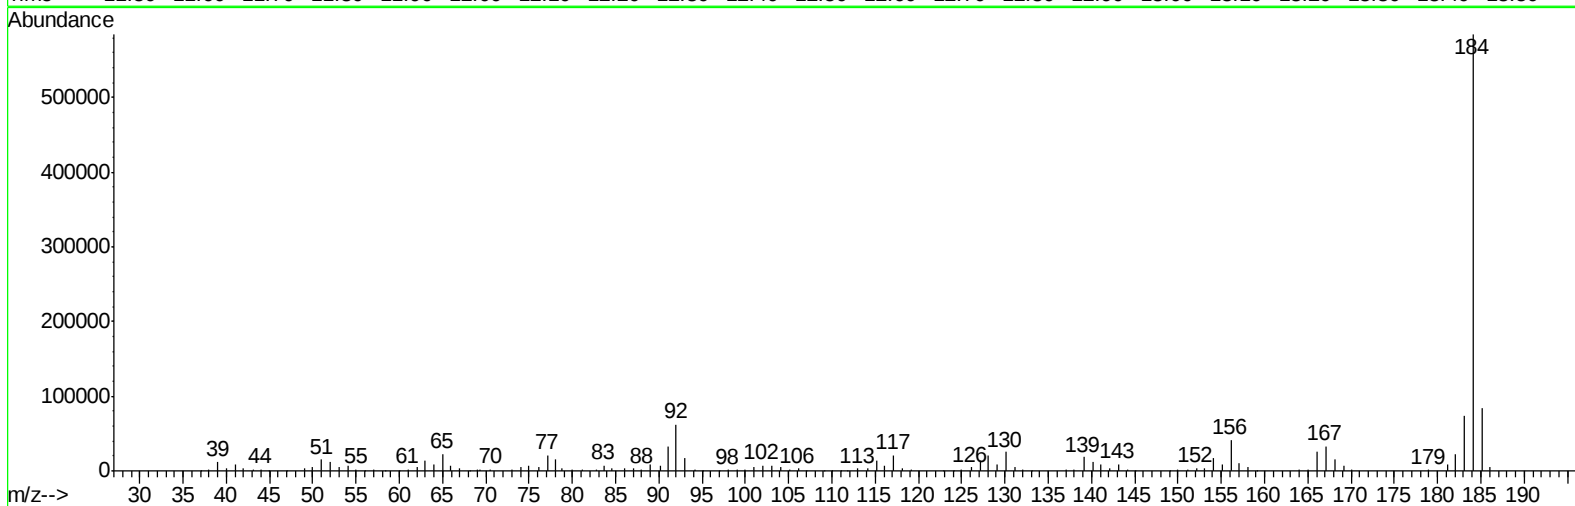


Data Path : Z:\HPCHEM1\BNA F\DATA\BF071217\  
Data File : BF096686.D  
Acq On : 12 Jul 2017 12:35  
Operator : SJ/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 13 06:09:04 2017  
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF070117.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Jul 07 13:02:33 2017  
Response via : Initial Calibration

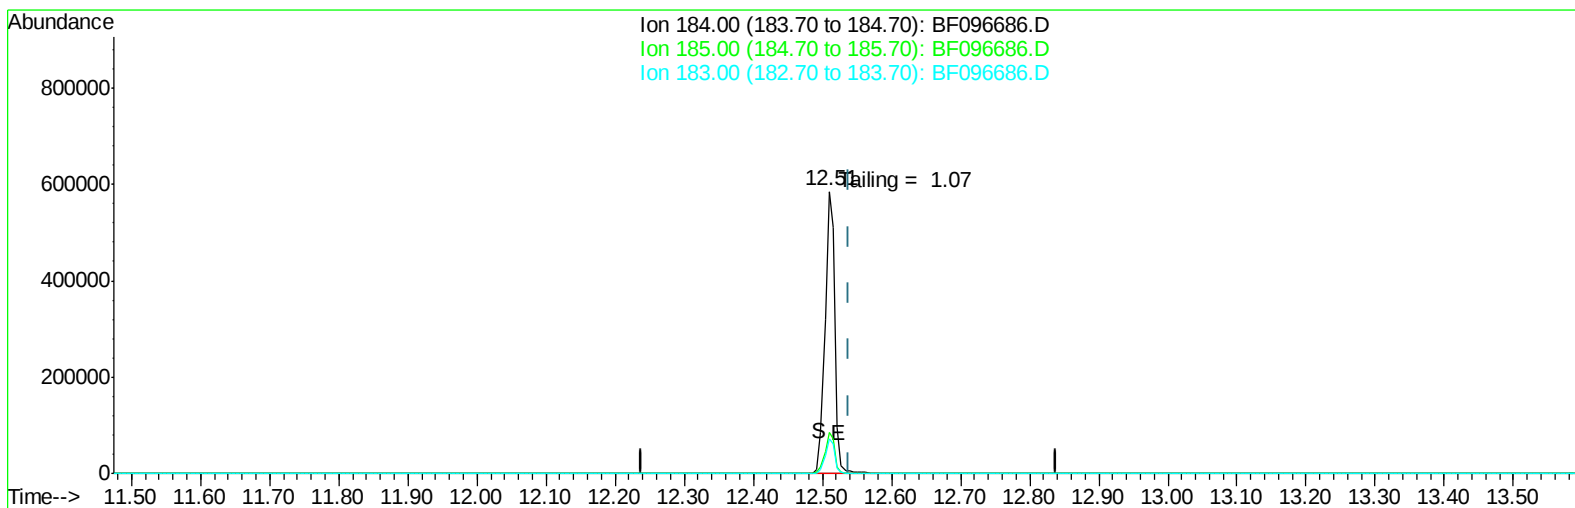

TIC: BF096686.D

(76) Benzidine

12.510min (-0.029) 0.00ng m

response 580082

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 184.00 | 100   | 100    |
| 185.00 | 19.40 | 14.47# |
| 183.00 | 12.20 | 12.51  |
| 0.00   | 0.00  | 0.00   |