
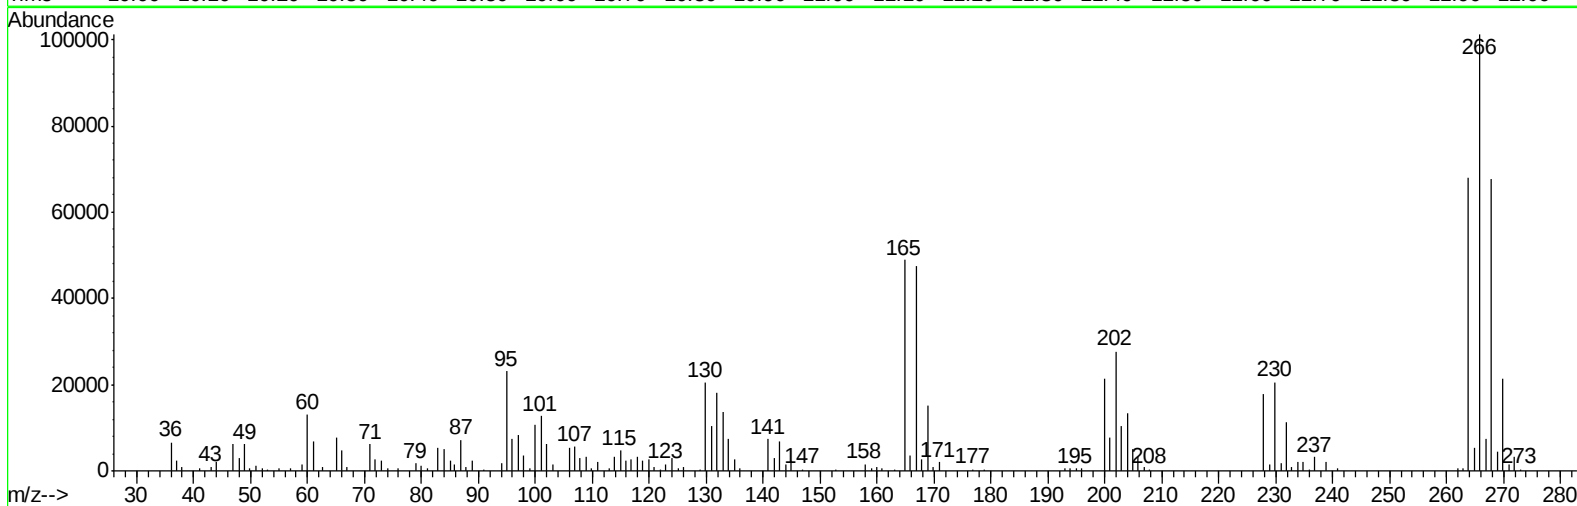


Data Path : Z:\HPCHEM1\BNA F\DATA\BF071217\
Data File : BF096686.D
Acq On : 12 Jul 2017 12:35
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 13 06:07:25 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF070117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 07 13:02:33 2017
Response via : Initial Calibration

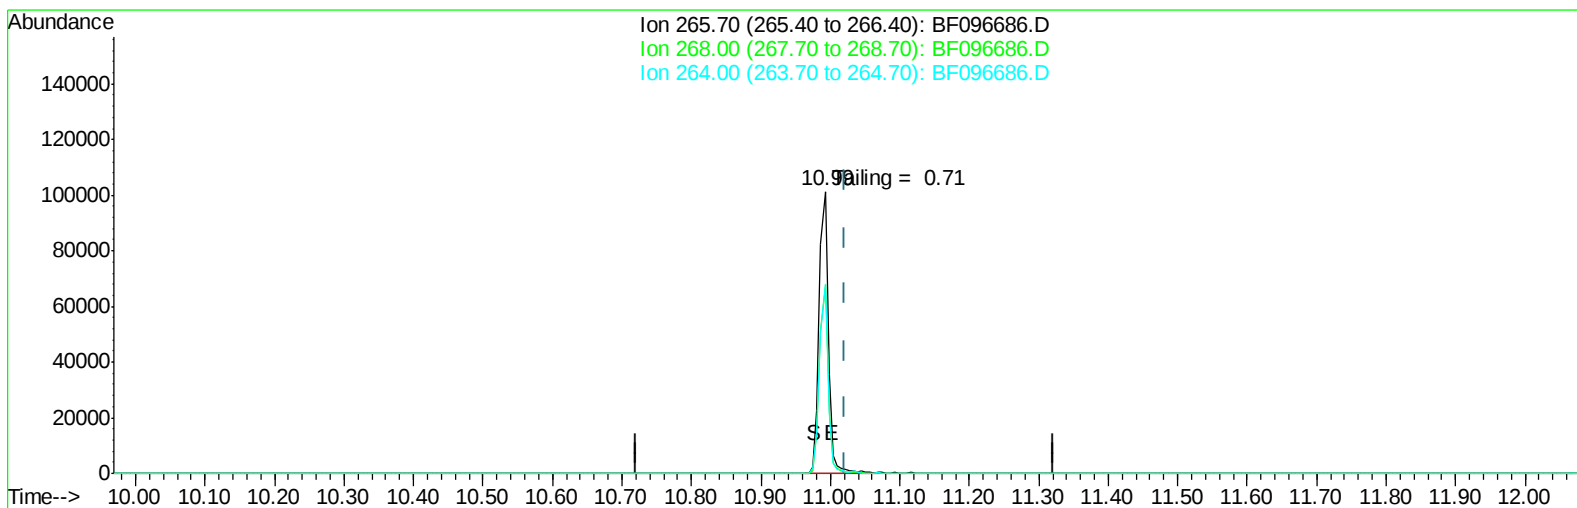

TIC: BF096686.D

(69) Pentachlorophenol (C)



10.992min (-0.029) 51213.30ng

response 91859

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	66.80
264.00	64.60	67.23
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF071217\
Data File : BF096686.D
Acq On : 12 Jul 2017 12:35
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 13 06:09:04 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF070117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 07 13:02:33 2017
Response via : Initial Calibration

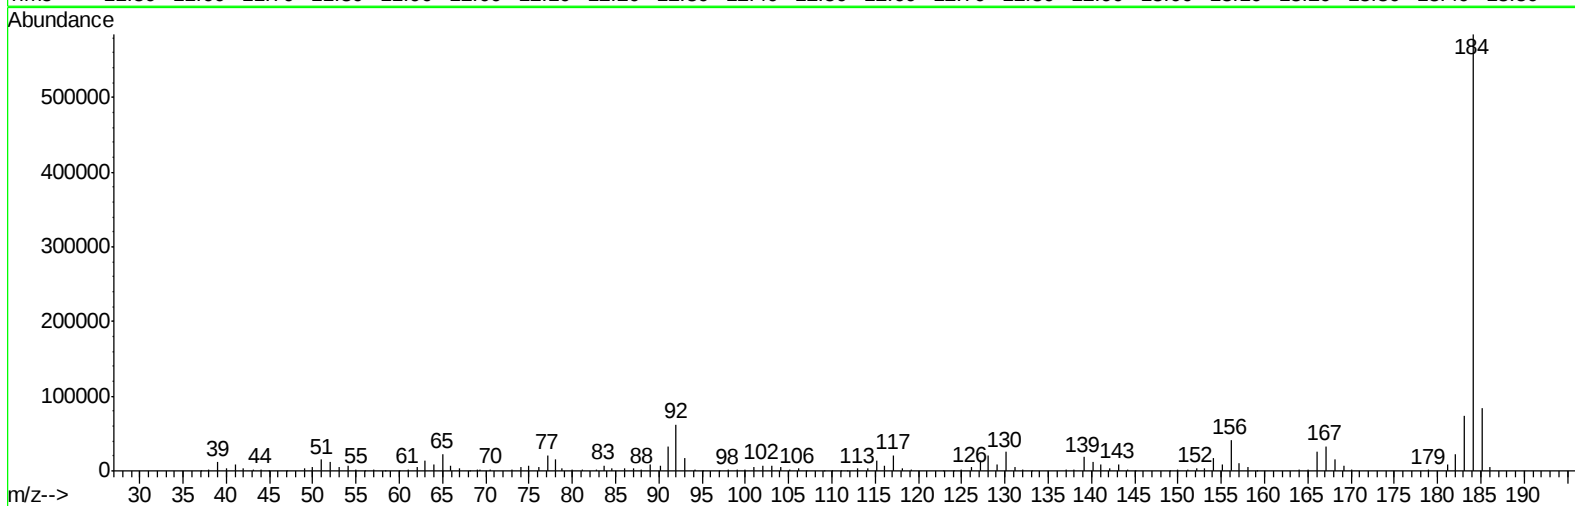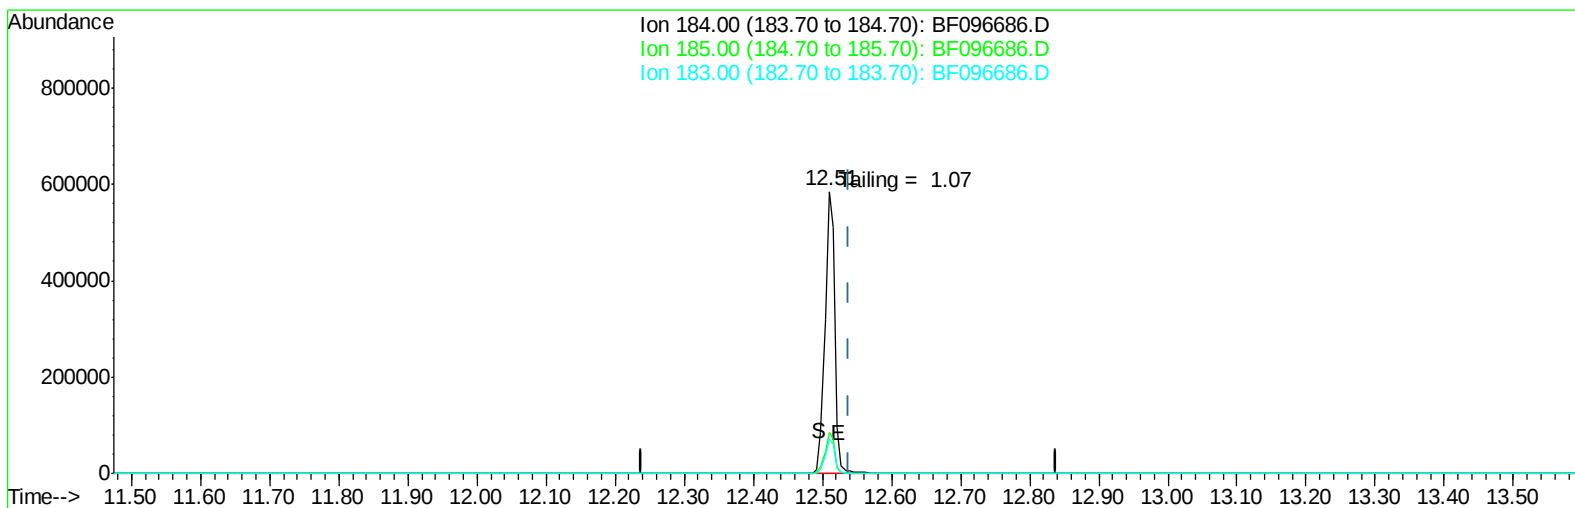

TIC: BF096686.D

(76) Benzidine

12.510min (-0.029) 0.00ng m

response 580082

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	14.47#
183.00	12.20	12.51
0.00	0.00	0.00