
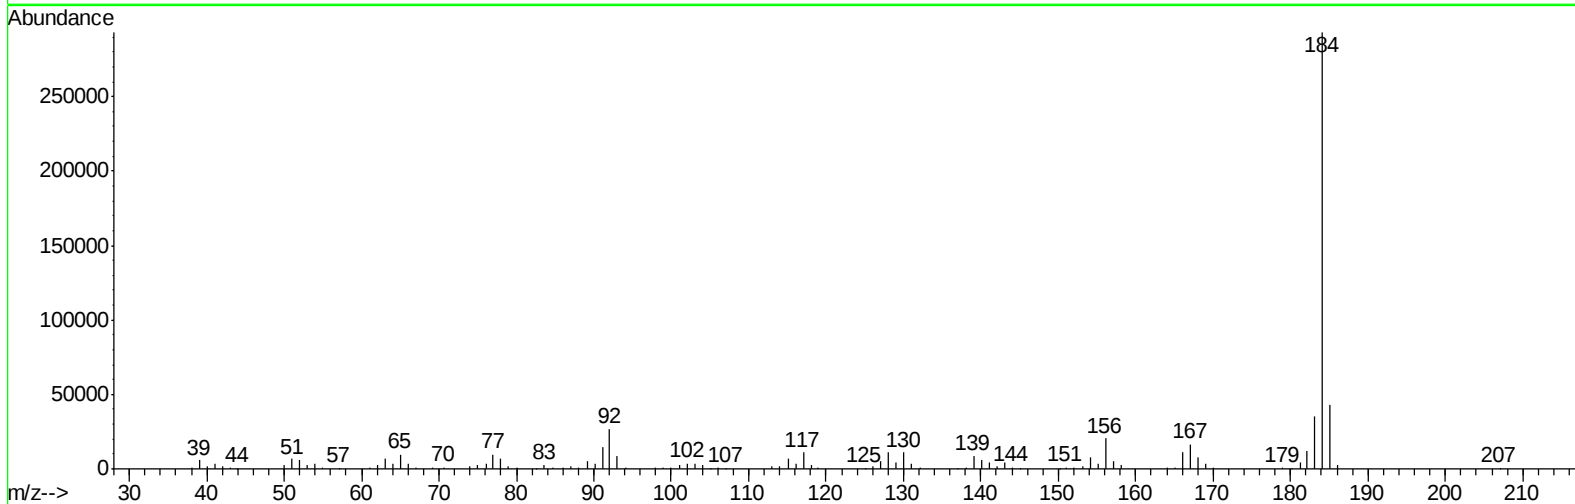


Data Path : Z:\HPCHEM1\BNA F\DATA\BF071217\
Data File : BF096713.D
Acq On : 13 Jul 2017 2:09
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 13 06:12:42 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF070117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 07 13:02:33 2017
Response via : Initial Calibration

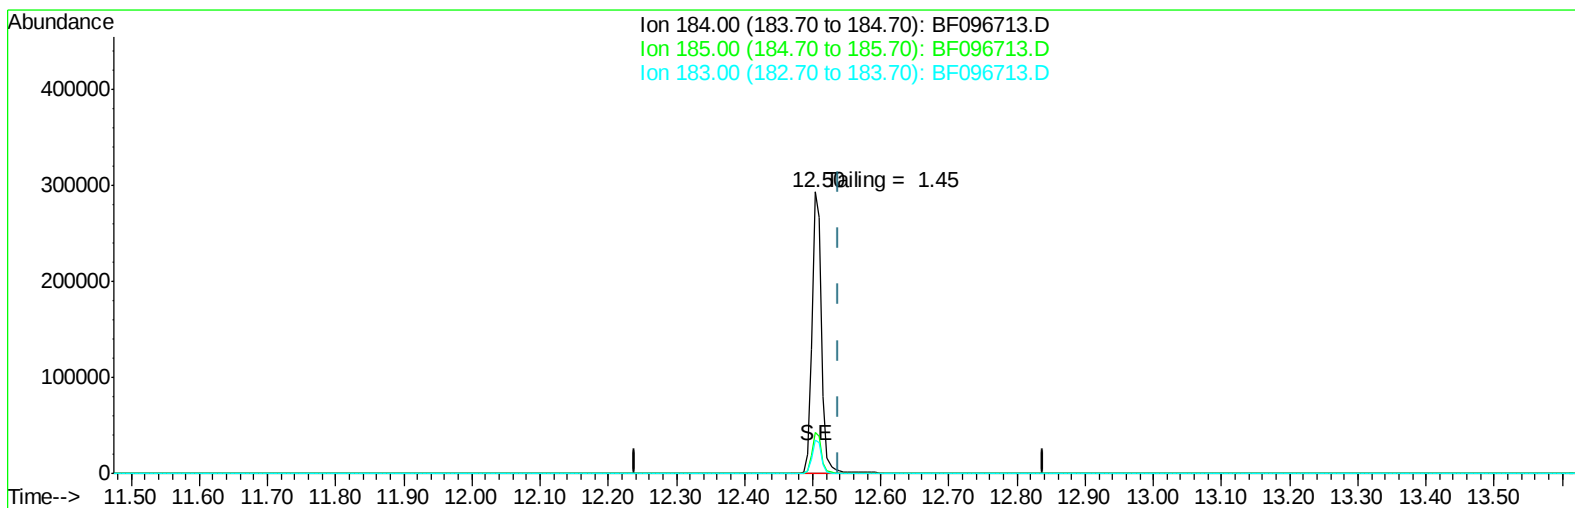

TIC: BF096713.D

(76) Benzidine



12.504min (-0.035) 0.00ng

response 294053

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	14.68#
183.00	12.20	11.95
0.00	0.00	0.00

```
Data Path : Z:\HPCHEM1\BNA F\DATA\BF071217\  
Data File : BF096713.D  
Acq On    : 13 Jul 2017    2:09  
Operator  : SJ/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Jul 13 06:11:43 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF070117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 07 13:02:33 2017
Response via : Initial Calibration

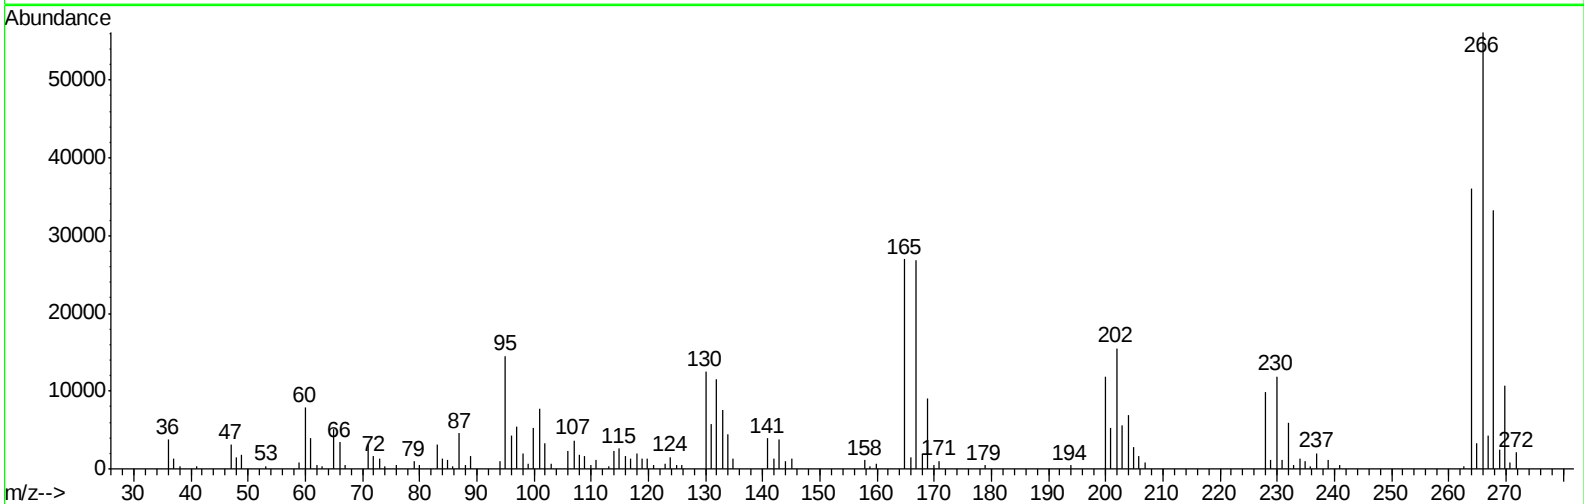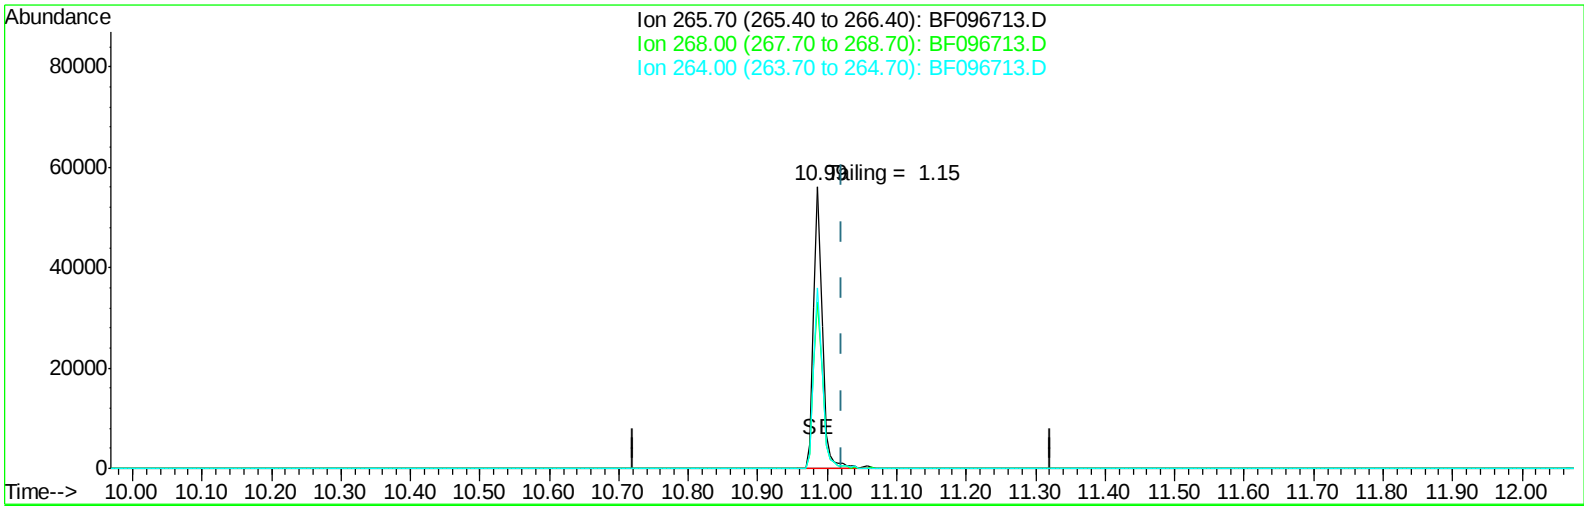

TIC: BF096713.D

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	59.20
264.00	64.60	64.11
0.00	0.00	0.00