

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF071217\
 Data File : BF096703.D
 Acq On : 12 Jul 2017 20:35
 Operator : SJ/JU
 Sample : I4140-02
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 EP-05

Quant Time: Jul 13 02:30:12 2017
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF070117.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 07 13:02:33 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.66	152	101843	20.00	ng	-0.04
21) Naphthalene-d8	7.95	136	422742	20.00	ng	-0.04
38) Acenaphthene-d10	9.70	164	173760	20.00	ng	-0.04
63) Phenanthrene-d10	11.17	188	246394	20.00	ng	-0.04
75) Chrysene-d12	13.80	240	179263	20.00	ng	-0.04
86) Perylene-d12	15.20	264	169542	20.00	ng	-0.05
System Monitoring Compounds						
5) 2-Fluorophenol	5.28	112	692662	100.38	ng	-0.03
7) Phenol-d6	6.31	99	848943	100.08	ng	-0.04
23) Nitrobenzene-d5	7.23	82	491160	69.82	ng	-0.04
41) 2,4,6-Tribromophenol	10.49	330	141948	104.58	ng	-0.04
44) 2-Fluorobiphenyl	9.03	172	907006	89.25	ng	-0.04
78) Terphenyl-d14	12.76	244	479146	57.11	ng	-0.04
Target Compounds						
49) Dimethylphthalate	9.42	163	123981	9.558	ng	Qvalue # 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF071217\
Data File : BF096703.D
Acq On : 12 Jul 2017 20:35
Operator : SJ/JU
Sample : I4140-02
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
EP-05

Quant Time: Jul 13 02:30:12 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF070117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 07 13:02:33 2017
Response via : Initial Calibration

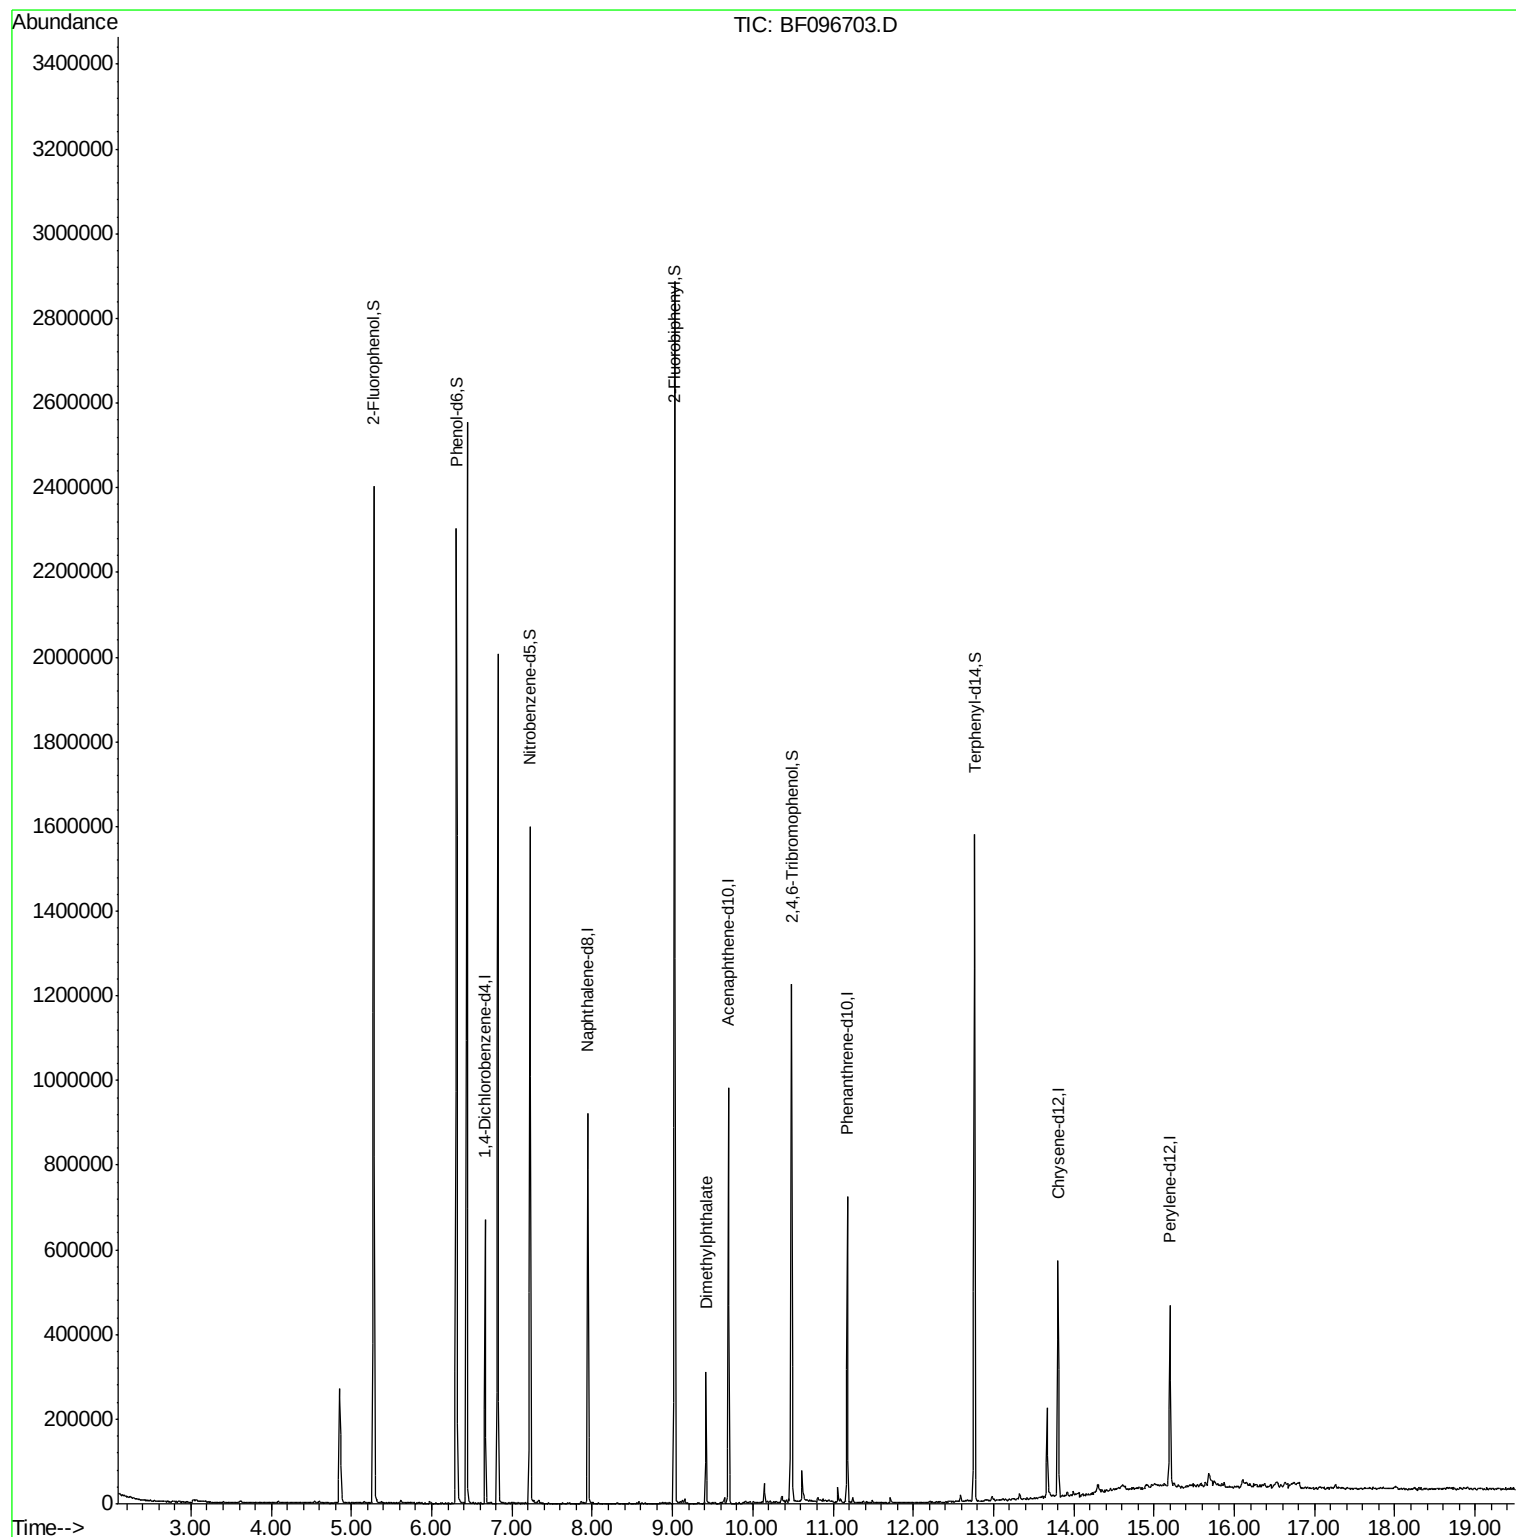

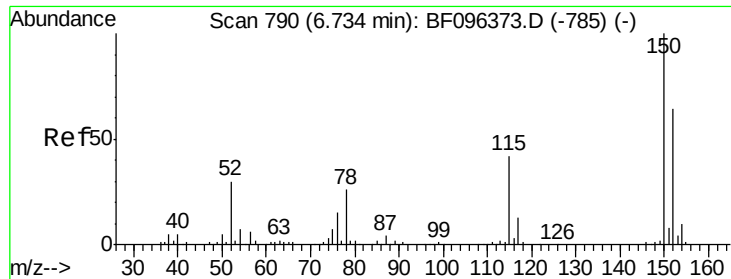


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.66 min Scan# 778
Delta R.T. -0.04 min
Lab File: BF096703.D
Acq: 12 Jul 2017 20:35

Instrument :
BNA_F
ClientSampleId :
EP-05

Tgt Ion:152 Resp: 101843
Ion Ratio Lower Upper
152 100
150 154.6 126.2 189.2
115 67.4 52.2 78.2

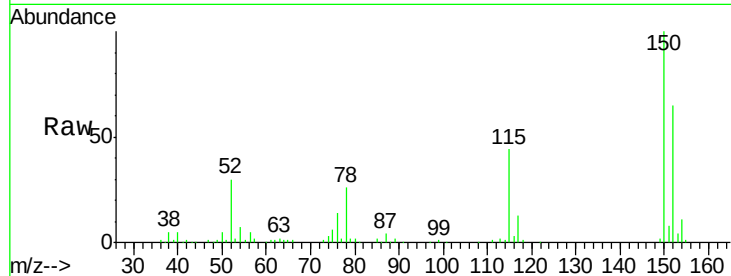


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

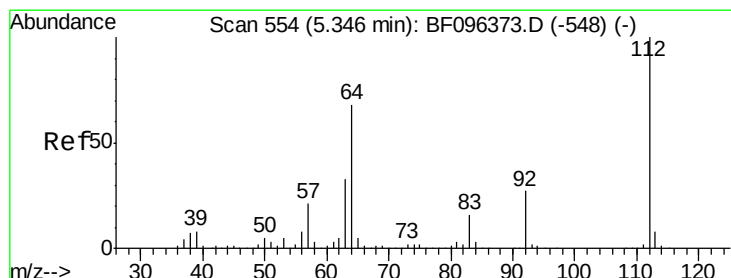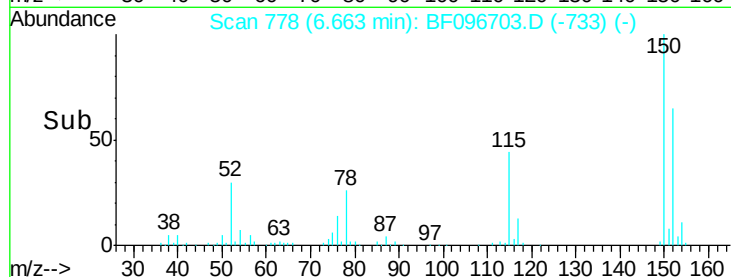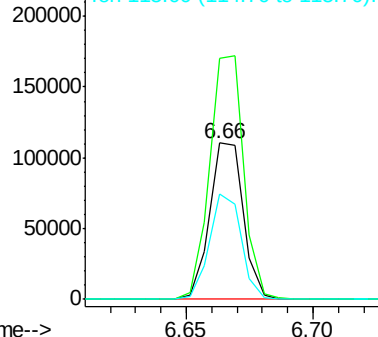



#5


2-Fluorophenol
Concen: 100.385 ng
RT: 5.28 min Scan# 543
Delta R.T. -0.03 min
Lab File: BF096703.D
Acq: 12 Jul 2017 20:35

Tgt Ion:112 Resp: 692662
Ion Ratio Lower Upper
112 100
64 63.5 46.0 69.0
63 32.6 23.4 35.0

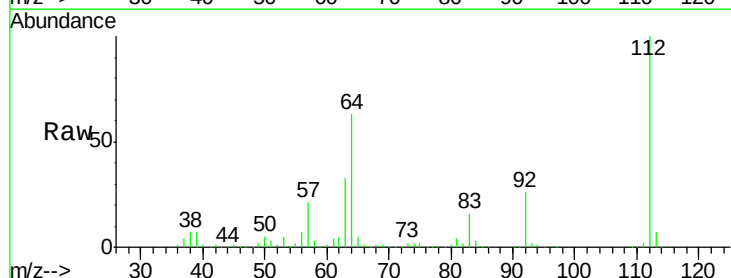

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

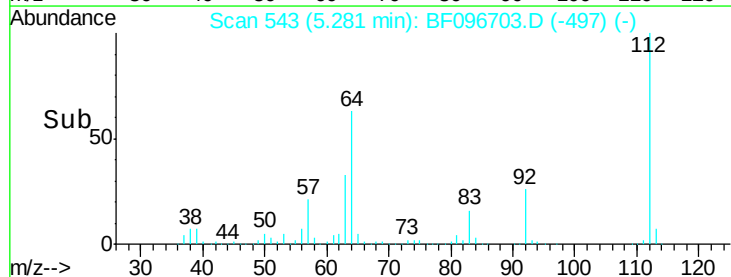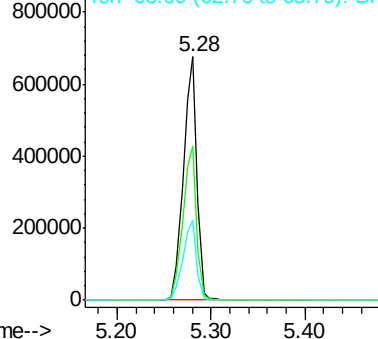

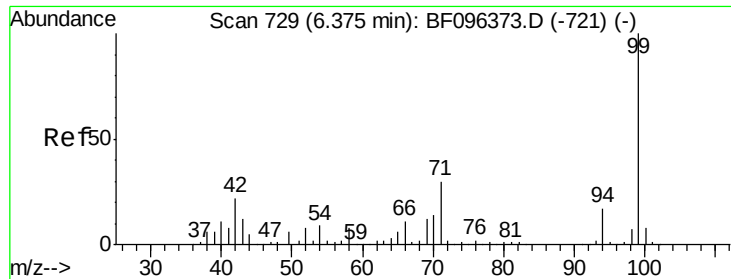

#7

Phenol-d6

Concen: 100.079 ng

RT: 6.31 min Scan# 718

Delta R.T. -0.04 min

Lab File: BF096703.D

Acq: 12 Jul 2017 20:35

Instrument :

BNA_F

ClientSampled :

EP-05


Tgt Ion: 99 Resp: 848943

Ion Ratio Lower Upper

99 100

42 22.9 13.5 20.3#




71 32.3 24.5 36.7

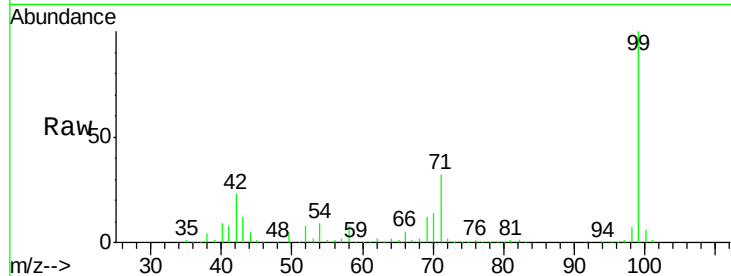

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

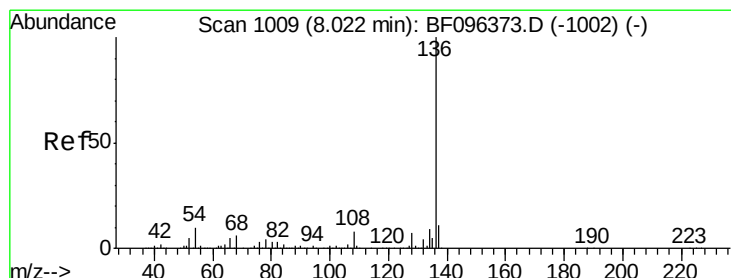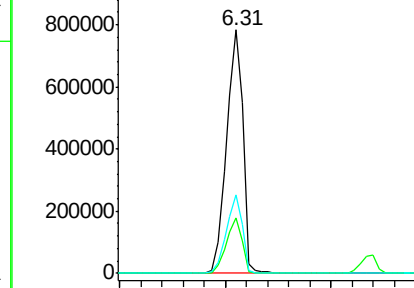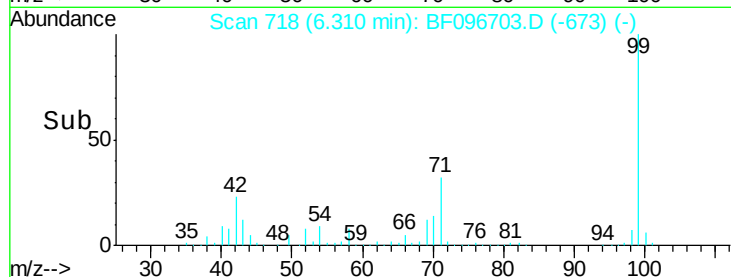

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 7.95 min Scan# 996

Delta R.T. -0.04 min

Lab File: BF096703.D

Acq: 12 Jul 2017 20:35

Tgt Ion: 136 Resp: 422742


Ion Ratio Lower Upper

136 100

137 11.2 8.5 12.7

54 10.5 4.9 7.3#

68 5.1 4.1 6.1


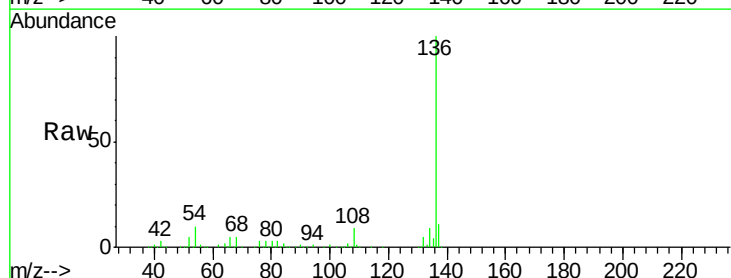



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0



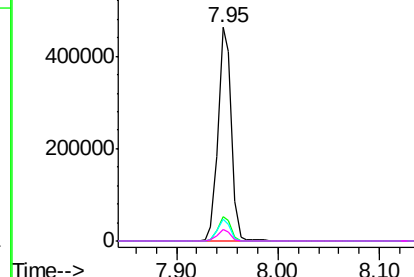
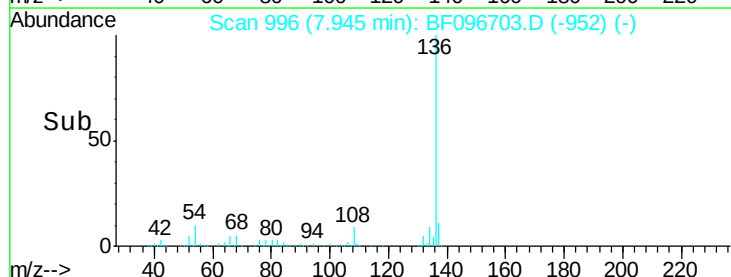


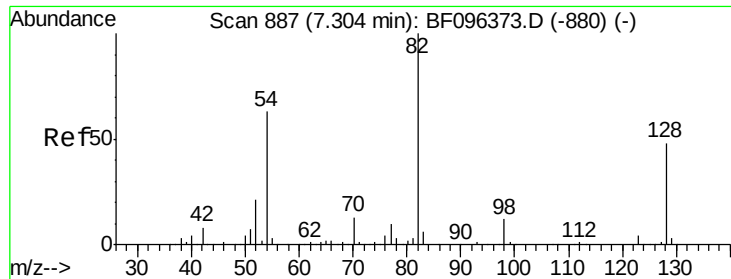

#23
 Nitrobenzene-d5
 Concen: 69.816 ng
 RT: 7.23 min Scan# 874
 Delta R.T. -0.04 min
 Lab File: BF096703.D
 Acq: 12 Jul 2017 20:35




Instrument :
 BNA_F
 ClientSampleId :
 EP-05


Tgt Ion: 82 Resp: 491160
 Ion Ratio Lower Upper
 82 100
 128 47.6 34.0 51.0
 54 67.6 42.2 63.2#

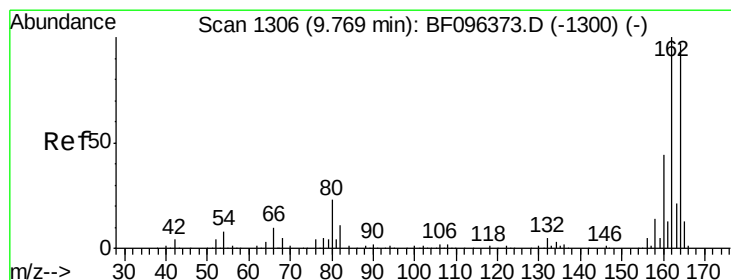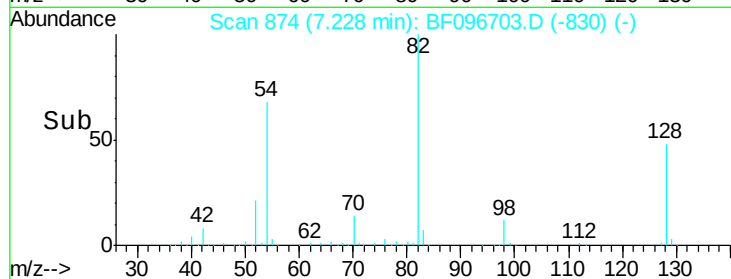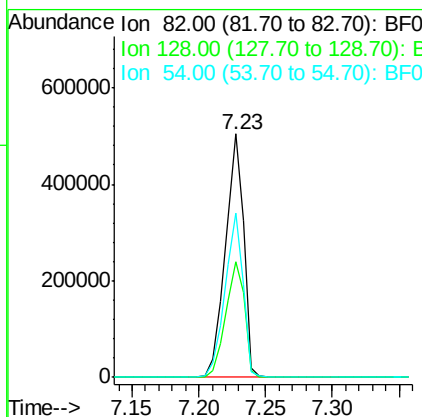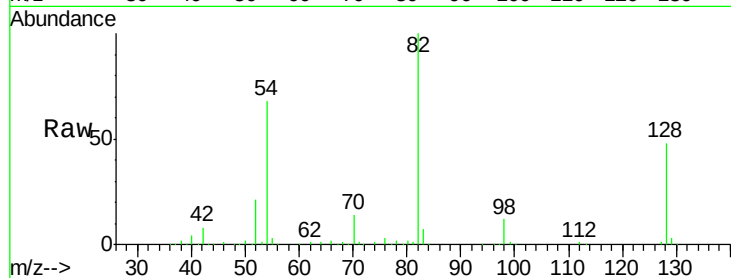

#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.70 min Scan# 1294
 Delta R.T. -0.04 min
 Lab File: BF096703.D
 Acq: 12 Jul 2017 20:35

Tgt Ion: 164 Resp: 173760
 Ion Ratio Lower Upper
 164 100
 162 103.8 82.6 123.8
 160 45.6 36.2 54.2

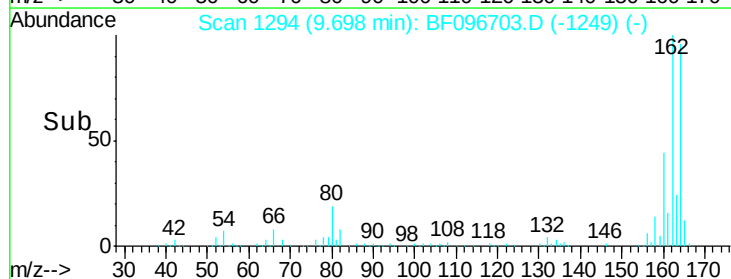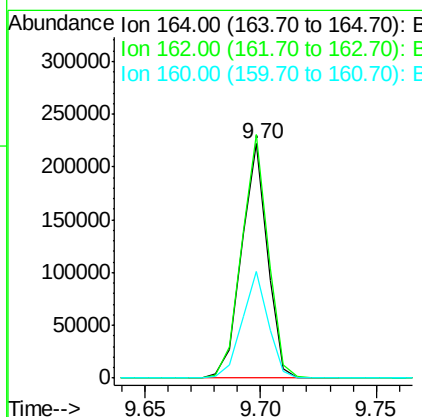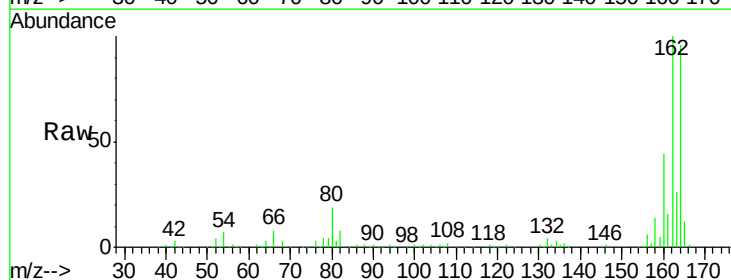


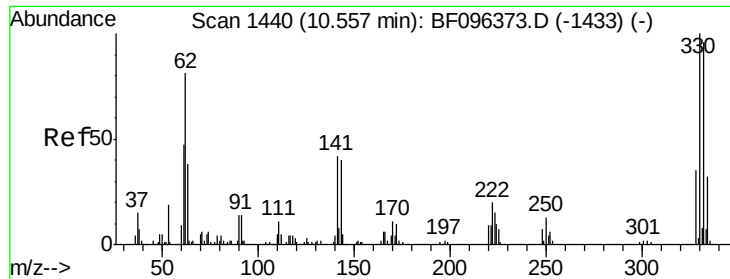




#41
 2,4,6-Tribromophenol
 Concen: 104.583 ng
 RT: 10.49 min Scan# 1428
 Delta R.T. -0.04 min
 Lab File: BF096703.D
 Acq: 12 Jul 2017 20:35

Instrument :
 BNA_F
 ClientSampleId :
 EP-05

Tgt Ion	Ratio	Lower	Upper
330	100		
332	97.5	76.6	115.0
141	37.6	31.4	47.2

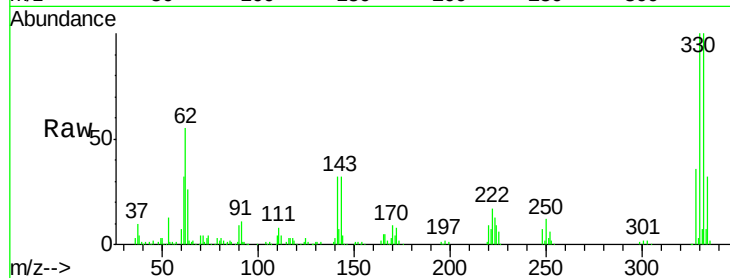


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

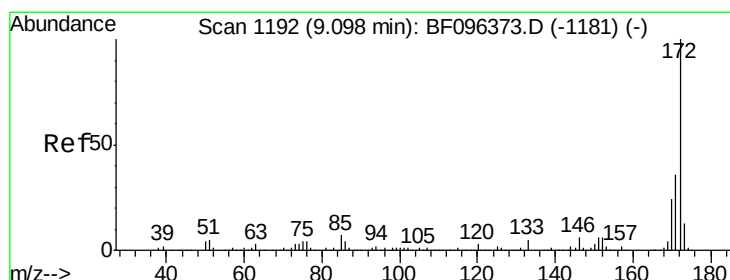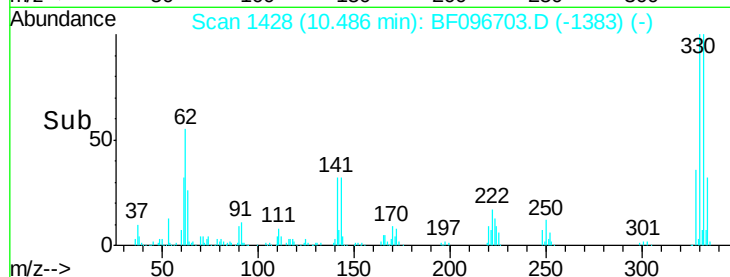
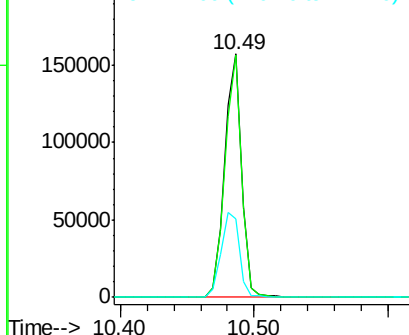



#44
 2-Fluorobiphenyl
 Concen: 89.248 ng
 RT: 9.03 min Scan# 1180
 Delta R.T. -0.04 min
 Lab File: BF096703.D
 Acq: 12 Jul 2017 20:35

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.9	29.6	44.4
170	24.6	19.8	29.8

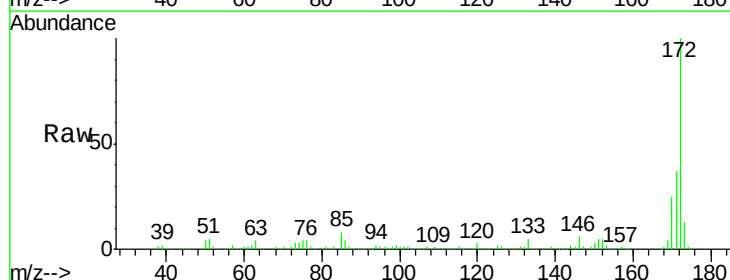

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

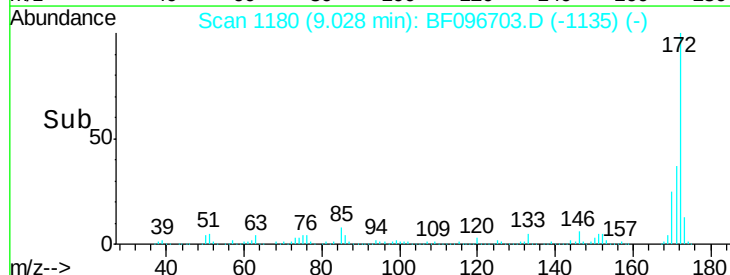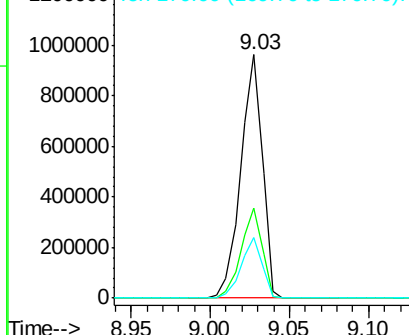

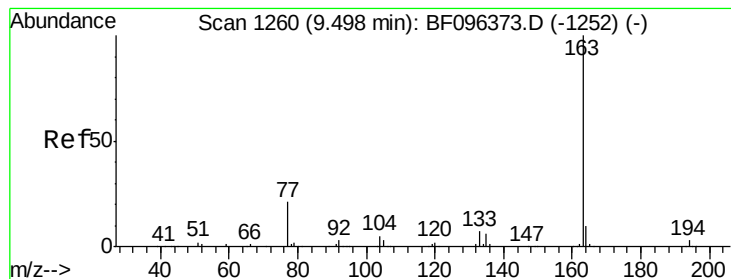

#49

Dimethylphthalate

Concen: 9.558 ng

RT: 9.42 min Scan# 1246

Delta R.T. -0.05 min

Lab File: BF096703.D

Acq: 12 Jul 2017 20:35

Instrument :

BNA_F

ClientSampleId :

EP-05


Tgt Ion:163 Resp: 123981

Ion Ratio Lower Upper

163 100

194 2.6 2.6 4.0#




164 10.1 8.4 12.6

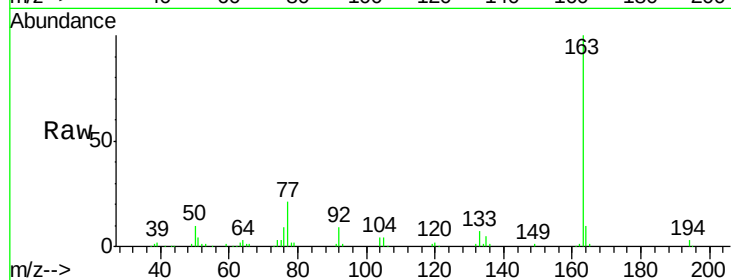

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

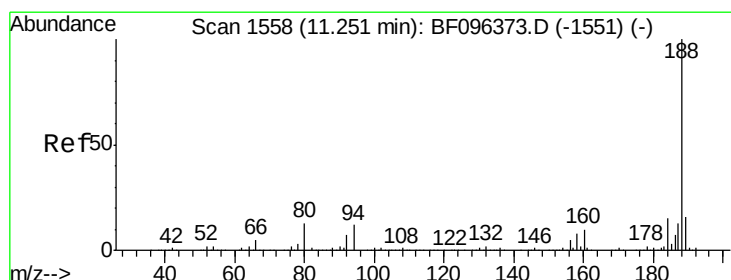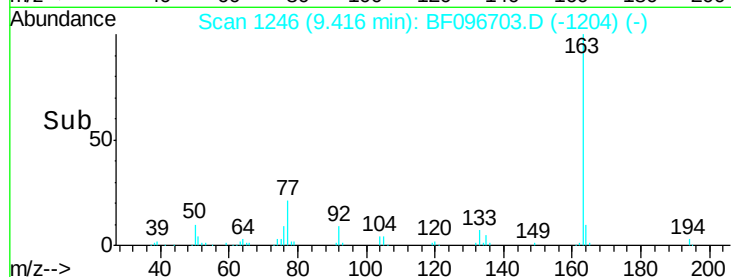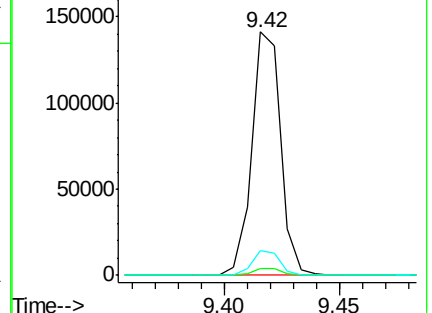

#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.17 min Scan# 1545

Delta R.T. -0.04 min

Lab File: BF096703.D

Acq: 12 Jul 2017 20:35


Tgt Ion:188 Resp: 246394

Ion Ratio Lower Upper

188 100

94 11.7 9.4 14.2



80 12.3 10.2 15.2

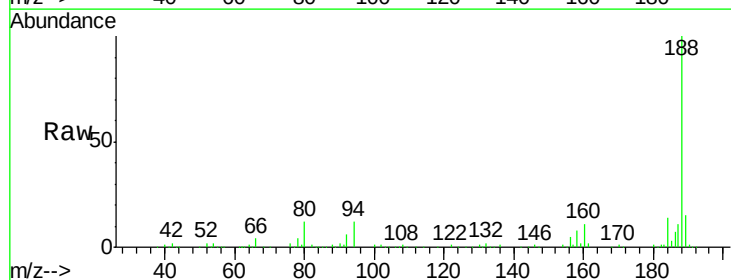


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

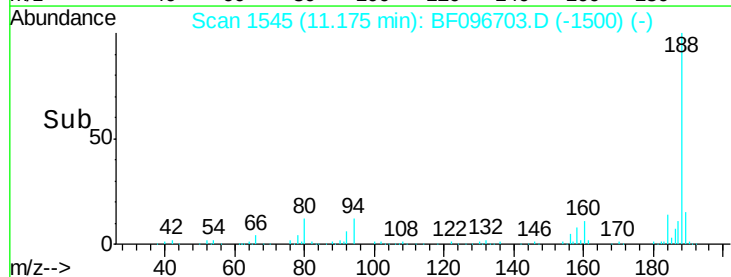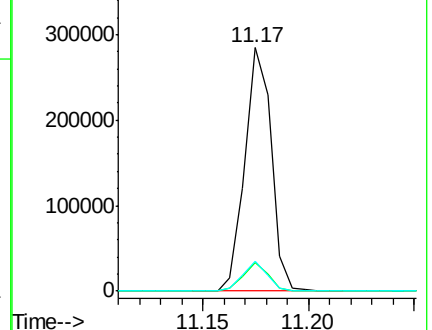

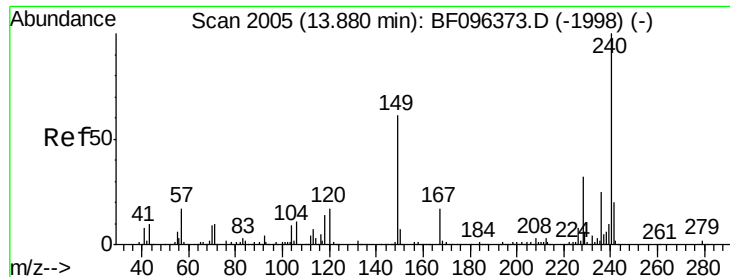

#75

Chrysene-d12

Concen: 20.000 ng

RT: 13.80 min Scan# 1992

Delta R.T. -0.04 min

Lab File: BF096703.D

Acq: 12 Jul 2017 20:35

Instrument :

BNA_F

ClientSampleId :

EP-05


Tgt Ion:240 Resp: 179263

Ion Ratio Lower Upper

240 100

120 13.7 5.8 8.8#




236 24.8 20.5 30.7

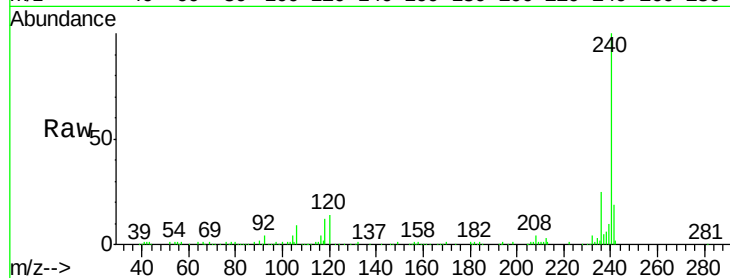

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

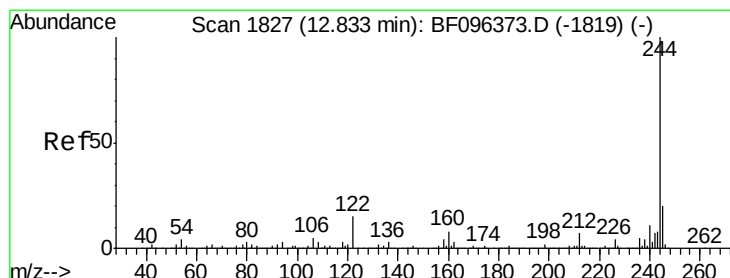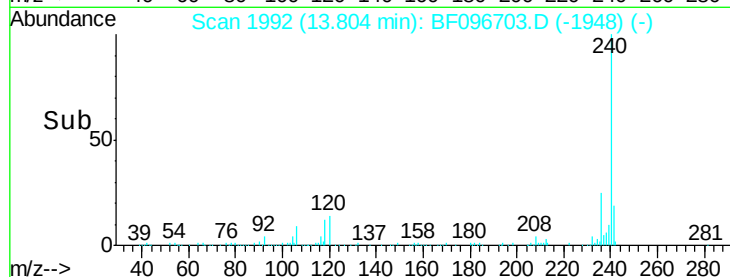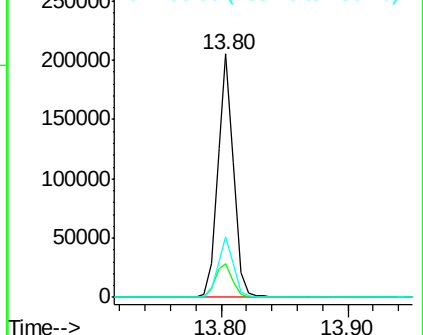

#78

Terphenyl-d14

Concen: 57.115 ng

RT: 12.76 min Scan# 1815

Delta R.T. -0.04 min

Lab File: BF096703.D

Acq: 12 Jul 2017 20:35


Tgt Ion:244 Resp: 479146

Ion Ratio Lower Upper

244 100

212 7.0 6.0 9.0



122 14.2 10.3 15.5

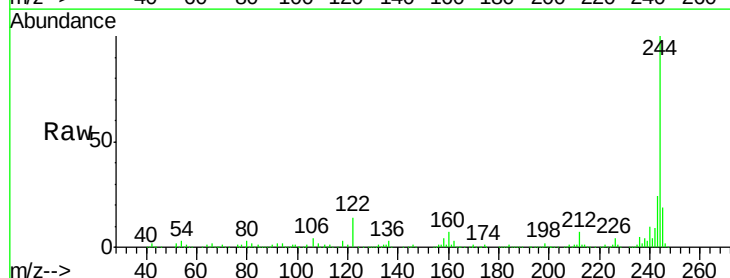


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

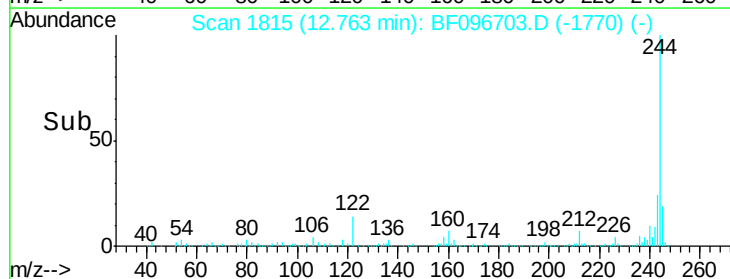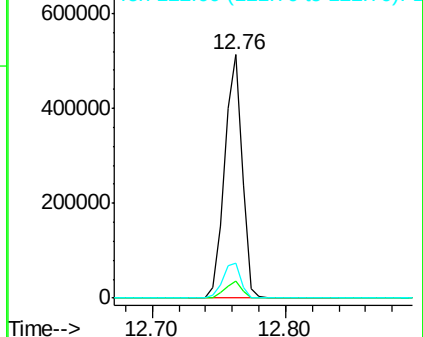


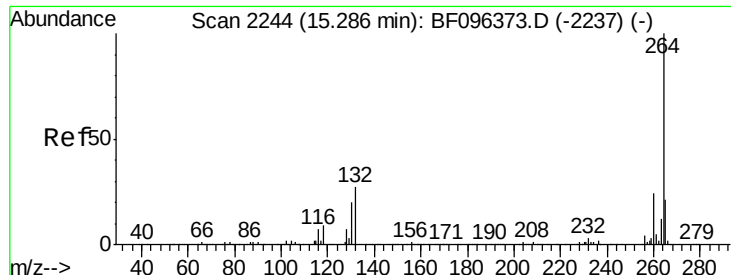

#86
Perylene-d12
Concen: 20.000 ng
RT: 15.20 min Scan# 2229
Delta R.T. -0.05 min
Lab File: BF096703.D
Acq: 12 Jul 2017 20:35

Instrument :
BNA_F
ClientSampleId :
EP-05

Tgt Ion	Ratio	Lower	Upper
264	100		
260	23.4	19.5	29.3
265	21.2	17.2	25.8

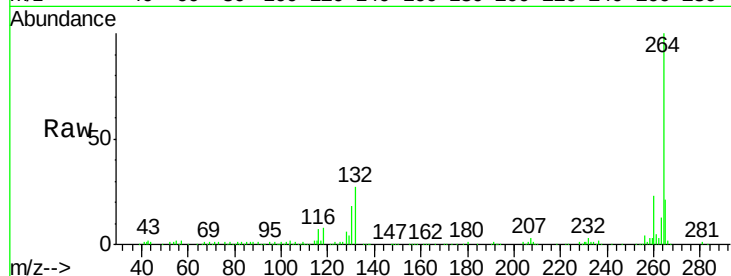

Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

