

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF071217\
 Data File : BF096705.D
 Acq On : 12 Jul 2017 21:31
 Operator : SJ/JU
 Sample : I4140-04
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 EP-15

Quant Time: Jul 13 08:20:51 2017
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF070117.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 07 13:02:33 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.66	152	109489	20.00	ng	-0.04
21) Naphthalene-d8	7.95	136	454576	20.00	ng	-0.04
38) Acenaphthene-d10	9.70	164	189012	20.00	ng	-0.04
63) Phenanthrene-d10	11.17	188	276529	20.00	ng	-0.04
75) Chrysene-d12	13.80	240	220668	20.00	ng	-0.04
86) Perylene-d12	15.20	264	181408	20.00	ng	-0.05
System Monitoring Compounds						
5) 2-Fluorophenol	5.28	112	617362	83.22	ng	-0.03
7) Phenol-d6	6.31	99	749709	82.21	ng	-0.04
23) Nitrobenzene-d5	7.23	82	456291	60.32	ng	-0.04
41) 2,4,6-Tribromophenol	10.49	330	123313	83.52	ng	-0.04
44) 2-Fluorobiphenyl	9.03	172	720643	65.19	ng	-0.04
78) Terphenyl-d14	12.76	244	390929	37.86	ng	-0.04
Target Compounds						
49) Dimethylphthalate	9.42	163	139779	9.906	ng	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF071217\
Data File : BF096705.D
Acq On : 12 Jul 2017 21:31
Operator : SJ/JU
Sample : I4140-04
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
EP-15

Quant Time: Jul 13 08:20:51 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF070117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 07 13:02:33 2017
Response via : Initial Calibration

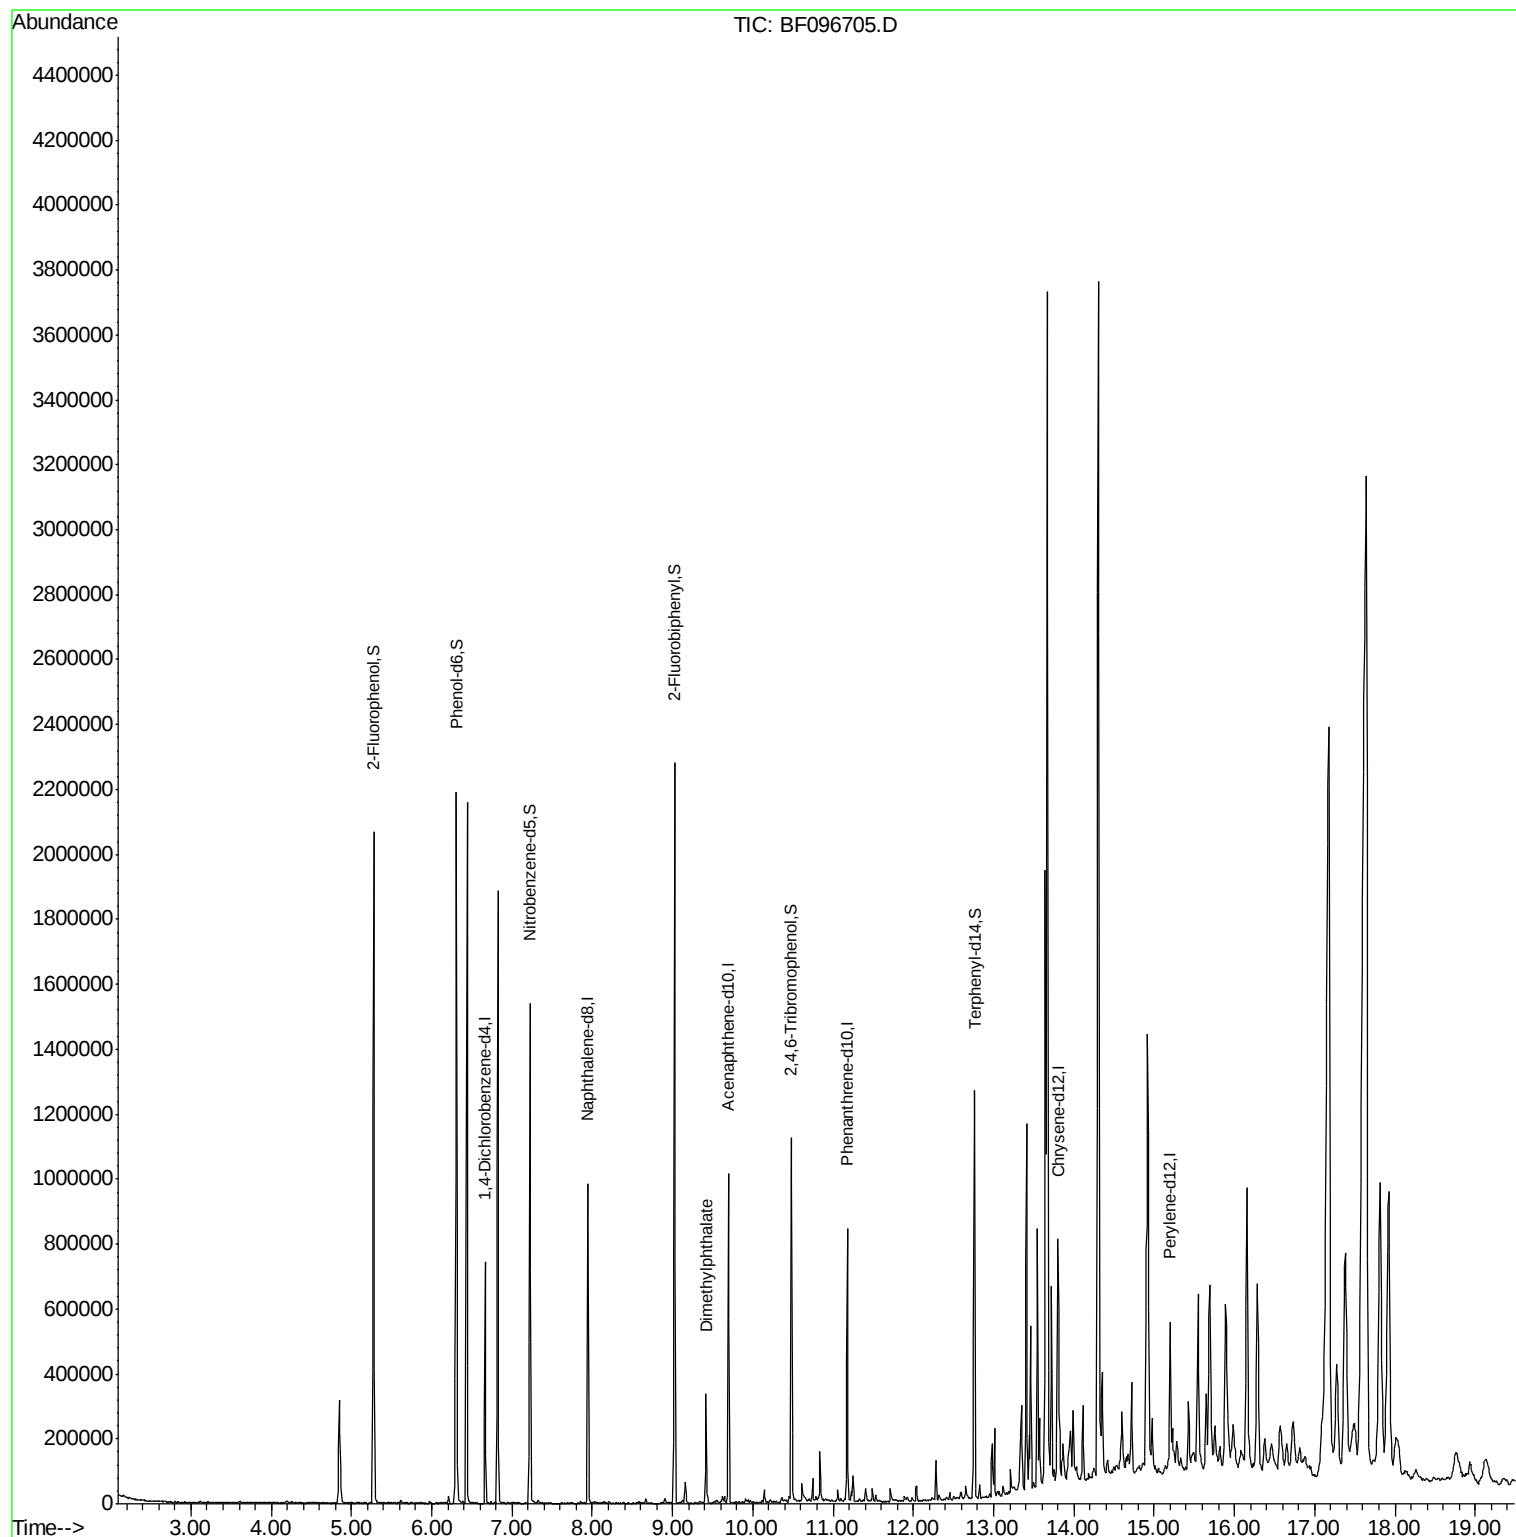

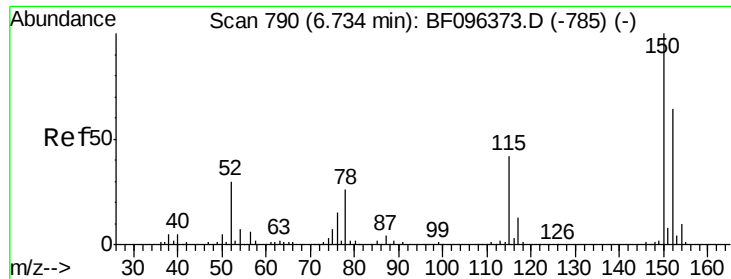


#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.66 min Scan# 778
Delta R.T. -0.04 min
Lab File: BF096705.D
Acq: 12 Jul 2017 21:31

Instrument :
BNA_F
ClientSampleId :
EP-15

Tgt Ion:152 Resp: 109489
Ion Ratio Lower Upper
152 100
150 160.3 126.2 189.2
115 65.9 52.2 78.2

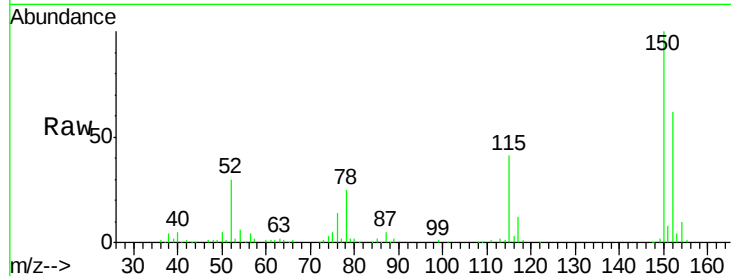


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

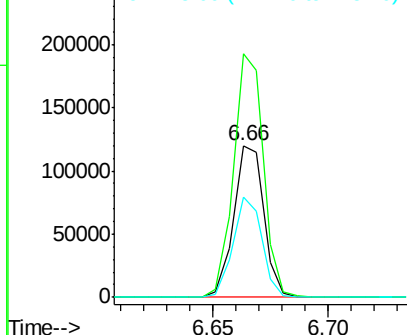



#5

2-Fluorophenol
Concen: 83.224 ng
RT: 5.28 min Scan# 543
Delta R.T. -0.03 min
Lab File: BF096705.D
Acq: 12 Jul 2017 21:31

Tgt Ion:112 Resp: 617362
Ion Ratio Lower Upper
112 100
64 62.4 46.0 69.0
63 31.5 23.4 35.0

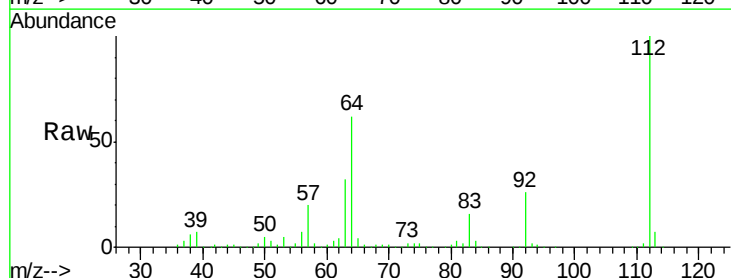

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

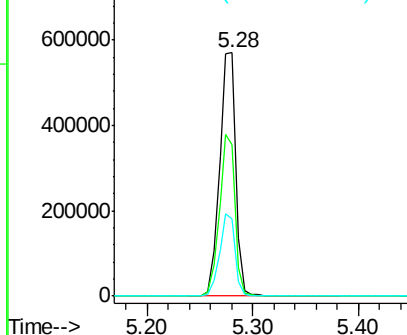



#7

Phenol-d6

Concen: 82.209 ng

RT: 6.31 min Scan# 718

Delta R.T. -0.04 min

Lab File: BF096705.D

Acq: 12 Jul 2017 21:31

Instrument :

BNA_F

ClientSampleId :

EP-15


Tgt Ion: 99 Resp: 749709

Ion Ratio Lower Upper

99 100

42 22.3 13.5 20.3#




71 32.1 24.5 36.7

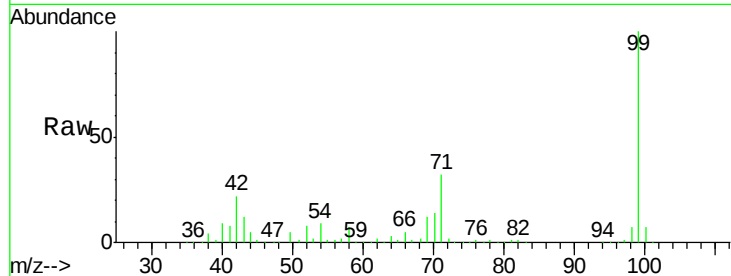

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

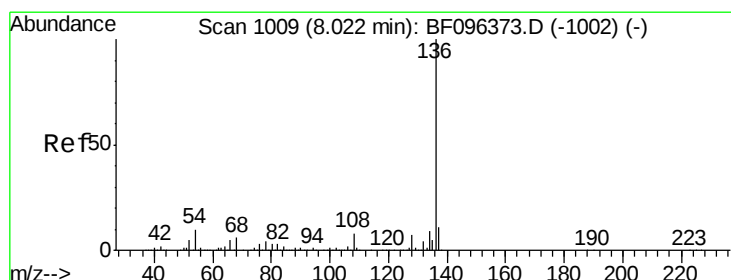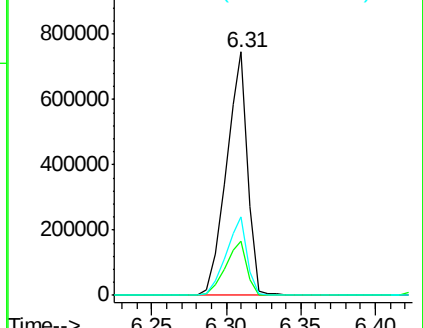

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 7.95 min Scan# 996

Delta R.T. -0.04 min

Lab File: BF096705.D

Acq: 12 Jul 2017 21:31

Tgt Ion: 136 Resp: 454576


Ion Ratio Lower Upper

136 100

137 11.1 8.5 12.7

54 10.6 4.9 7.3#

68 5.1 4.1 6.1


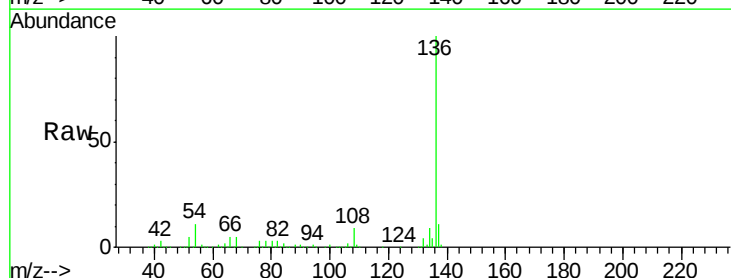



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

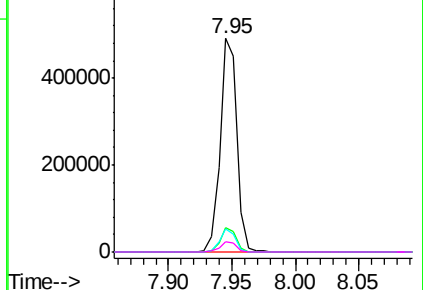



#23

Nitrobenzene-d5

Concen: 60.318 ng

RT: 7.23 min Scan# 874

Delta R.T. -0.04 min

Lab File: BF096705.D

Acq: 12 Jul 2017 21:31

Instrument :

BNA_F

ClientSampleId :

EP-15


Tgt Ion: 82 Resp: 456291

Ion Ratio Lower Upper

82 100

128 47.7 34.0 51.0




54 65.7 42.2 63.2#

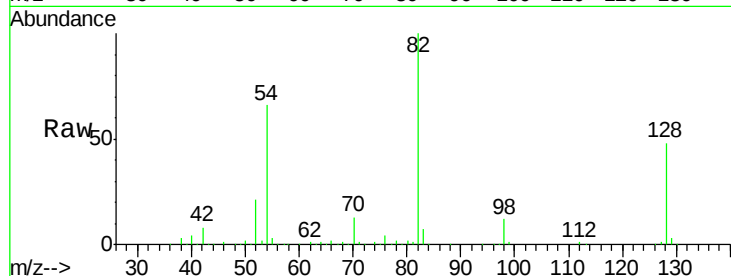

Abundance Ion 82.00 (81.70 to 82.70): BF0

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF0

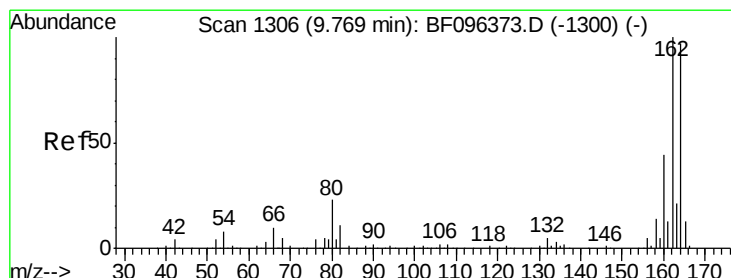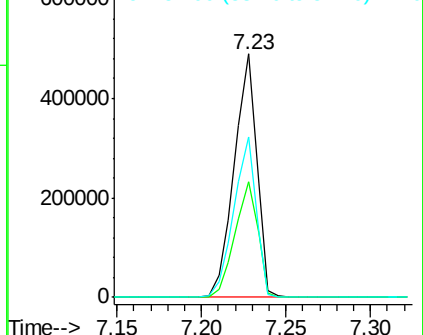

#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.70 min Scan# 1294

Delta R.T. -0.04 min

Lab File: BF096705.D

Acq: 12 Jul 2017 21:31


Tgt Ion: 164 Resp: 189012

Ion Ratio Lower Upper

164 100

162 105.3 82.6 123.8



160 44.9 36.2 54.2

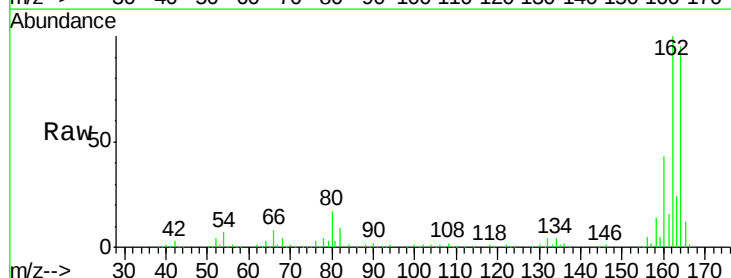


Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

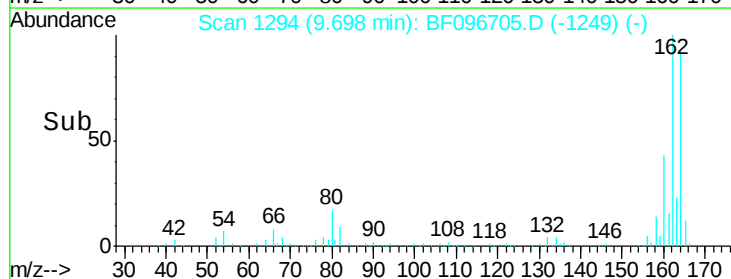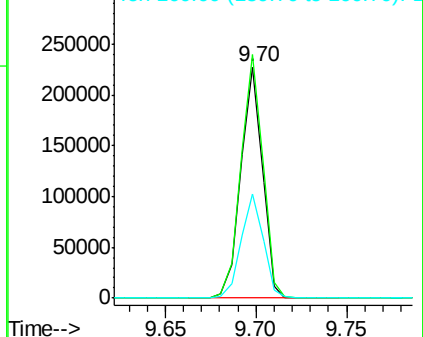


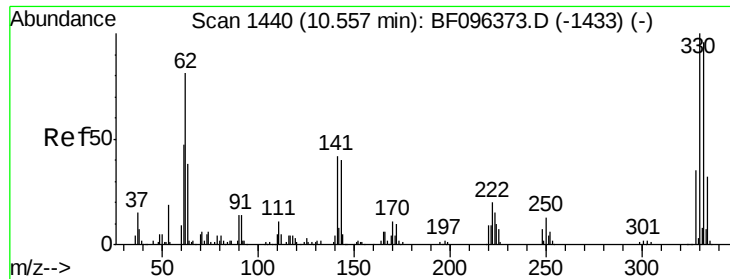




#41
 2,4,6-Tribromophenol
 Concen: 83.522 ng
 RT: 10.49 min Scan# 1428
 Delta R.T. -0.04 min
 Lab File: BF096705.D
 Acq: 12 Jul 2017 21:31

Instrument :
 BNA_F
 ClientSampleId :
 EP-15

Tgt Ion	Ratio	Lower	Upper
330	100		
332	97.5	76.6	115.0
141	39.4	31.4	47.2

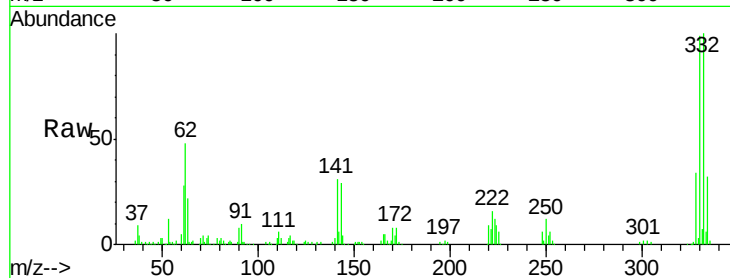


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

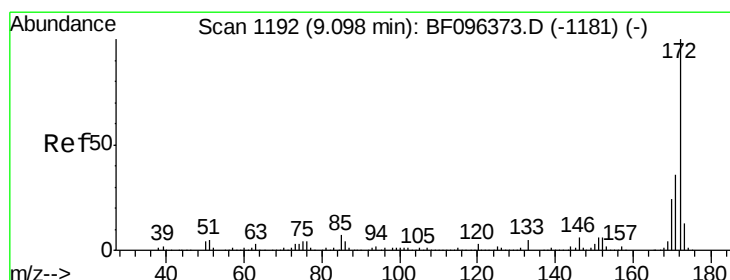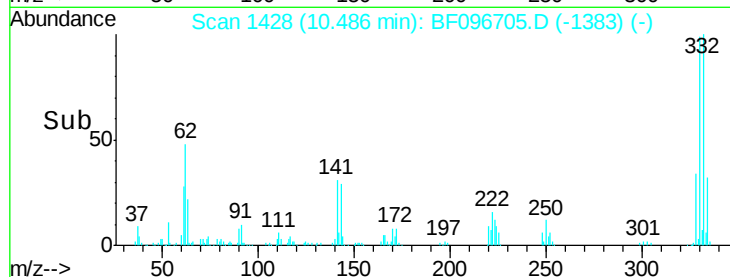
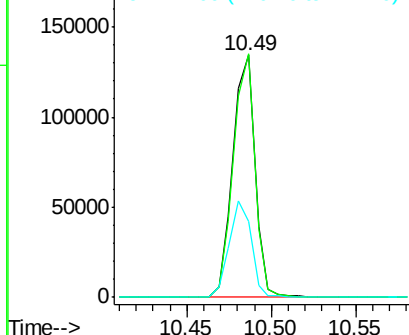



#44
 2-Fluorobiphenyl
 Concen: 65.188 ng
 RT: 9.03 min Scan# 1180
 Delta R.T. -0.04 min
 Lab File: BF096705.D
 Acq: 12 Jul 2017 21:31

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.2	29.6	44.4
170	23.7	19.8	29.8

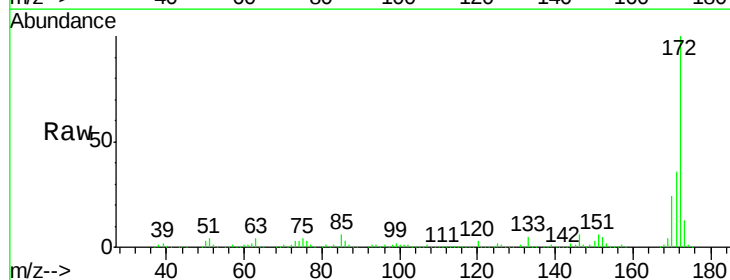

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



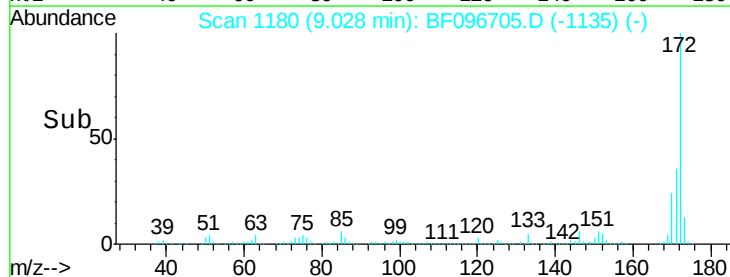
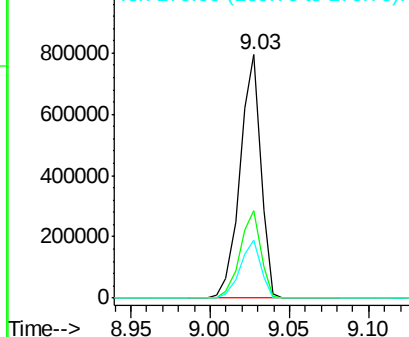




#49
Dimethylphthalate
Concen: 9.906 ng
RT: 9.42 min Scan# 1247
Delta R.T. -0.05 min
Lab File: BF096705.D
Acq: 12 Jul 2017 21:31




Instrument :
BNA_F
ClientSampleId :
EP-15


Tgt Ion:163 Resp: 139779
Ion Ratio Lower Upper
163 100
194 3.3 2.6 4.0
164 10.0 8.4 12.6

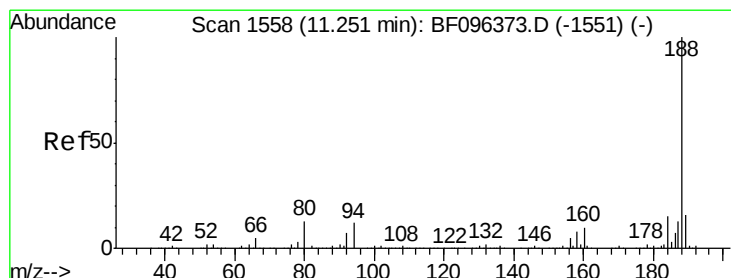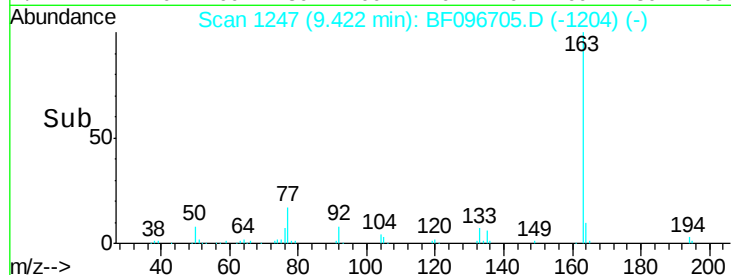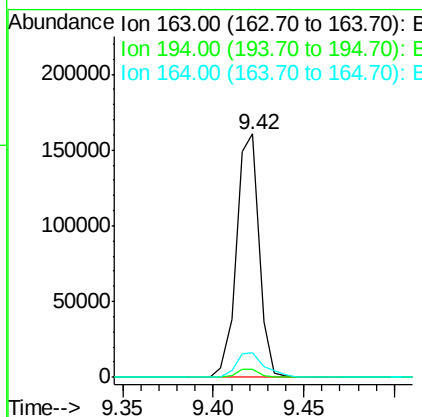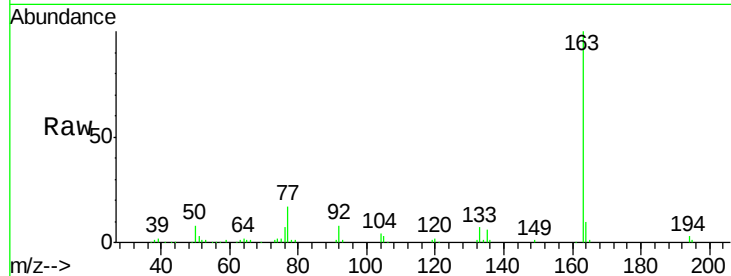

#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.17 min Scan# 1545
Delta R.T. -0.04 min
Lab File: BF096705.D
Acq: 12 Jul 2017 21:31

Tgt Ion:188 Resp: 276529
Ion Ratio Lower Upper
188 100
94 11.4 9.4 14.2
80 10.9 10.2 15.2

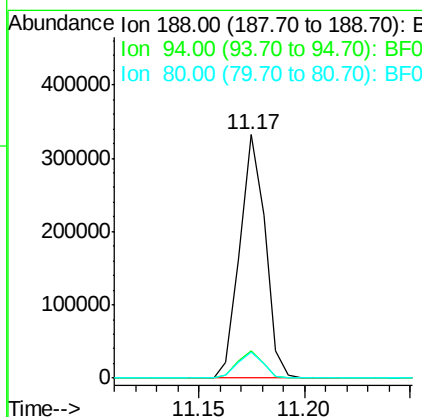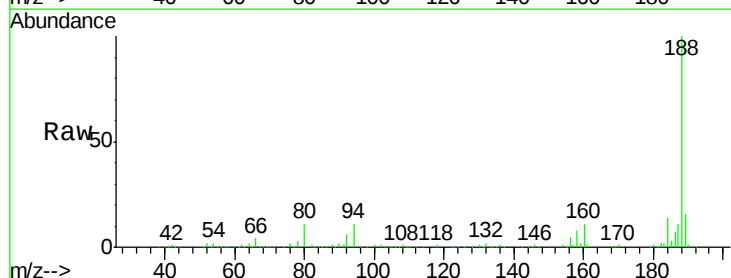

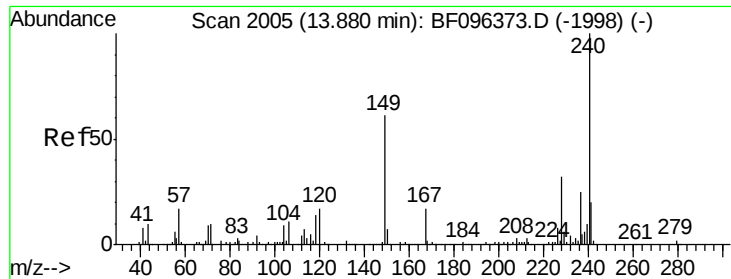

#75

Chrysene-d12

Concen: 20.000 ng

RT: 13.80 min Scan# 1992

Delta R.T. -0.04 min

Lab File: BF096705.D

Acq: 12 Jul 2017 21:31

Instrument :

BNA_F

ClientSampleId :

EP-15


Tgt Ion:240 Resp: 220668

Ion Ratio Lower Upper

240 100

120 15.3 5.8 8.8#




236 25.8 20.5 30.7

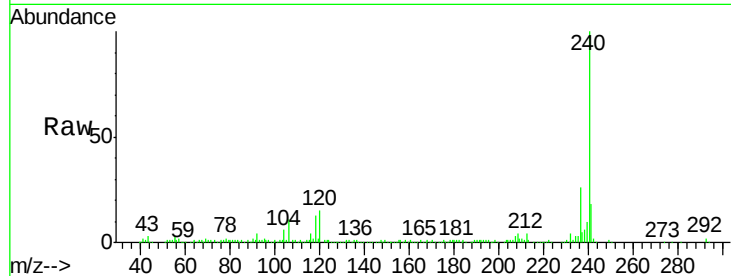

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

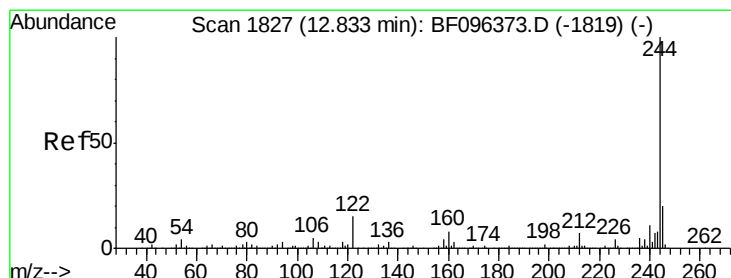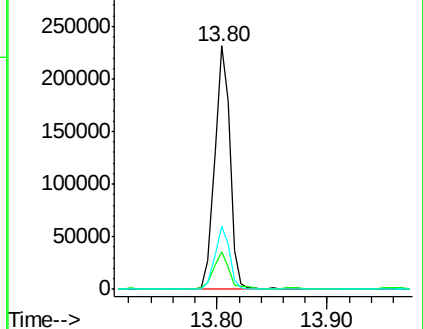

#78

Terphenyl-d14

Concen: 37.856 ng

RT: 12.76 min Scan# 1815

Delta R.T. -0.04 min

Lab File: BF096705.D

Acq: 12 Jul 2017 21:31


Tgt Ion:244 Resp: 390929

Ion Ratio Lower Upper

244 100

212 5.9 6.0 9.0#



122 12.8 10.3 15.5

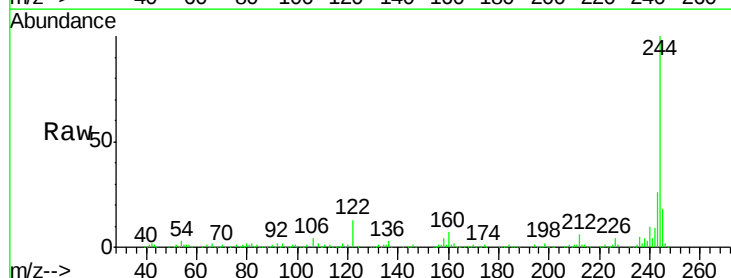


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

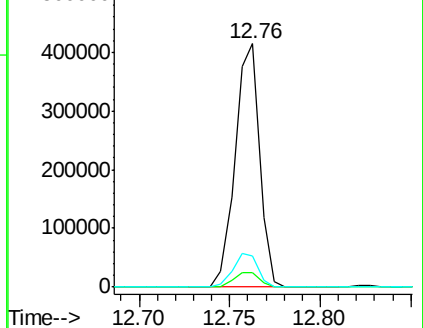


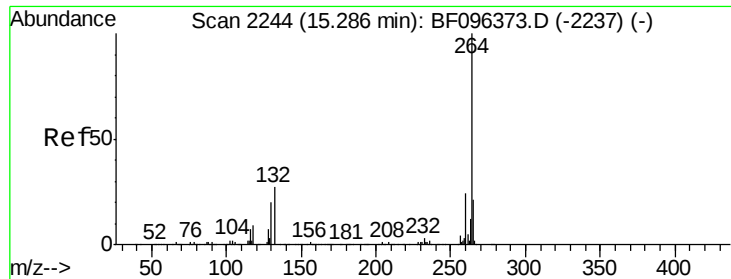

#86
Perylene-d12
Concen: 20.000 ng
RT: 15.20 min Scan# 2229
Delta R.T. -0.05 min
Lab File: BF096705.D
Acq: 12 Jul 2017 21:31

Instrument :
BNA_F
ClientSampleId :
EP-15

Tgt Ion: 264 Resp: 181408
Ion Ratio Lower Upper
264 100
260 23.5 19.5 29.3
265 20.7 17.2 25.8

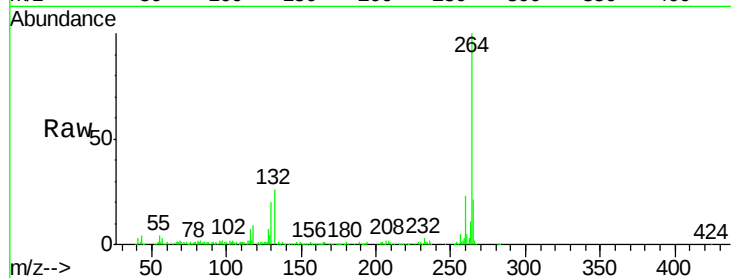

Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

