


Data Path : Z:\HPCHEM1\BNA_F\Data\BF071217\
 Data File : BF096686.D
 Acq On : 12 Jul 2017 12:35
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF070117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jul 07 13:02:33 2017

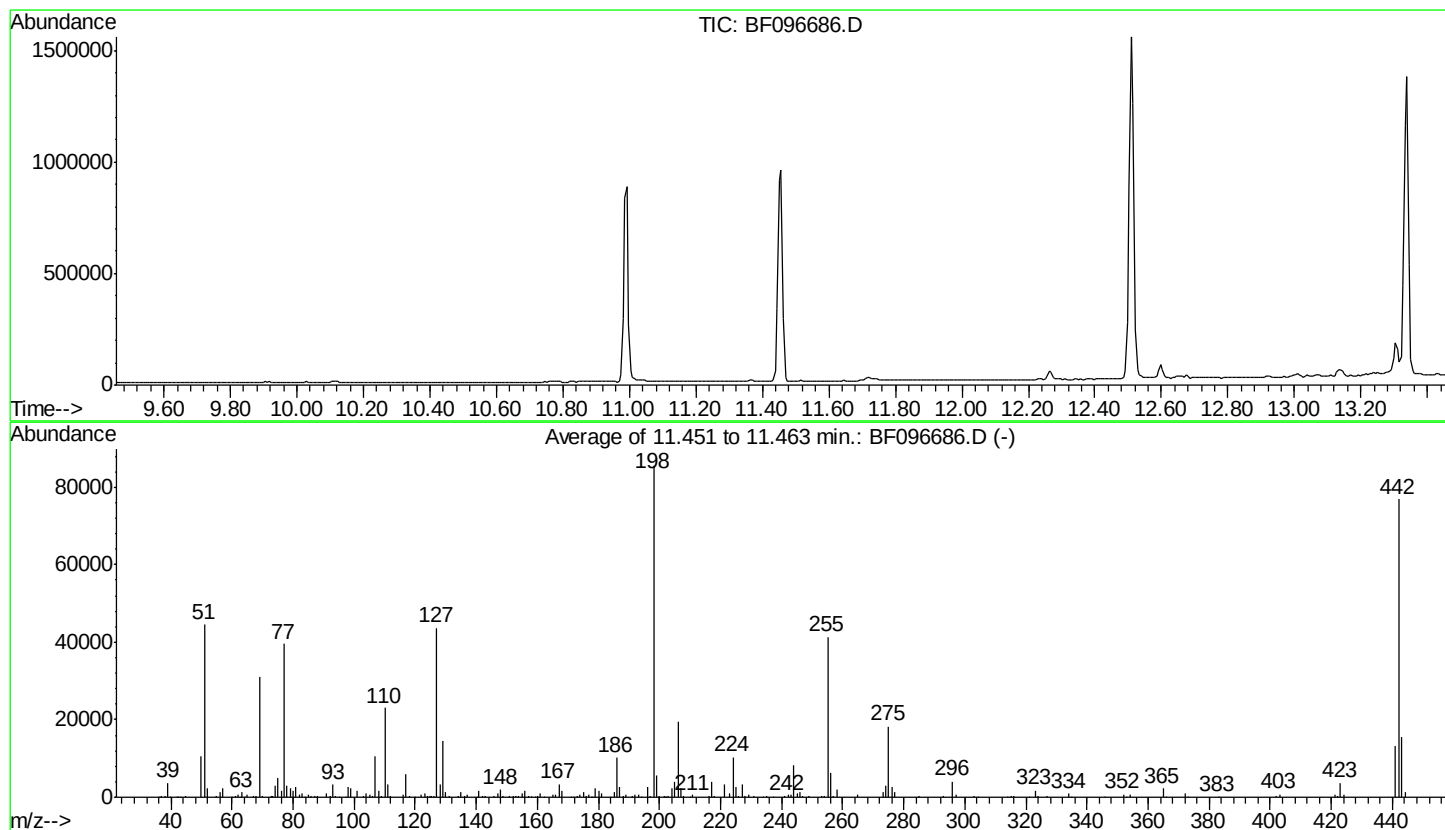

AutoFind: Scans 1592, 1593, 1594; Background Corrected with Scan 1586

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	52.0	44513	PASS
68	69	0.00	2	1.6	504	PASS
69	198	0.00	100	36.4	31173	PASS
70	69	0.00	2	0.8	261	PASS
127	198	10	80	51.1	43741	PASS
197	198	0.00	2	0.3	264	PASS
198	198	100	100	100.0	85552	PASS
199	198	5	9	6.6	5681	PASS
275	198	10	60	21.4	18297	PASS
365	198	1	100	2.6	2214	PASS
441	442	0.01	24	17.0	13089	PASS
442	198	50	100	89.8	76813	PASS
443	442	15	24	20.1	15419	PASS