


Data Path : Z:\HPCHEM1\BNA_F\Data\BF071217\
Data File : BF096713.D
Acq On : 13 Jul 2017 2:09
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF070117.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jul 07 13:02:33 2017

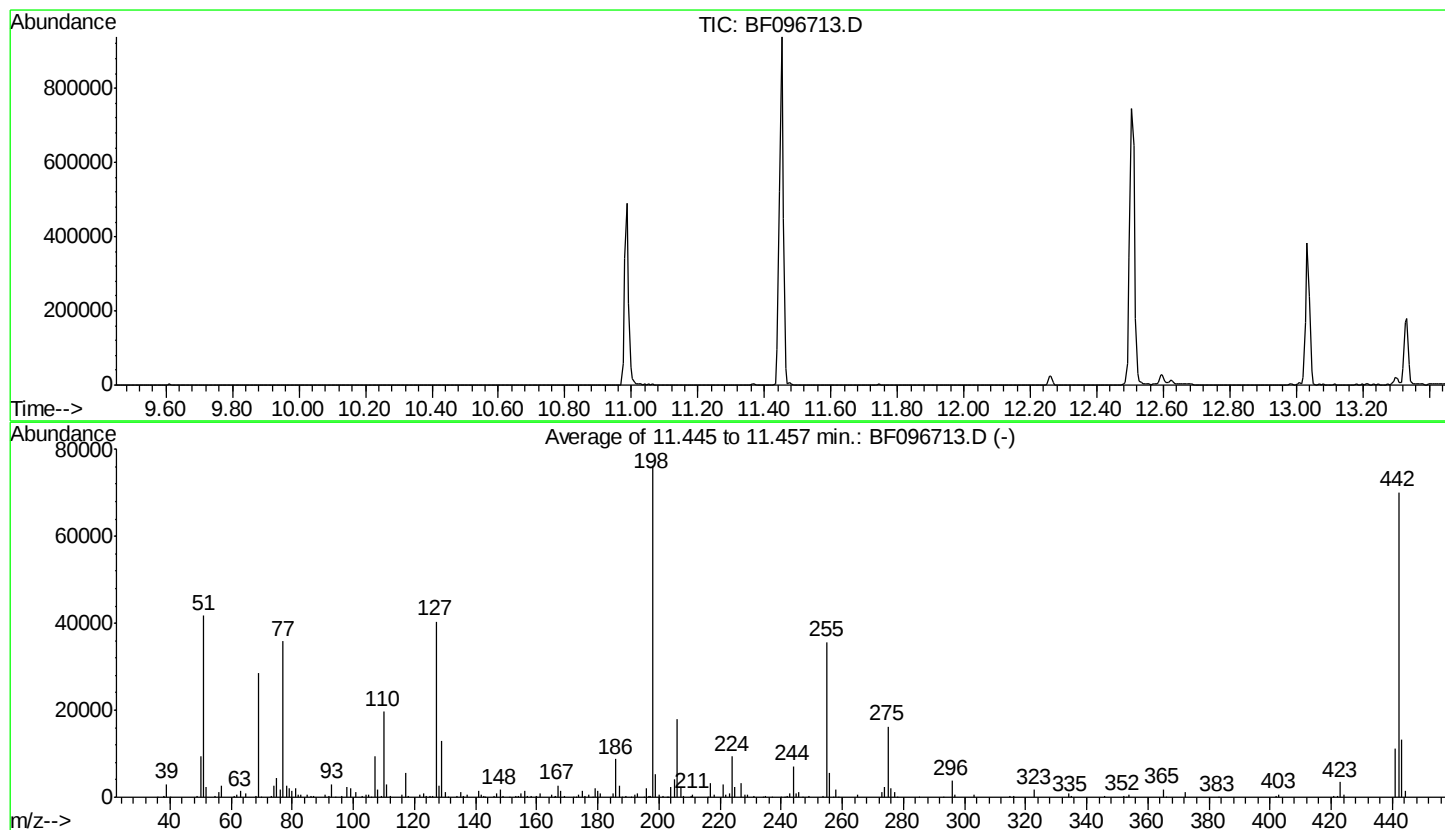

AutoFind: Scans 1591, 1592, 1593; Background Corrected with Scan 1586

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	54.7	41730	PASS
68	69	0.00	2	1.4	407	PASS
69	198	0.00	100	37.4	28545	PASS
70	69	0.00	2	0.5	131	PASS
127	198	10	80	52.9	40368	PASS
197	198	0.00	2	0.6	439	PASS
198	198	100	100	100.0	76250	PASS
199	198	5	9	7.0	5372	PASS
275	198	10	60	21.3	16254	PASS
365	198	1	100	2.4	1793	PASS
441	442	0.01	24	16.2	11343	PASS
442	198	50	100	92.0	70165	PASS
443	442	15	24	18.9	13249	PASS