


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF071315\
 Data File : BF080446.D
 Acq On : 14 Jul 2015 3:30
 Operator : TP/UM
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF071015.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Jul 11 05:35:30 2015

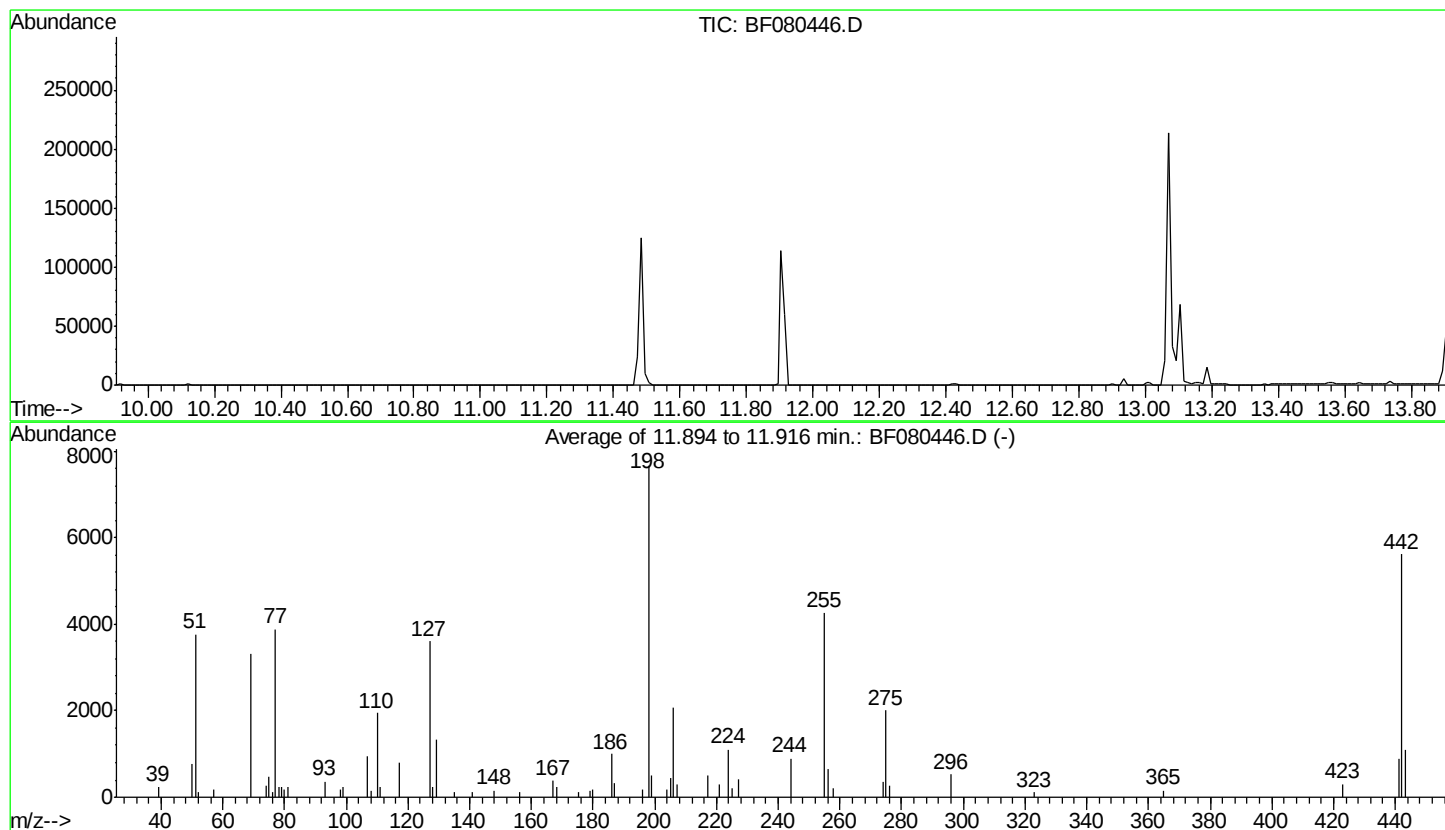

AutoFind: Scans 858, 859, 860; Background Corrected with Scan 856

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.1	3758	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	43.1	3302	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.1	3606	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	7661	PASS
199	198	5	9	6.4	491	PASS
275	198	10	60	26.2	2009	PASS
365	198	1	100	2.0	153	PASS
441	442	0.01	24	16.1	901	PASS
442	198	50	100	73.3	5612	PASS
443	442	15	24	19.6	1100	PASS