
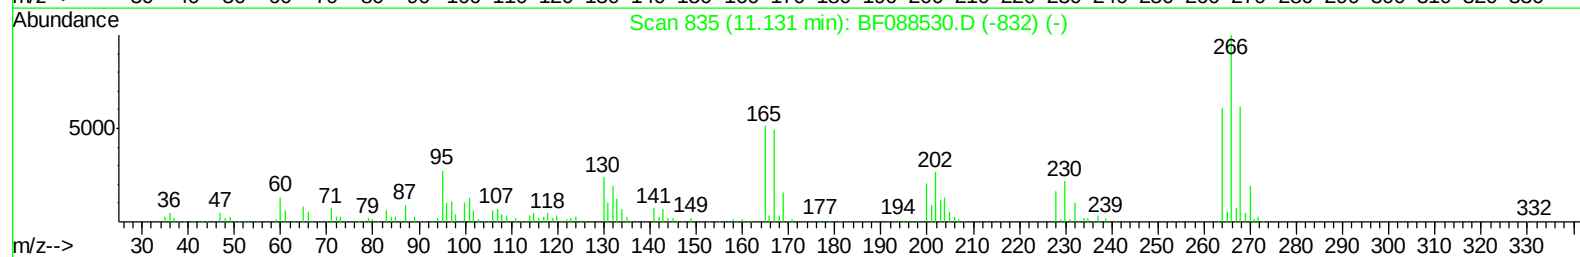
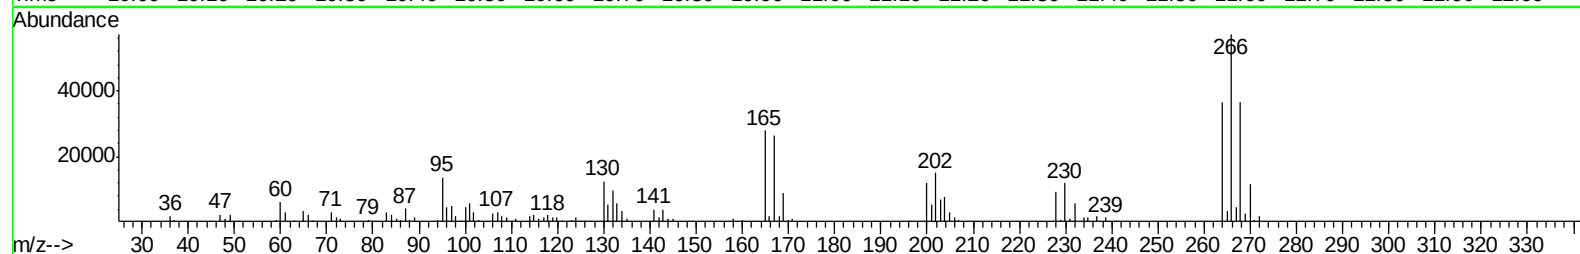


Data Path : Z:\HPCHEM1\BNA F\Data\BF071316\
Data File : BF088956.D
Acq On : 13 Jul 2016 14:01
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 13 19:12:24 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF063016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 11 18:13:32 2016
Response via : Initial Calibration

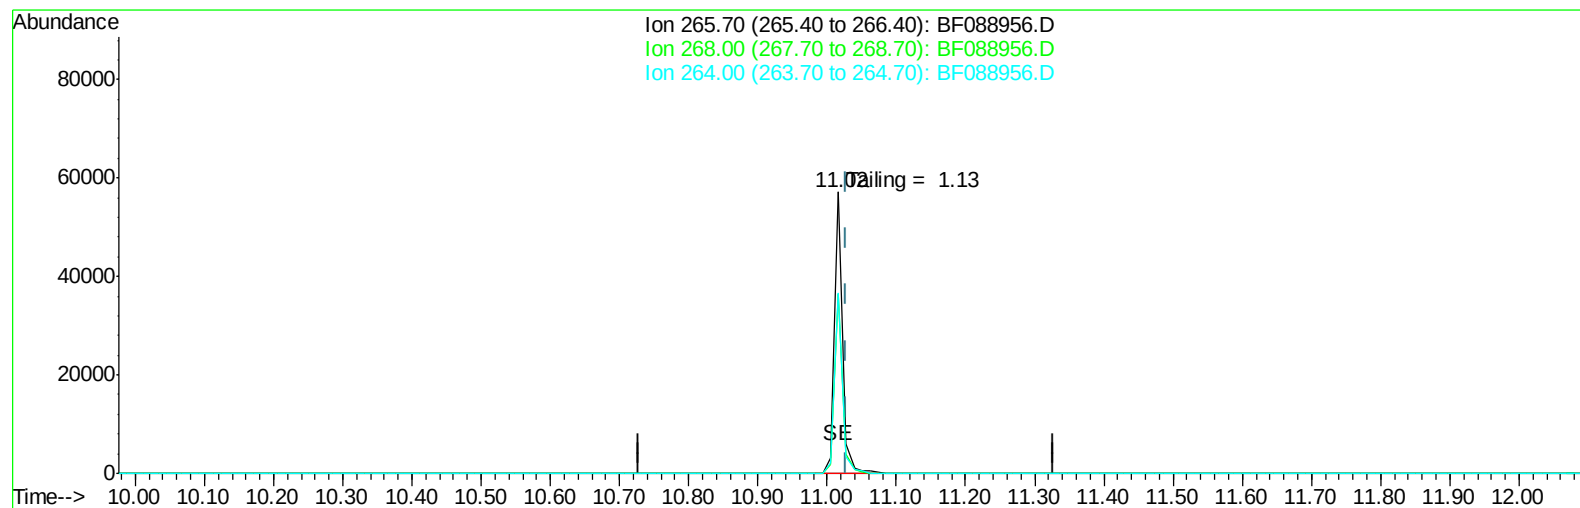

TIC: BF088956.D

(69) Pentachlorophenol (C)




11.016min (-0.011) 0.00ng

response 47243

Ion	Exp%	Act%
265.70	100	100
268.00	66.00	63.79
264.00	62.00	64.13
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF071316\
Data File : BF088956.D
Acq On : 13 Jul 2016 14:01
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 13 19:12:24 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF063016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 11 18:13:32 2016
Response via : Initial Calibration

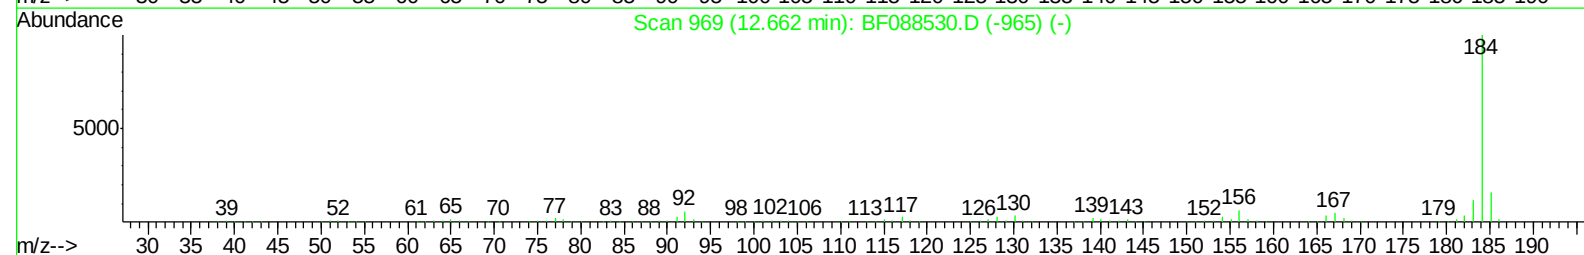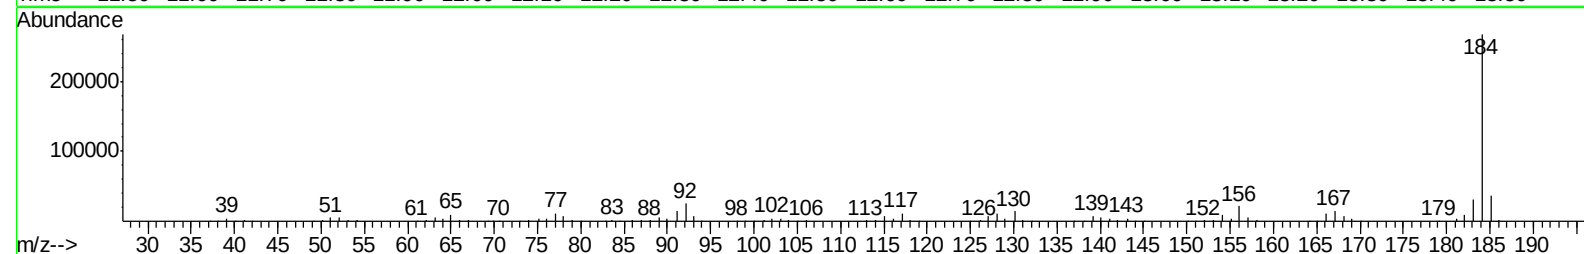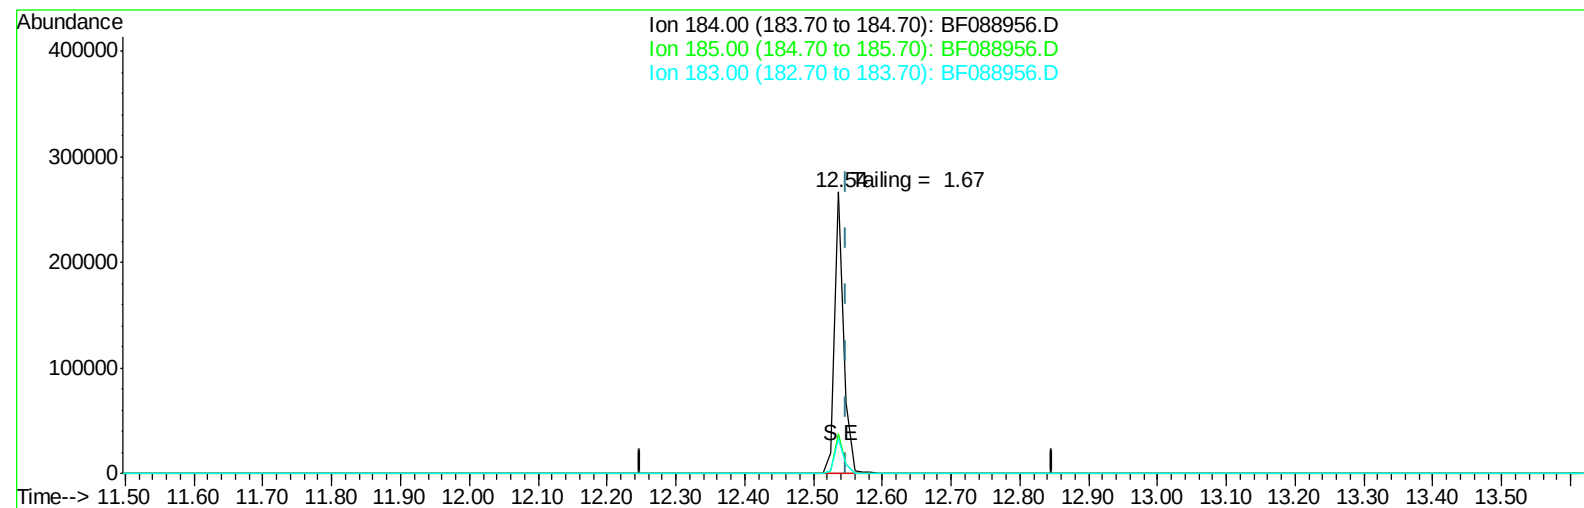

TIC: BF088956.D

(76) Benzidine

12.537min (-0.011) 0.00ng

response 244616

Ion	Exp%	Act%
184.00	100	100
185.00	15.60	14.15
183.00	11.60	12.09
0.00	0.00	0.00