

Data Path : Z:\HPCHEM1\BNA F\DATA\BF071316\
 Data File : BF088979.D
 Acq On : 14 Jul 2016 1:34
 Operator : UM/SJ
 Sample : H3946-11
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 P7-B7(0-8)C

Quant Time: Jul 14 03:23:14 2016
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF063016.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 14 01:23:58 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.70	152	68796	20.00	ng	0.00
21) Naphthalene-d8	7.98	136	238843	20.00	ng	-0.01
38) Acenaphthene-d10	9.72	164	97492	20.00	ng	-0.01
63) Phenanthrene-d10	11.20	188	157025	20.00	ng	-0.01
75) Chrysene-d12	13.83	240	129549	20.00	ng	-0.01
86) Perylene-d12	15.20	264	108207	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.30	112	590540	128.65	ng	0.01
7) Phenol-d6	6.35	99	751461	126.69	ng	0.00
23) Nitrobenzene-d5	7.27	82	497656	109.19	ng	0.00
41) 2,4,6-Tribromophenol	10.51	330	119812	132.34	ng	-0.01
44) 2-Fluorobiphenyl	9.06	172	706123	114.41	ng	0.00
78) Terphenyl-d14	12.79	244	424018	72.90	ng	-0.01
Target Compounds						
49) Dimethylphthalate	9.45	163	109627	15.78	ng	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF071316\
Data File : BF088979.D
Acq On : 14 Jul 2016 1:34
Operator : UM/SJ
Sample : H3946-11
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P7-B7(0-8)C

Quant Time: Jul 14 03:23:14 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF063016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 14 01:23:58 2016
Response via : Initial Calibration

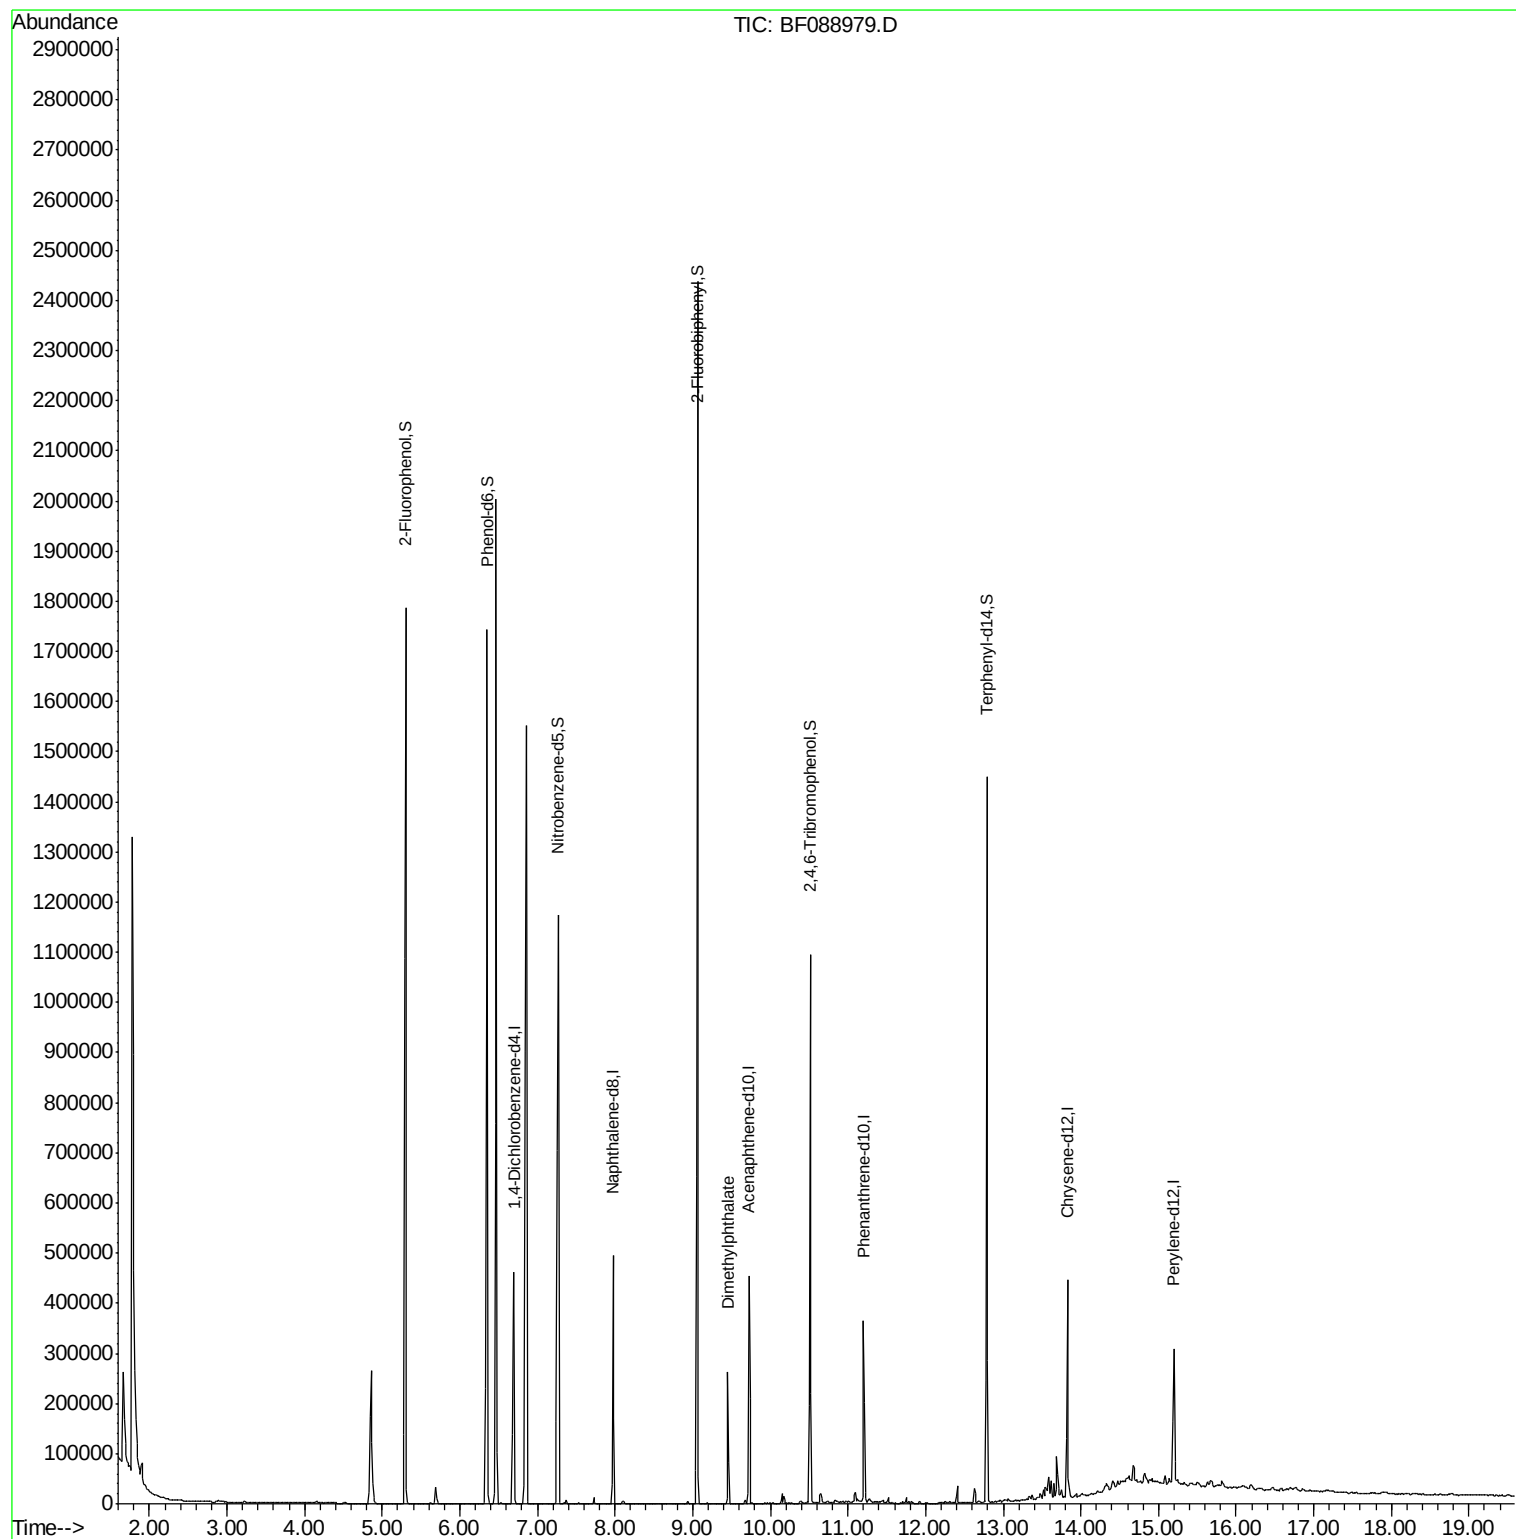

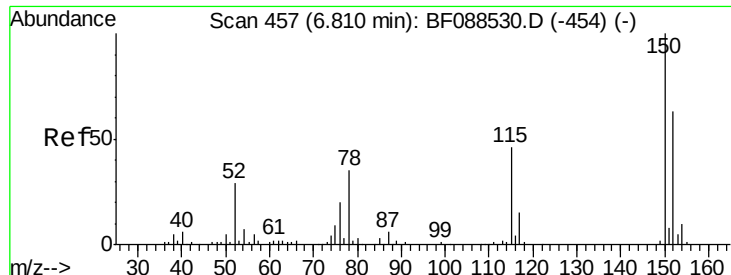

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.70 min Scan# 447

Delta R.T. 0.00 min

Lab File: BF088979.D

Acq: 14 Jul 2016 1:34

Instrument :

BNA_F

ClientSampleId :

P7-B7(0-8)C


Tot Ion:152 Resp: 68796

Ion Ratio Lower Upper

152 100

150 157.0 123.8 185.6




115 63.1 39.6 59.4#

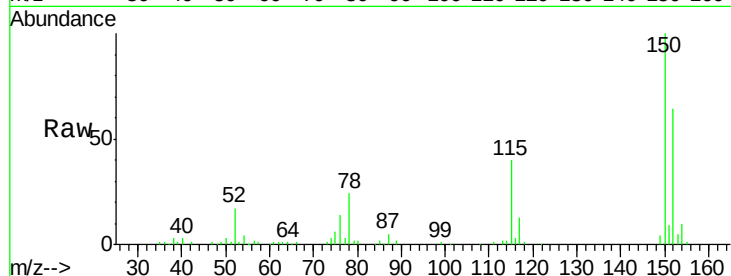

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

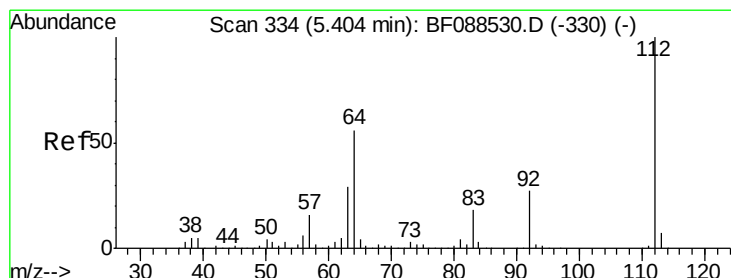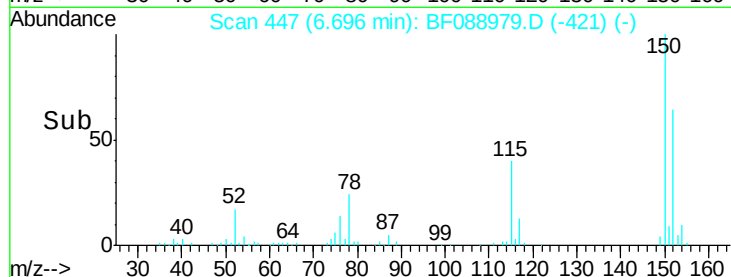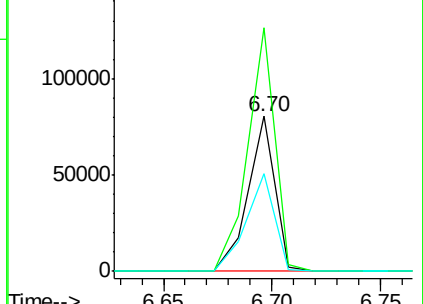

#5

2-Fluorophenol

Concen: 128.65 ng

RT: 5.30 min Scan# 325

Delta R.T. 0.01 min

Lab File: BF088979.D

Acq: 14 Jul 2016 1:34


Tgt Ion:112 Resp: 590540

Ion Ratio Lower Upper

112 100

64 55.3 42.2 63.2



63 30.1 21.8 32.8

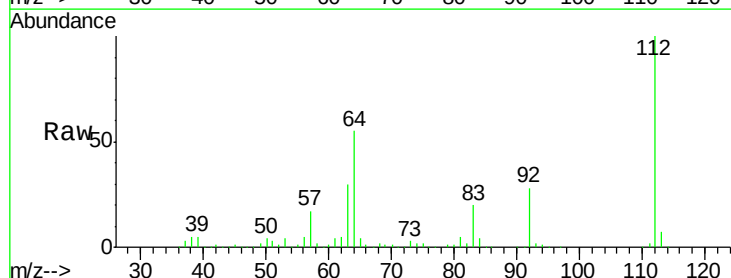


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

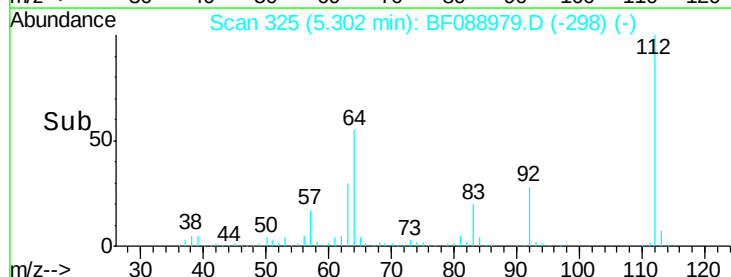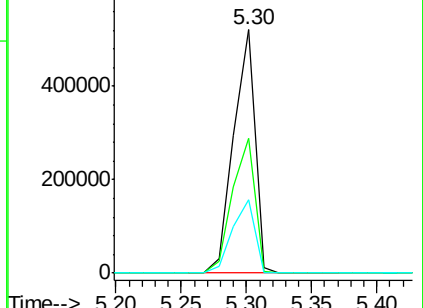

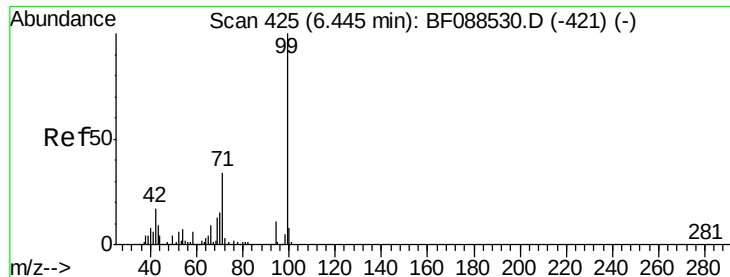

#7

Phenol-d6

Concen: 126.69 ng

RT: 6.35 min Scan# 417

Delta R.T. 0.00 min

Lab File: BF088979.D

Acq: 14 Jul 2016 1:34

Instrument :

BNA_F

ClientSampleId :

P7-B7(0-8)C


Tot Ion: 99 Resp: 751461

Ion Ratio Lower Upper

99 100

42 17.5 12.2 18.2

71 38.3 23.4 35.0#

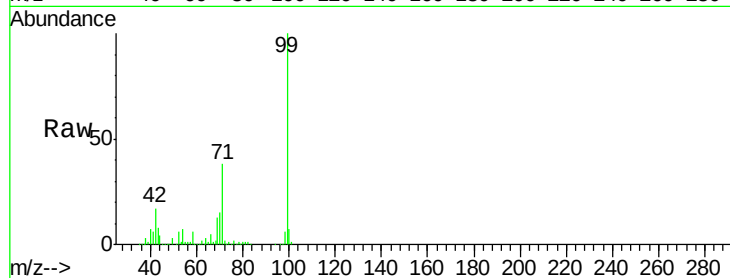

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

6.35

800000

600000



400000

200000

0

6.30 6.35 6.40 6.45

Time-->

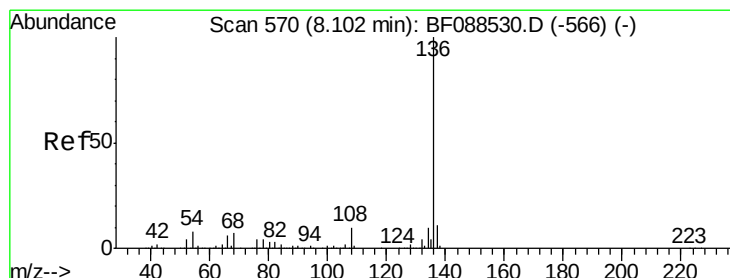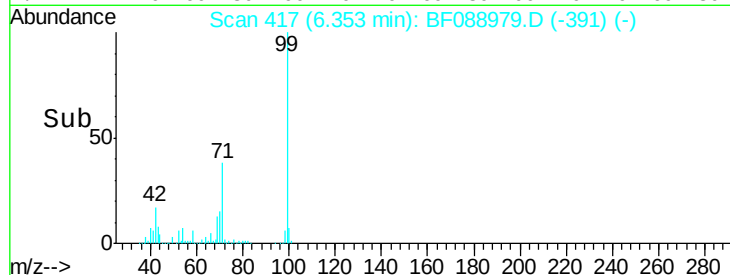

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 7.98 min Scan# 559

Delta R.T. -0.01 min

Lab File: BF088979.D

Acq: 14 Jul 2016 1:34

Tgt Ion: 136 Resp: 238843


Ion Ratio Lower Upper

136 100

137 11.1 9.1 13.7

54 8.6 6.6 10.0

68 6.6 5.1 7.7

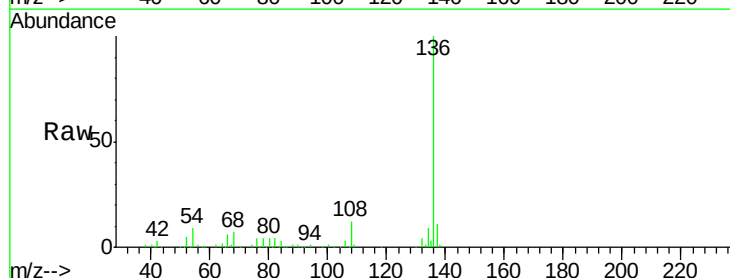

Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

7.98

300000


200000


100000

0

7.95 8.00 8.05

Time-->

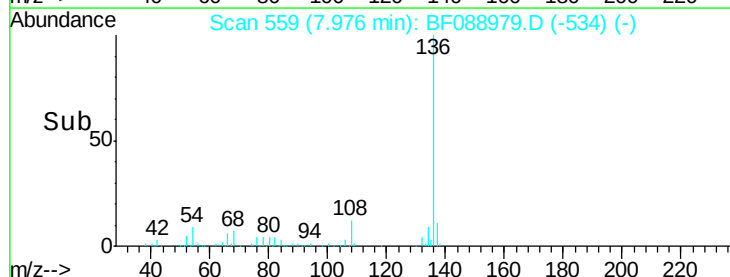


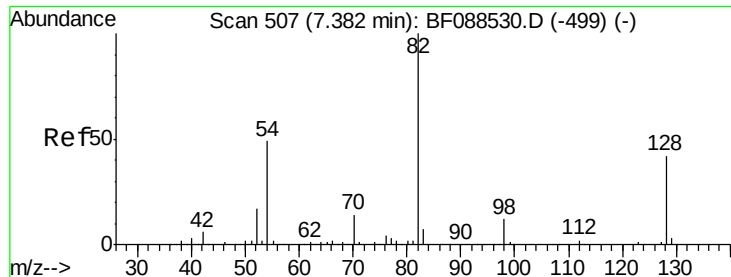




#23
 Nitrobenzene-d5
 Concen: 109.19 ng
 RT: 7.27 min Scan# 497
 Delta R.T. 0.00 min
 Lab File: BF088979.D
 Acq: 14 Jul 2016 1:34

Instrument :
 BNA_F
 ClientSampled :
 P7-B7(0-8)C

Tot Ion	82	Resp	497656
Ion Ratio	Lower	Upper	
82	100		
128	46.1	35.9	53.9
54	44.1	40.9	61.3

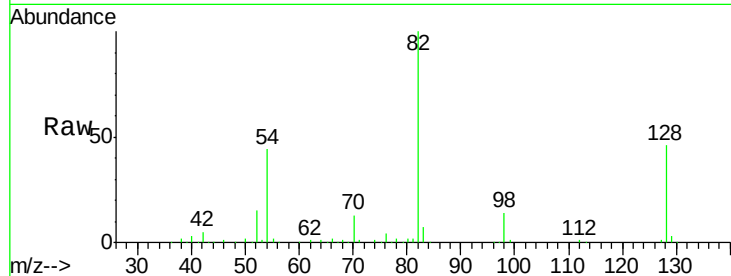


Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 128.00 (127.70 to 128.70): B
 Ion 54.00 (53.70 to 54.70): BF0

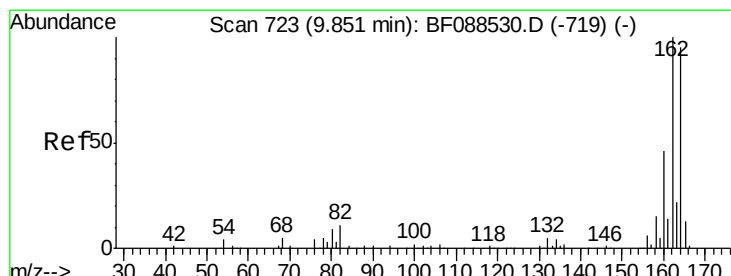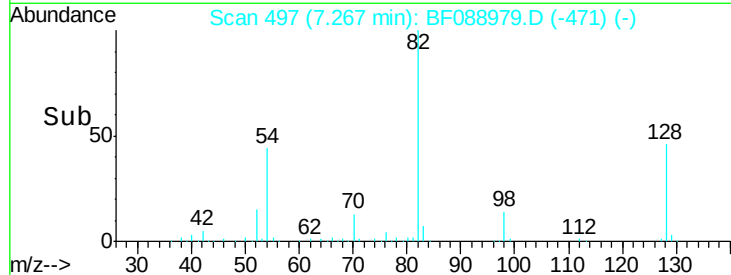
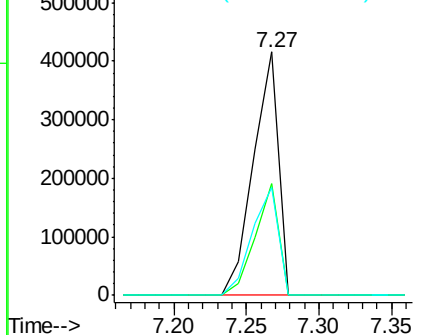



#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.72 min Scan# 712
 Delta R.T. -0.01 min
 Lab File: BF088979.D
 Acq: 14 Jul 2016 1:34

Tgt Ion	164	Resp	97492
Ion Ratio	Lower	Upper	
164	100		
162	104.8	85.4	128.2
160	46.1	39.5	59.3

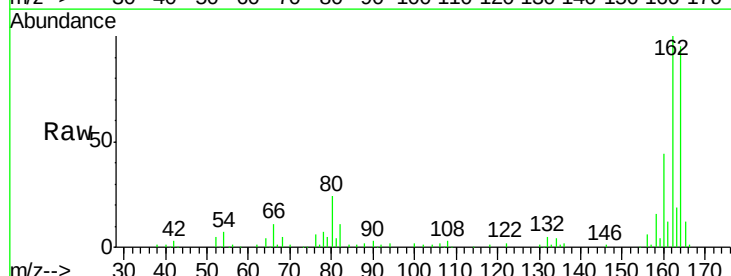

Abundance Ion 164.00 (163.70 to 164.70): B
 Ion 162.00 (161.70 to 162.70): B
 Ion 160.00 (159.70 to 160.70): B

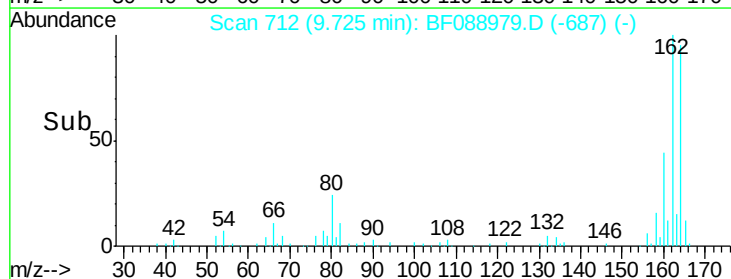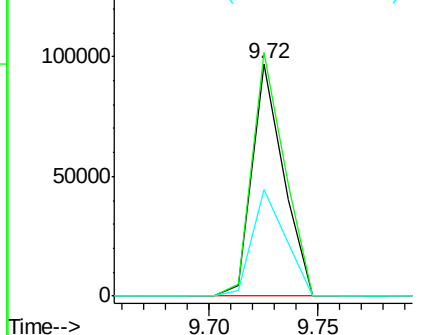


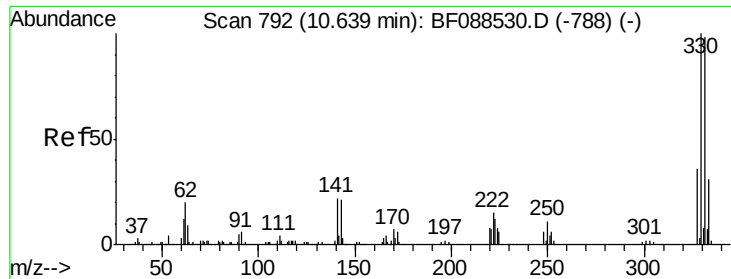




#41
 2,4,6-Tribromophenol
 Concen: 132.34 ng
 RT: 10.51 min Scan# 781
 Delta R.T. -0.01 min
 Lab File: BF088979.D
 Acq: 14 Jul 2016 1:34

Instrument :
 BNA_F
 ClientSampleId :
 P7-B7(0-8)C

Tot Ion	Ratio	Lower	Upper
330	100		
332	97.4	0.0	0.0#
141	41.4	0.0	0.0#

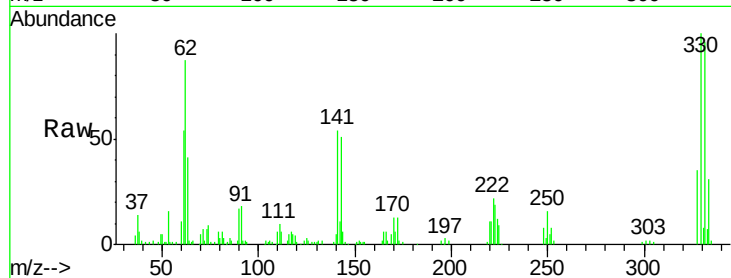


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

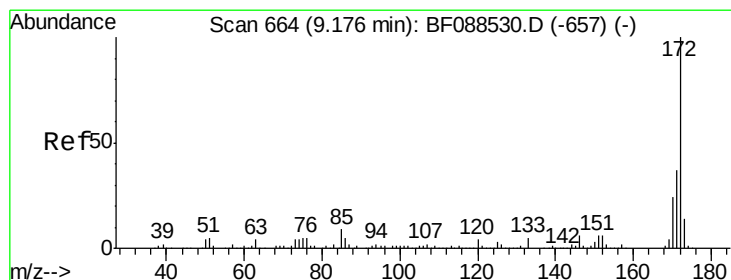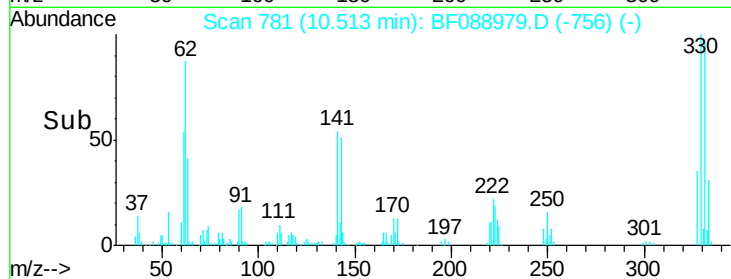
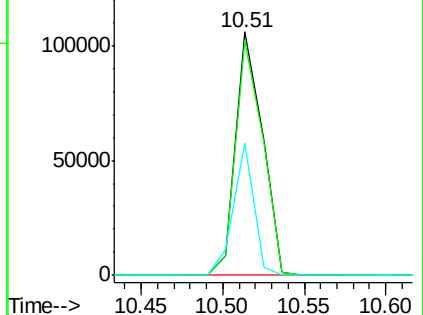



#44
 2-Fluorobiphenyl
 Concen: 114.41 ng
 RT: 9.06 min Scan# 654
 Delta R.T. 0.00 min
 Lab File: BF088979.D
 Acq: 14 Jul 2016 1:34

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.4	28.6	43.0
170	24.0	19.2	28.8

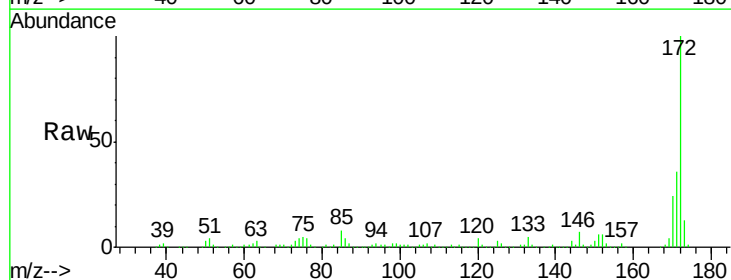

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

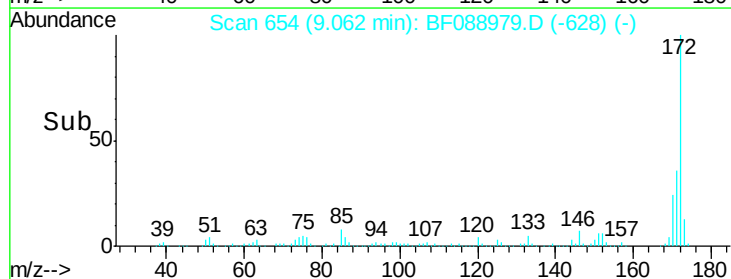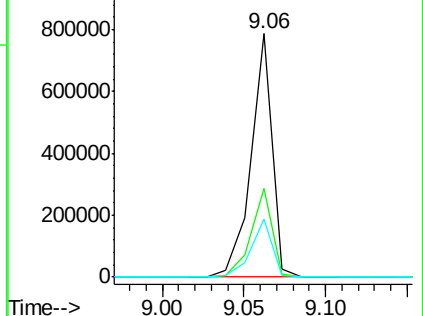

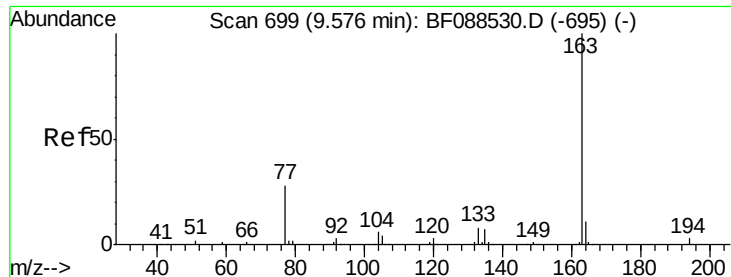

#49

Dimethylphthalate

Concen: 15.78 ng

RT: 9.45 min Scan# 688

Delta R.T. -0.02 min

Lab File: BF088979.D

Acq: 14 Jul 2016 1:34

Instrument :

BNA_F

ClientSampleId :

P7-B7(0-8)C


Tot Ion:163 Resp: 109627

Ion Ratio Lower Upper

163 100

194 3.2 2.8 4.2




164 10.6 8.3 12.5

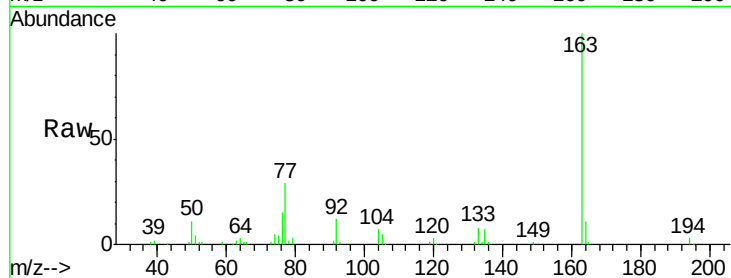

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

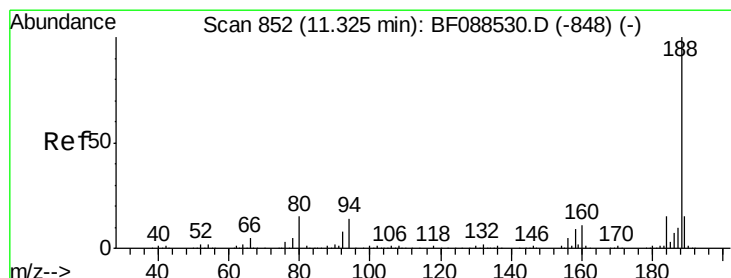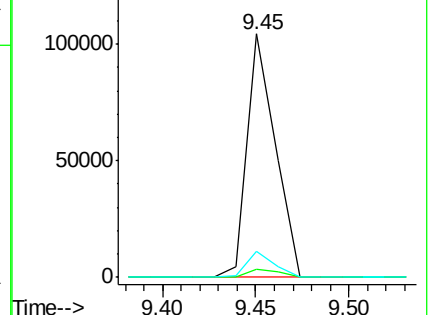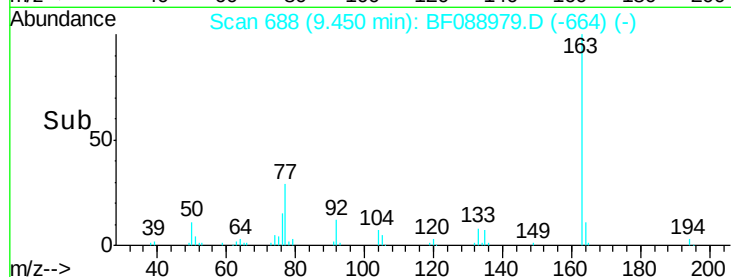

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 11.20 min Scan# 841

Delta R.T. -0.01 min

Lab File: BF088979.D

Acq: 14 Jul 2016 1:34


Tgt Ion:188 Resp: 157025

Ion Ratio Lower Upper

188 100

94 12.0 9.0 13.6



80 14.2 10.0 15.0

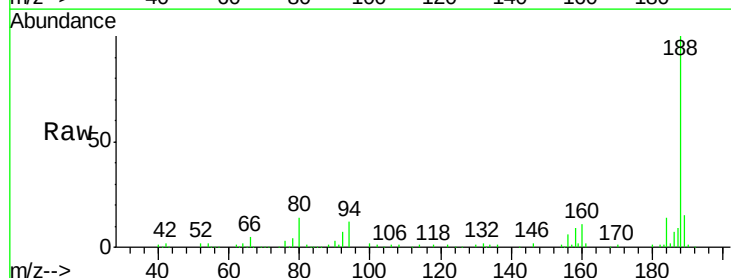


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

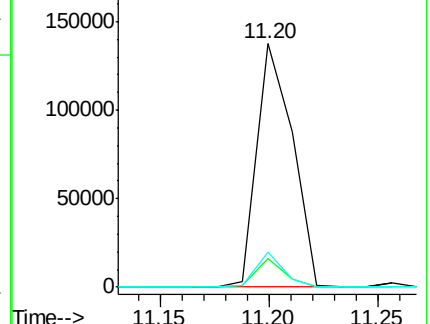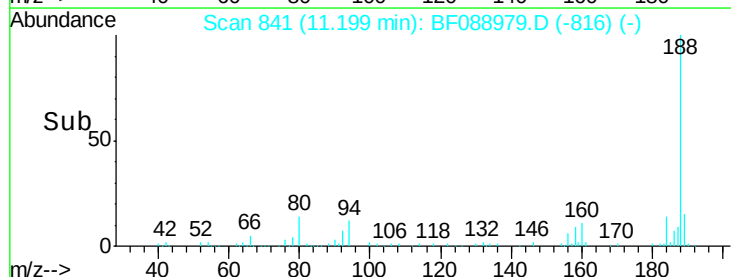

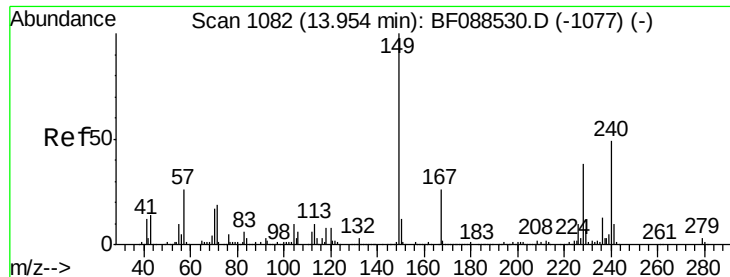

#75

Chrysene-d12

Concen: 20.00 ng

RT: 13.83 min Scan# 1071

Delta R.T. -0.01 min

Lab File: BF088979.D

Acq: 14 Jul 2016 1:34

Instrument :

BNA_F

ClientSampleId :

P7-B7(0-8)C


Tot Ion:240 Resp: 129549

Ion Ratio Lower Upper

240 100

120 11.2 6.8 10.2#




236 25.3 20.2 30.2

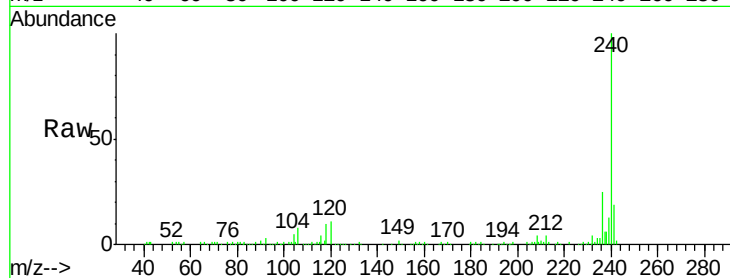

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

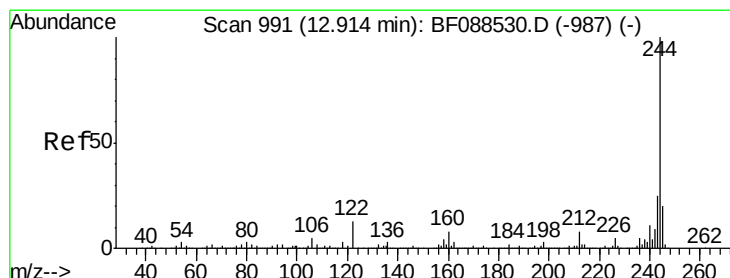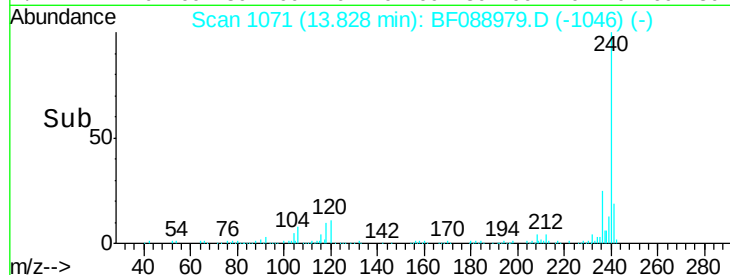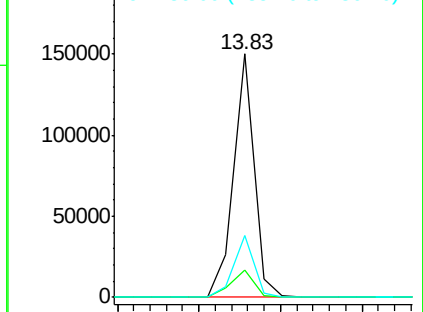

#78

Terphenyl-d14

Concen: 72.90 ng

RT: 12.79 min Scan# 980

Delta R.T. -0.01 min

Lab File: BF088979.D

Acq: 14 Jul 2016 1:34


Tgt Ion:244 Resp: 424018

Ion Ratio Lower Upper

244 100

212 8.0 6.0 9.0



122 15.2 11.2 16.8



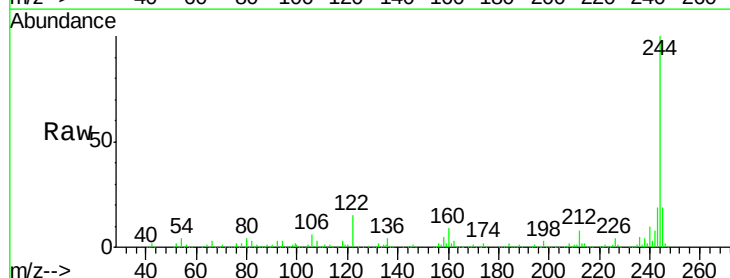


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

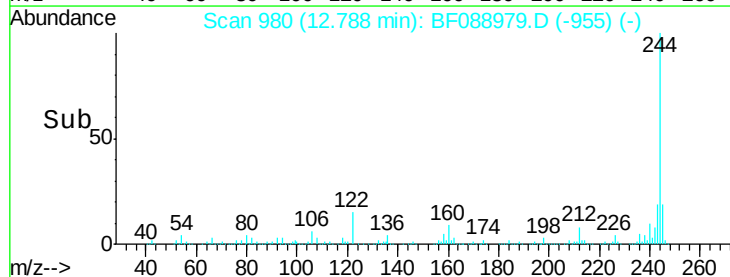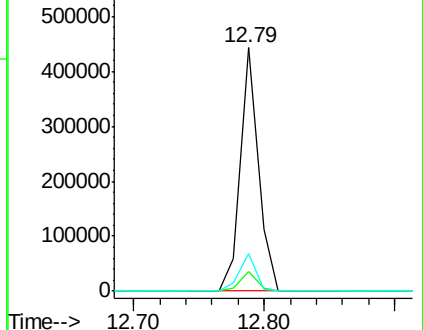

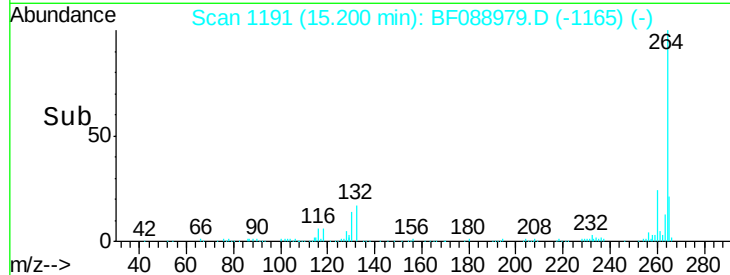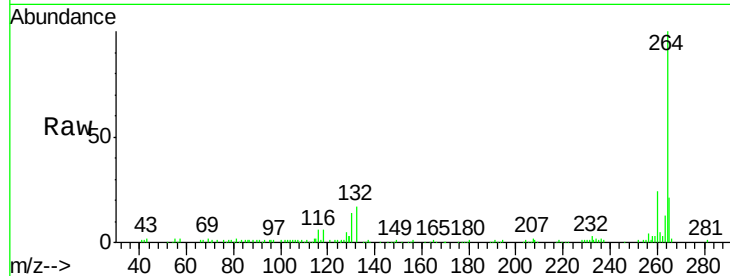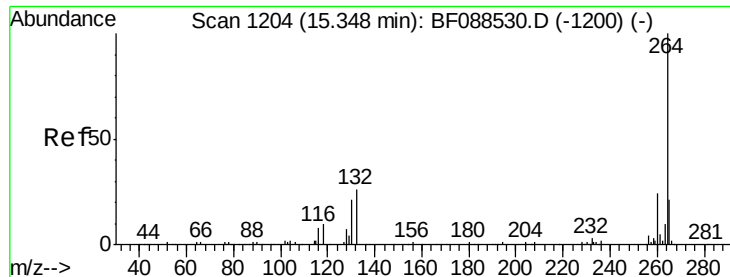

#86
 Pervlene-d12
 Concen: 20.00 ng
 RT: 15.20 min Scan# 1191
 Delta R.T. 0.00 min
 Lab File: BF088979.D
 Acq: 14 Jul 2016 1:34

Instrument :
 BNA_F
 ClientSampleId :
 P7-B7(0-8)C

Tot Ion:	264	Resp:	108207
Ion	Ratio	Lower	Upper
264	100		
260	24.0	19.2	28.8
265	21.5	16.9	25.3

