


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF071316\
 Data File : BF088956.D
 Acq On : 13 Jul 2016 14:01
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jul 11 18:13:32 2016

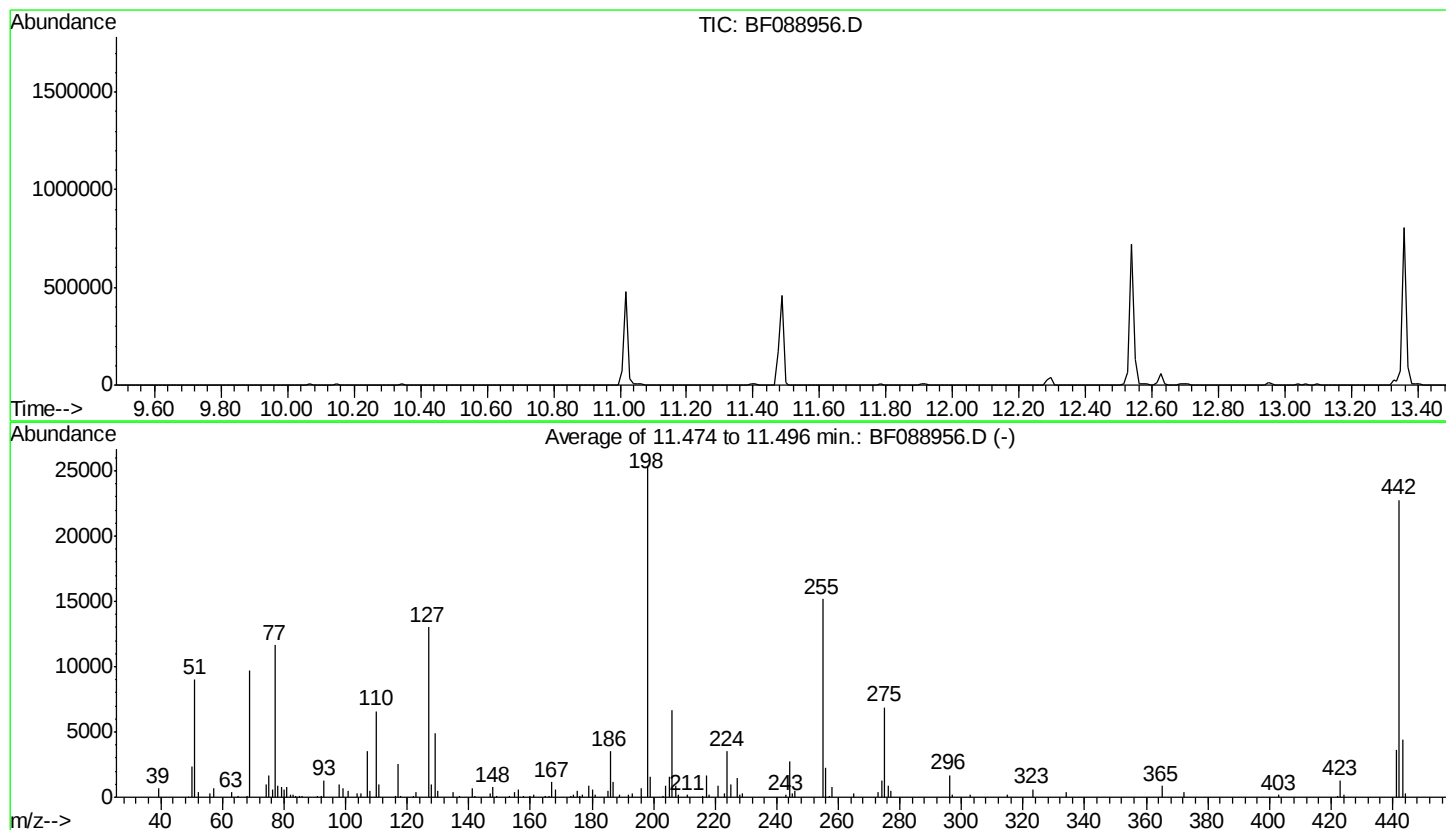

AutoFind: Scans 865, 866, 867; Background Corrected with Scan 862

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.4	8976	PASS
68	69	0.00	2	1.1	111	PASS
69	198	0.00	100	38.3	9726	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.3	13022	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	25387	PASS
199	198	5	9	6.2	1568	PASS
275	198	10	60	27.2	6909	PASS
365	198	1	100	3.5	881	PASS
441	442	0.01	24	16.1	3663	PASS
442	198	50	100	89.8	22785	PASS
443	442	15	24	19.6	4460	PASS