

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF071317\
 Data File : BF096750.D
 Acq On : 14 Jul 2017 1:50
 Operator : SJ/JU
 Sample : I4163-01
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SU-04-071217

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF071317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.810	476	480	490	rBV	279627	377097	16.02%	1.599%
2	5.245	549	554	557	rBV	2396833	2354502	100.00%	9.983%
3	6.281	725	730	733	rBV	2260990	2260049	95.99%	9.583%
4	6.404	747	751	755	rBV	2256472	2212394	93.96%	9.381%
5	6.792	813	817	821	rBV	1729996	1496689	63.57%	6.346%
6	7.198	879	886	889	rBV	1499747	1318767	56.01%	5.592%
7	7.292	898	902	906	rBV6	18218	26243	1.11%	0.111%
8	7.445	925	928	933	rVB4	21862	25559	1.09%	0.108%
9	7.663	961	965	968	rBV2	34976	40666	1.73%	0.172%
10	7.939	1010	1012	1015	rVB	36956	26759	1.14%	0.113%
11	8.634	1126	1130	1133	rVB	70017	63278	2.69%	0.268%
12	8.728	1142	1146	1151	rBV	73665	67711	2.88%	0.287%
13	8.998	1187	1192	1195	rBV	2017833	1775320	75.40%	7.528%
14	9.092	1202	1208	1212	rBV5	28208	31670	1.35%	0.134%
15	9.192	1222	1225	1229	rBV	18604	24445	1.04%	0.104%
16	9.257	1231	1236	1239	rBV2	44514	59729	2.54%	0.253%
17	9.328	1245	1248	1251	rBV	75968	71437	3.03%	0.303%
18	9.357	1251	1253	1255	rVV	42651	31784	1.35%	0.135%
19	9.386	1255	1258	1261	rVV	257740	223927	9.51%	0.949%
20	9.445	1265	1268	1274	rVB	42480	49940	2.12%	0.212%
21	9.528	1278	1282	1286	rBV	107056	106185	4.51%	0.450%
22	9.586	1289	1292	1295	rVB4	25175	24613	1.05%	0.104%
23	9.657	1301	1304	1307	rBV4	22870	26881	1.14%	0.114%
24	9.698	1307	1311	1315	rVB	88892	80626	3.42%	0.342%
25	9.781	1320	1325	1328	rBV3	25447	38064	1.62%	0.161%
26	9.822	1328	1332	1335	rBV3	18887	25016	1.06%	0.106%
27	9.875	1337	1341	1345	rVV4	45910	57189	2.43%	0.242%
28	9.910	1345	1347	1350	rVB	35781	30586	1.30%	0.130%
29	9.986	1356	1360	1363	rBV3	41216	56870	2.42%	0.241%
30	10.016	1363	1365	1367	rVB	33084	25251	1.07%	0.107%
31	10.080	1372	1376	1380	rBV5	31393	46827	1.99%	0.199%
32	10.116	1380	1382	1385	rVB	45170	36034	1.53%	0.153%
33	10.163	1385	1390	1393	rBV5	18826	28938	1.23%	0.123%
34	10.210	1396	1398	1401	rBV2	92039	79547	3.38%	0.337%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF071317\
 Data File : BF096750.D
 Acq On : 14 Jul 2017 1:50
 Operator : SJ/JU
 Sample : I4163-01
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SU-04-071217

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF071317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	10.280	1405	1410	1411	rBV2	37357	39213	1.67%	0.166%
36	10.328	1416	1418	1422	rVB4	22961	33480	1.42%	0.142%
37	10.451	1435	1439	1443	rBV	1042113	922676	39.19%	3.912%
38	10.586	1458	1462	1469	rVB3	74093	95625	4.06%	0.405%
39	10.763	1486	1492	1494	rBV4	43999	68274	2.90%	0.289%
40	10.786	1494	1496	1500	rVV2	58803	72448	3.08%	0.307%
41	10.845	1503	1506	1509	rVB2	42396	49107	2.09%	0.208%
42	10.910	1515	1517	1522	rVB4	34229	30531	1.30%	0.129%
43	10.951	1522	1524	1530	rVB5	23711	26517	1.13%	0.112%
44	11.004	1530	1533	1535	rBV3	29363	29446	1.25%	0.125%
45	11.039	1535	1539	1542	rVV2	82214	88276	3.75%	0.374%
46	11.063	1542	1543	1548	rVB	32305	29883	1.27%	0.127%
47	11.169	1557	1561	1564	rBV	628073	507683	21.56%	2.153%
48	11.222	1566	1570	1573	rVB	195117	184381	7.83%	0.782%
49	11.257	1573	1576	1580	rBV3	39975	63351	2.69%	0.269%
50	11.475	1609	1613	1616	rVB3	59789	72385	3.07%	0.307%
51	11.557	1625	1627	1631	rVB	42680	40456	1.72%	0.172%
52	11.645	1639	1642	1645	rBV	150912	155711	6.61%	0.660%
53	11.675	1645	1647	1652	rVB	217299	183986	7.81%	0.780%
54	11.722	1652	1655	1658	rBV	104527	80731	3.43%	0.342%
55	11.757	1658	1661	1663	rVV	297339	290787	12.35%	1.233%
56	11.780	1663	1665	1668	rVB	139681	108719	4.62%	0.461%
57	11.845	1672	1676	1678	rBV4	26103	33211	1.41%	0.141%
58	11.880	1678	1682	1685	rVV2	35237	40619	1.73%	0.172%
59	11.939	1690	1692	1694	rBV	70971	57874	2.46%	0.245%
60	11.963	1694	1696	1700	rVB2	59673	65216	2.77%	0.277%
61	12.016	1703	1705	1708	rBV3	24519	27407	1.16%	0.116%
62	12.074	1712	1715	1716	rBV2	34949	37897	1.61%	0.161%
63	12.092	1716	1718	1721	rVB	51501	39525	1.68%	0.168%
64	12.122	1721	1723	1725	rBV	64983	59035	2.51%	0.250%
65	12.145	1725	1727	1731	rVB2	62187	60409	2.57%	0.256%
66	12.198	1732	1736	1739	rBV	156080	171475	7.28%	0.727%
67	12.233	1739	1742	1744	rVV3	104529	113443	4.82%	0.481%
68	12.257	1744	1746	1748	rVV3	53984	47638	2.02%	0.202%
69	12.280	1748	1750	1755	rVB4	63714	88921	3.78%	0.377%
70	12.357	1759	1763	1766	rBV	961068	840685	35.71%	3.565%
71	12.404	1768	1771	1776	rBV4	48887	85738	3.64%	0.364%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF071317\
 Data File : BF096750.D
 Acq On : 14 Jul 2017 1:50
 Operator : SJ/JU
 Sample : I4163-01
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SU-04-071217

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF071317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

72	12.580	1796	1801	1804	rBV	934354	953970	40.52%	4.045%
73	12.698	1819	1821	1823	rBV	50742	49644	2.11%	0.210%
74	12.733	1823	1827	1830	rVV	1497944	1404876	59.67%	5.957%
75	12.804	1835	1839	1841	rBV3	115183	120790	5.13%	0.512%
76	12.886	1851	1853	1854	rBV2	67845	57863	2.46%	0.245%
77	12.910	1855	1857	1860	rVB	241789	204541	8.69%	0.867%
78	12.974	1866	1868	1871	rVB	162470	151540	6.44%	0.643%
79	13.016	1872	1875	1878	rBV	180724	165175	7.02%	0.700%
80	13.104	1887	1890	1893	rVV2	148954	126867	5.39%	0.538%
81	13.133	1893	1895	1899	rVB	146751	133846	5.68%	0.568%
82	13.521	1958	1961	1965	rBV2	107721	169909	7.22%	0.720%
83	13.639	1979	1981	1989	rVB4	196780	316617	13.45%	1.342%
84	13.768	2000	2003	2005	rBV	372440	360690	15.32%	1.529%
85	13.804	2006	2009	2011	rVB	324987	299620	12.73%	1.270%
86	14.780	2172	2175	2183	rVB	270169	503035	21.36%	2.133%
87	15.051	2219	2221	2224	rVB	179892	172362	7.32%	0.731%
88	15.110	2228	2231	2236	rVB	216415	249493	10.60%	1.058%


Sum of corrected areas: 23584190

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF071317\
Data File : BF096750.D
Acq On : 14 Jul 2017 1:50
Operator : SJ/JU
Sample : I4163-01
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SU-04-071217

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF071317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

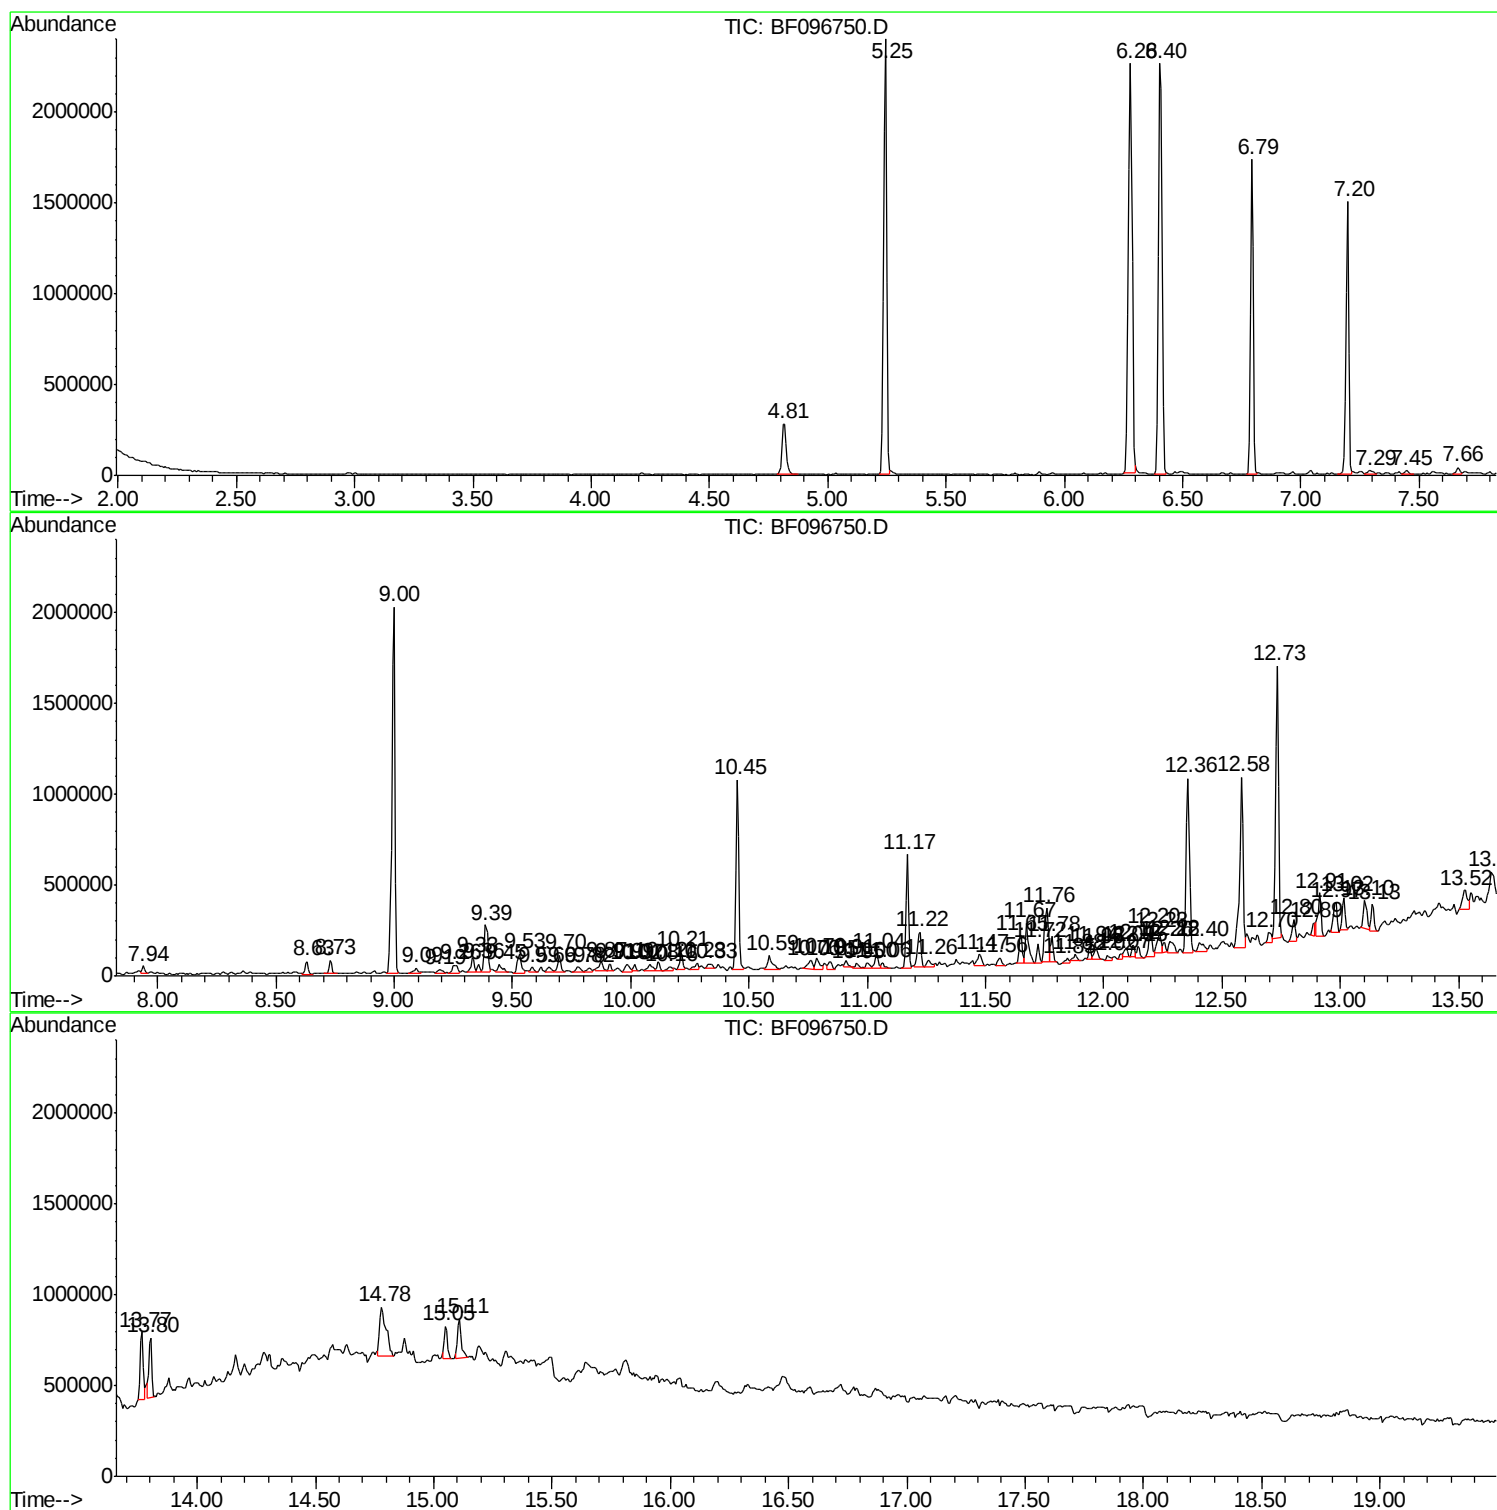

DbaaaPbhh::ZZ\NRPBHHM1BBAFNDAAAB001331X\
 DbaaaFfile::BB0000300DD
 Aeqq00n ::14Jul2007 11500
 Opeaaor ::SSJU
 Sample ::I4163001
 Misc ::
 ASSVaal ::300 SampleMultiplier:11

Instrument :
 BNA_F
 ClientSampleId :
 SU-04-071217

QqaabMebbdd::ZZ\NRPBHHM1BBAFMEH00S8200BB0013317MM
 QqaabTfile ::ASBPBNASSANDABBSF00R55P000NTC6AIBBATION

TICLibbaay ::CC\DAABASSEN0\$T11LL
 TICInteggaionPaaameess:LS6CNTPP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
