


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF071317\
 Data File : BF096718.D
 Acq On : 13 Jul 2017 10:39
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF071317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 13 14:49:34 2017

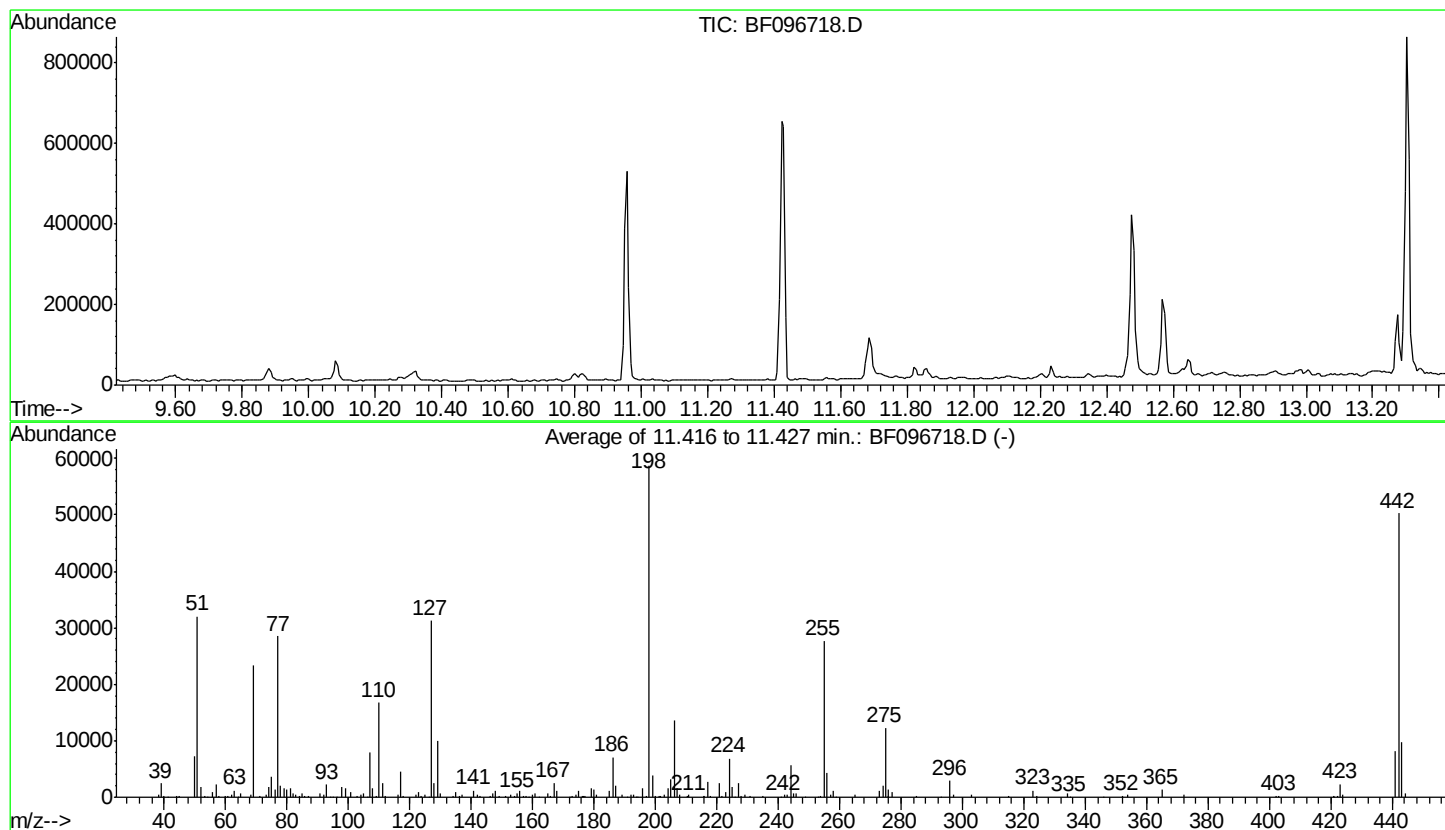

AutoFind: Scans 1586, 1587, 1588; Background Corrected with Scan 1582

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	54.5	31985	PASS
68	69	0.00	2	1.7	388	PASS
69	198	0.00	100	39.8	23394	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.1	31177	PASS
197	198	0.00	2	0.2	129	PASS
198	198	100	100	100.0	58714	PASS
199	198	5	9	6.5	3791	PASS
275	198	10	60	21.0	12355	PASS
365	198	1	100	2.3	1338	PASS
441	442	0.01	24	16.4	8242	PASS
442	198	50	100	85.6	50261	PASS
443	442	15	24	19.2	9642	PASS