


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF071317\
 Data File : BF096738.D
 Acq On : 13 Jul 2017 20:10
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF071317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 13 14:49:34 2017

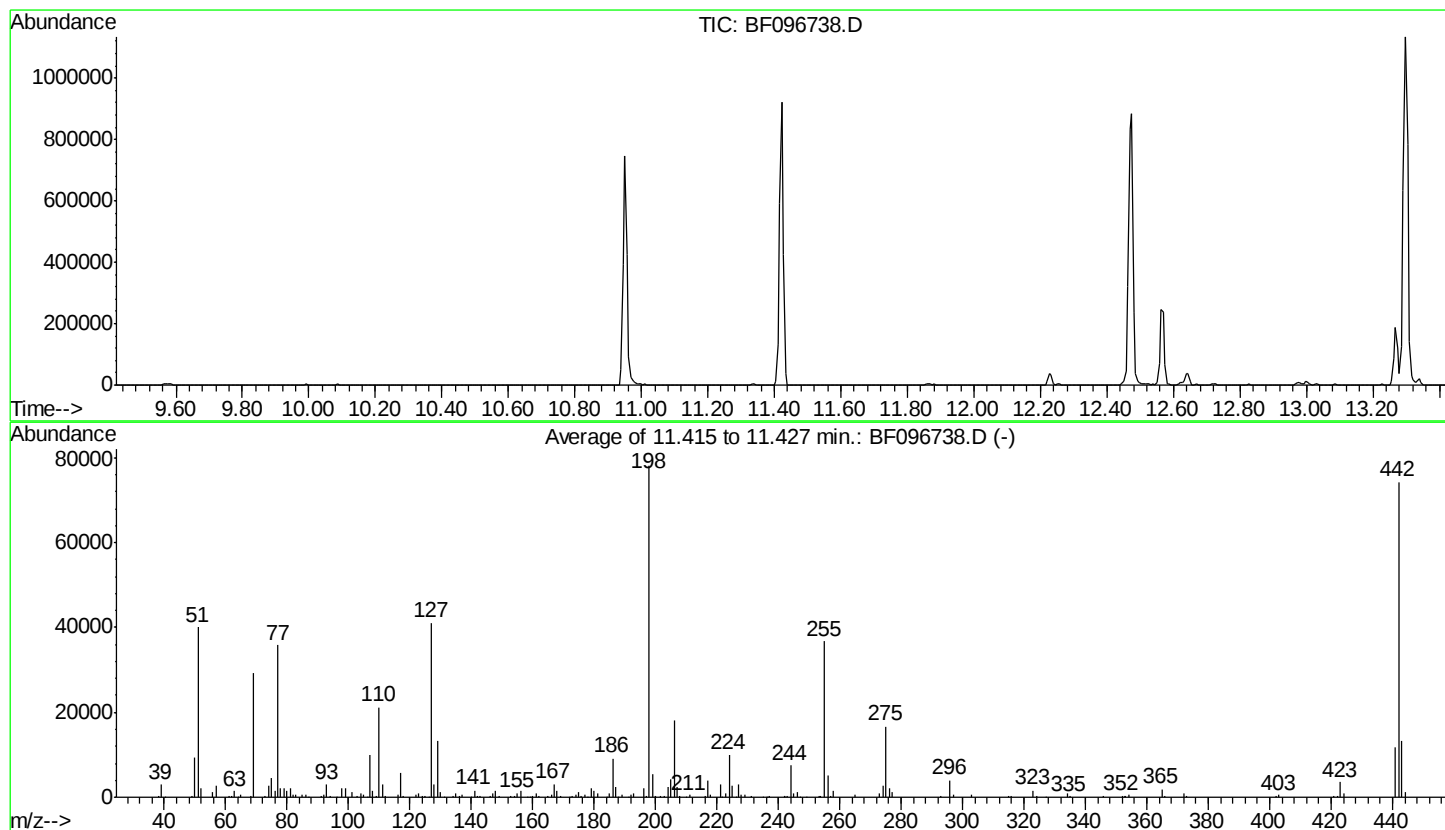

AutoFind: Scans 1586, 1587, 1588; Background Corrected with Scan 1581

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	51.3	40061	PASS
68	69	0.00	2	1.4	406	PASS
69	198	0.00	100	37.4	29201	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.7	41157	PASS
197	198	0.00	2	0.4	304	PASS
198	198	100	100	100.0	78154	PASS
199	198	5	9	6.8	5350	PASS
275	198	10	60	21.2	16596	PASS
365	198	1	100	2.5	1959	PASS
441	442	0.01	24	15.7	11671	PASS
442	198	50	100	95.1	74293	PASS
443	442	15	24	17.9	13295	PASS