

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF071318\
 Data File : BF107395.D
 Acq On : 14 Jul 2018 4:54
 Operator : JU/SJ
 Sample : J3970-09
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 071118-TIPC-F-U-B

Quant Time: Jul 14 05:43:28 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 13 11:54:53 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.92	152	40748	20.00	ng	0.00
21) Naphthalene-d8	8.21	136	138504	20.00	ng	0.00
38) Acenaphthene-d10	9.98	164	67471	20.00	ng	0.00
63) Phenanthrene-d10	11.47	188	145504	20.00	ng	0.00
75) Chrysene-d12	14.13	240	135563	20.00	ng	0.00
86) Perylene-d12	15.67	264	93909	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.57	112	106959	44.45	ng	0.00
7) Phenol-d6	6.58	99	75740	25.20	ng	0.00
23) Nitrobenzene-d5	7.50	82	234906	94.25	ng	0.00
41) 2,4,6-Tribromophenol	10.78	330	78376	100.22	ng	0.00
44) 2-Fluorobiphenyl	9.28	172	424483	111.00	ng	0.00
78) Terphenyl-d14	13.06	244	638046	114.01	ng	0.00
Target Compounds						
19) n-Nitroso-di-n-propylamine	7.50	70	29538	14.911	ng	# 72
25) Isophorone	7.50	82	234904	53.488	ng	# 64
49) Dimethylphthalate	9.68	163	32232	6.369	ng	# 99
50) 2,6-Dinitrotoluene	9.98	165	8511	7.943	ng	# 24
56) 2,4-Dinitrotoluene	9.98	165	8511	6.085	ng	# 21
66) 4-Bromophenyl-phenylether	10.77	248	4586	2.641	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF071318\
Data File : BF107395.D
Acq On : 14 Jul 2018 4:54
Operator : JU/SJ
Sample : J3970-09
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
071118-TIPC-F-U-B

Quant Time: Jul 14 05:43:28 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 13 11:54:53 2018
Response via : Initial Calibration

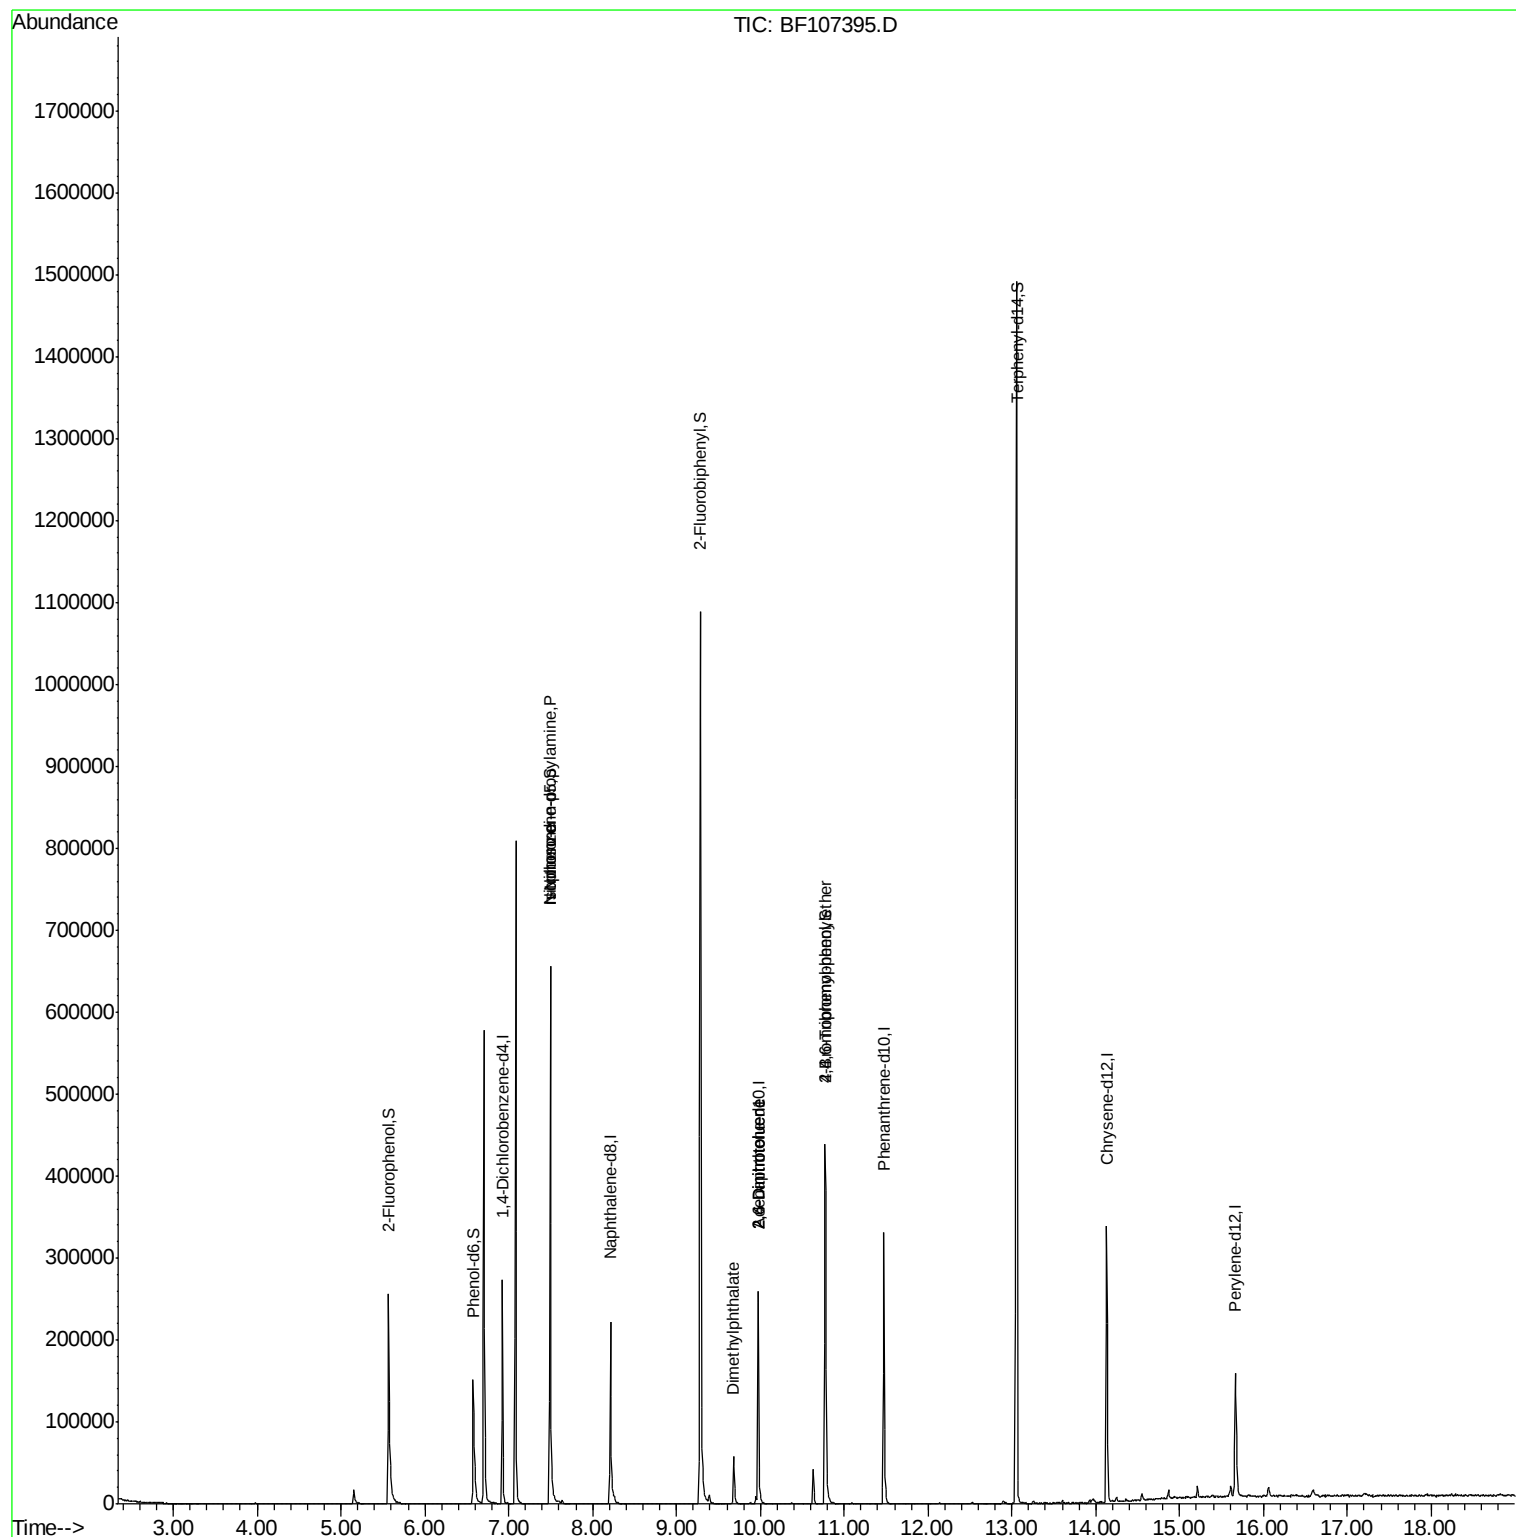


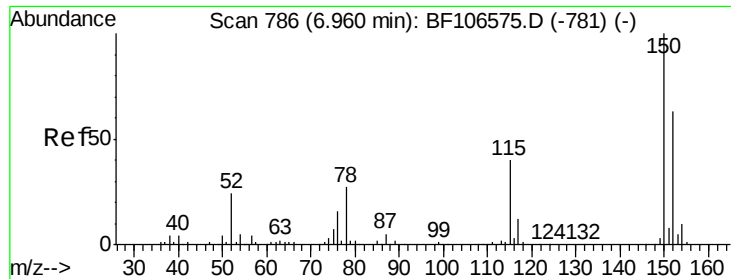




#1
 1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.92 min Scan# 780
 Delta R.T. -0.01 min
 Lab File: BF107395.D
 Acq: 14 Jul 2018 4:54

Instrument :
 BNA_F
 ClientSampleId :
 071118-TIPC-F-U-B

Tgt Ion:152 Resp: 40748
 Ion Ratio Lower Upper
 152 100
 150 159.7 124.6 186.8
 115 62.4 50.1 75.1

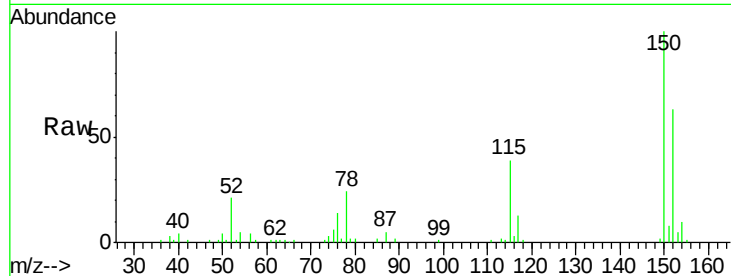


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

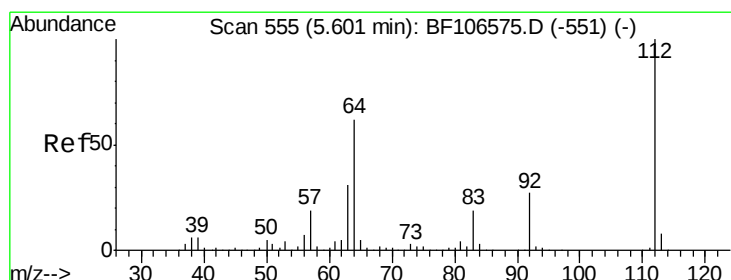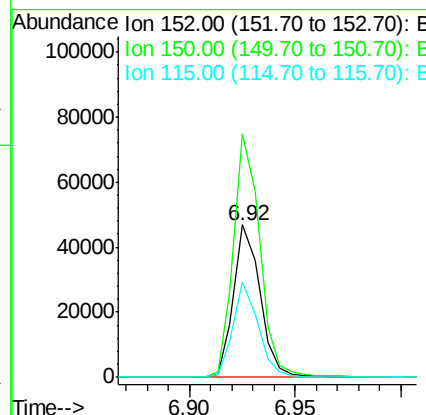
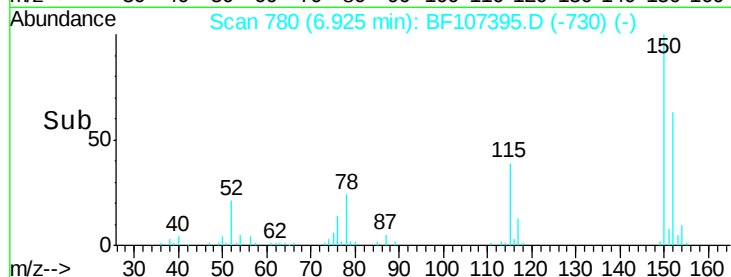



#5
 2-Fluorophenol
 Concen: 44.448 ng
 RT: 5.57 min Scan# 549
 Delta R.T. 0.00 min
 Lab File: BF107395.D
 Acq: 14 Jul 2018 4:54

Tgt Ion:112 Resp: 106959
 Ion Ratio Lower Upper
 112 100
 64 60.5 47.9 71.9
 63 29.4 23.7 35.5



Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BF1
 Ion 63.00 (62.70 to 63.70): BF1

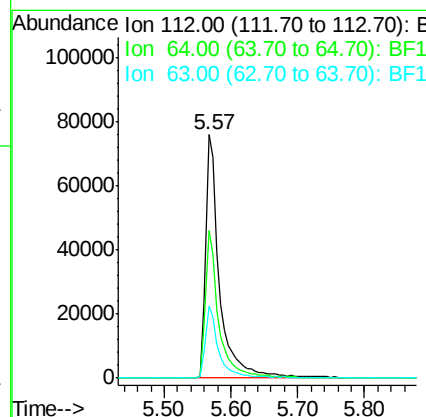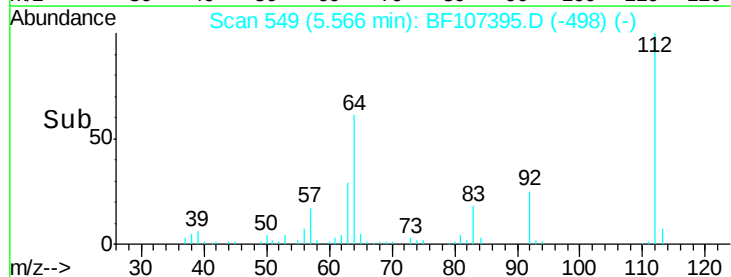

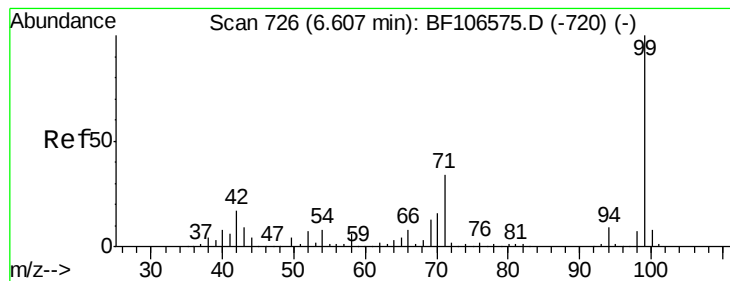

#7

Phenol-d6

Concen: 25.204 ng

RT: 6.58 min Scan# 721

Delta R.T. 0.00 min

Lab File: BF107395.D

Acq: 14 Jul 2018 4:54

Instrument :

BNA_F

ClientSampleId :

071118-TIPC-F-U-B


Tgt Ion: 99 Resp: 75740

Ion Ratio Lower Upper

99 100

42 17.4 14.5 21.7




71 32.5 25.4 38.0

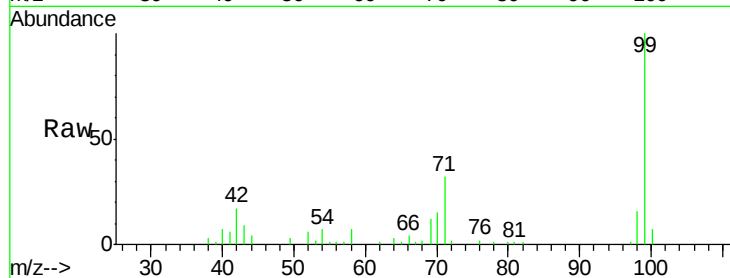

Abundance Ion 99.00 (98.70 to 99.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 71.00 (70.70 to 71.70): BF1

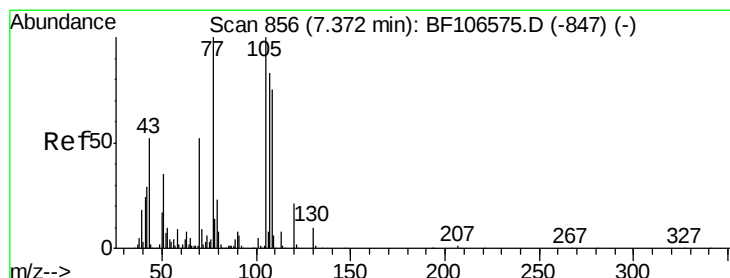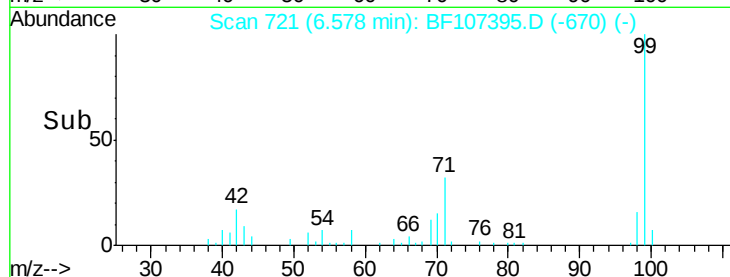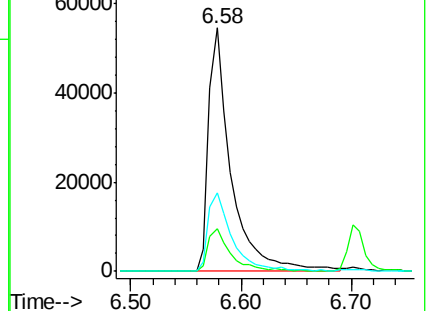

#19

n-Nitroso-di-n-propylamine

Concen: 14.911 ng

RT: 7.50 min Scan# 877

Delta R.T. 0.15 min

Lab File: BF107395.D

Acq: 14 Jul 2018 4:54

Tgt Ion: 70 Resp: 29538


Ion Ratio Lower Upper

70 100

42 41.4 47.5 71.3#

101 0.0 7.4 11.2#

130 2.4 16.6 25.0#


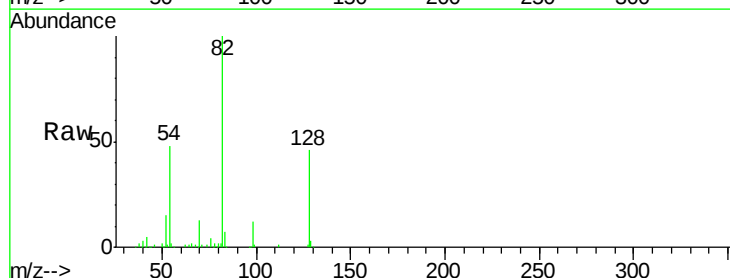



Abundance Ion 70.00 (69.70 to 70.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 101.00 (100.70 to 101.70): BF1

Ion 130.00 (129.70 to 130.70): BF1

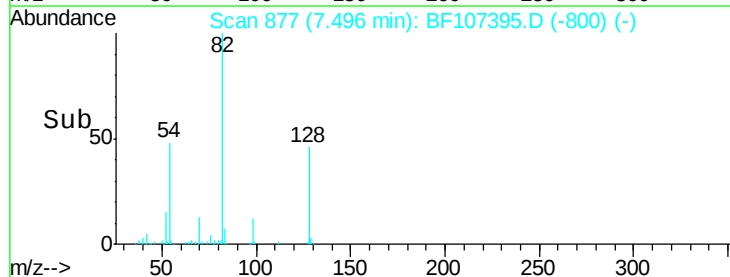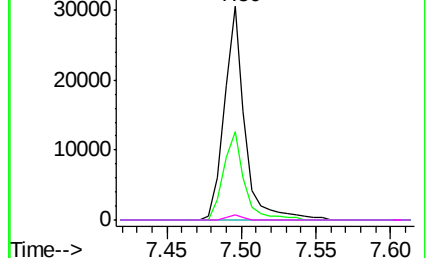


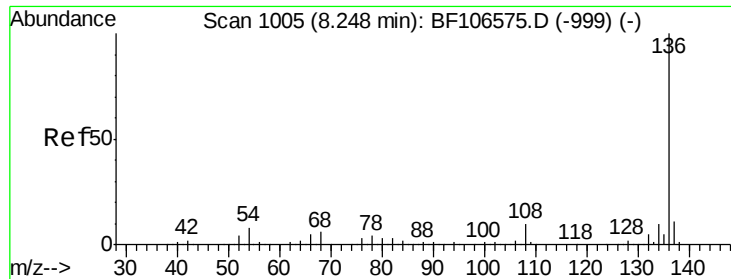




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.21 min Scan# 999
Delta R.T. 0.00 min
Lab File: BF107395.D
Acq: 14 Jul 2018 4:54

Instrument :
BNA_F
ClientSampleId :
071118-TIPC-F-U-B

Tgt Ion:	136	Resp:	138504
Ion	Ratio	Lower	Upper
136	100		
137	10.5	8.9	13.3
54	8.1	6.6	9.8
68	7.0	5.0	7.4




Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

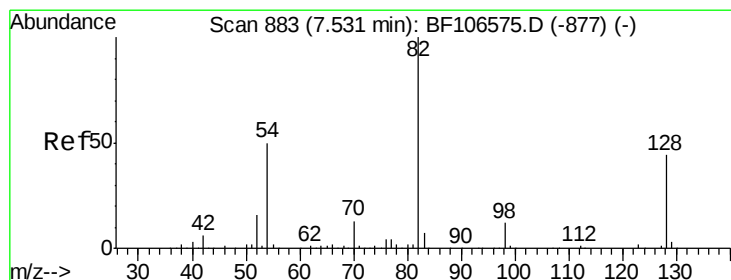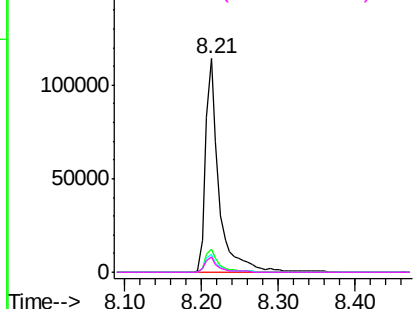
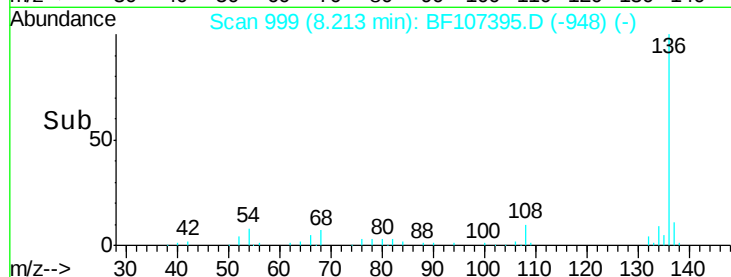



#23
Nitrobenzene-d5
Concen: 94.254 ng
RT: 7.50 min Scan# 877
Delta R.T. -0.01 min
Lab File: BF107395.D
Acq: 14 Jul 2018 4:54

Tgt Ion:	82	Resp:	234906
Ion	Ratio	Lower	Upper
82	100		
128	45.8	36.1	54.1
54	48.2	41.4	62.2



Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF1

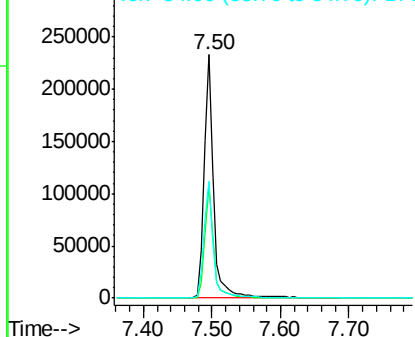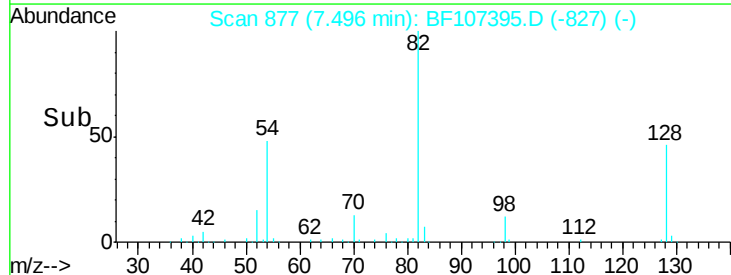

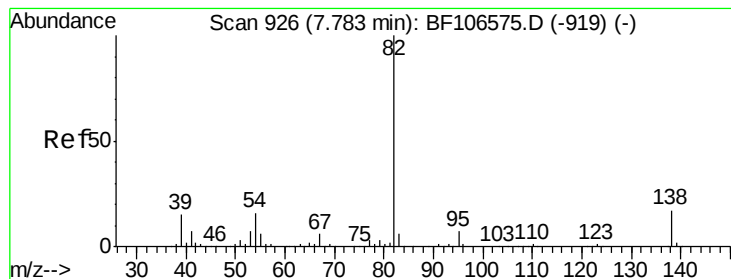

#25

Isophorone

Concen: 53.488 ng

RT: 7.50 min Scan# 877

Delta R.T. -0.26 min

Lab File: BF107395.D

Acq: 14 Jul 2018 4:54

Instrument :

BNA_F

ClientSampleId :

071118-TIPC-F-U-B


Tgt Ion: 82 Resp: 234904

Ion Ratio Lower Upper

82 100

95 0.0 5.2 7.8#




138 0.0 14.9 22.3#



Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 95.00 (94.70 to 95.70): BF1

Ion 138.00 (137.70 to 138.70): BF1

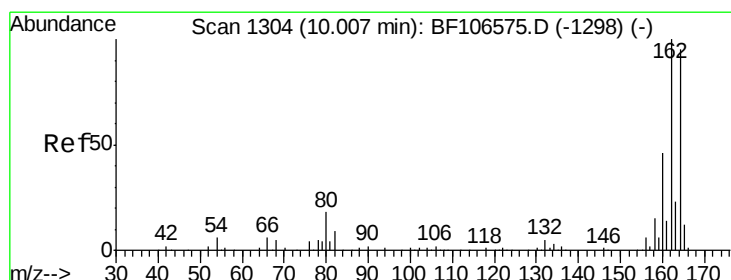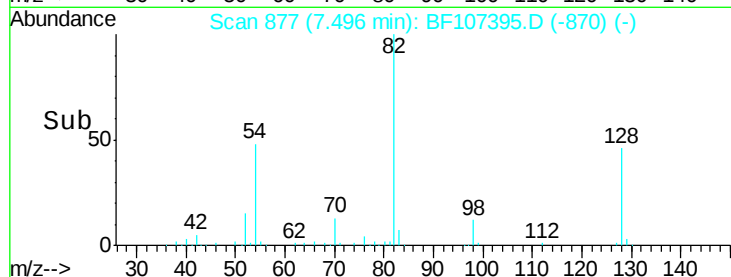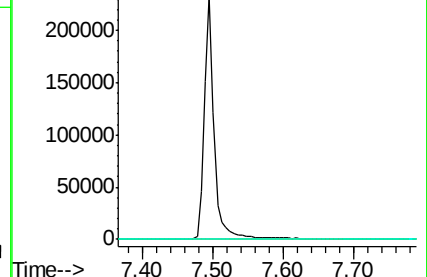

#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.98 min Scan# 1299

Delta R.T. 0.00 min

Lab File: BF107395.D

Acq: 14 Jul 2018 4:54


Tgt Ion: 164 Resp: 67471

Ion Ratio Lower Upper

164 100

162 99.1 86.1 129.1



160 44.2 38.3 57.5

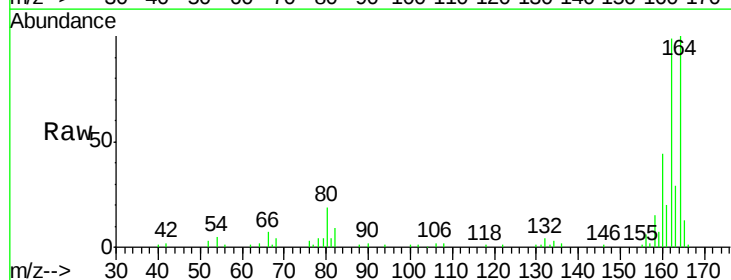


Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E



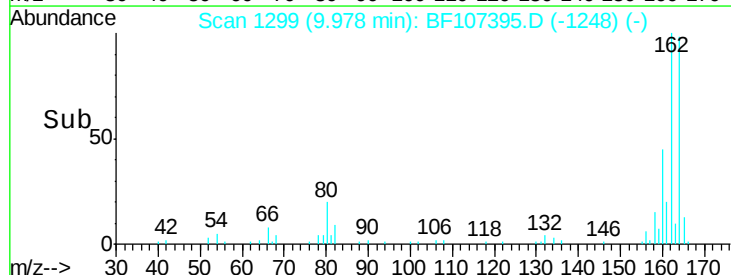
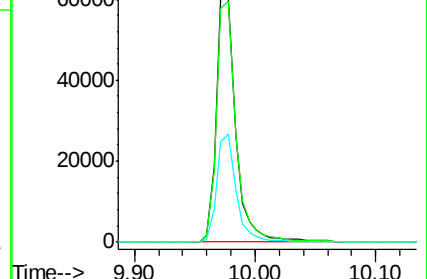


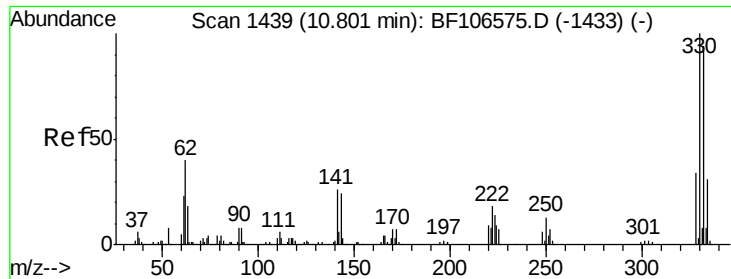

#41
 2,4,6-Tribromophenol
 Concen: 100.224 ng
 RT: 10.78 min Scan# 1435
 Delta R.T. 0.00 min
 Lab File: BF107395.D
 Acq: 14 Jul 2018 4:54




Instrument :
 BNA_F
 ClientSampleId :
 071118-TIPC-F-U-B


Tgt Ion:330 Resp: 78376
 Ion Ratio Lower Upper
 330 100
 332 96.6 77.0 115.6
 141 23.6 29.9 44.9#

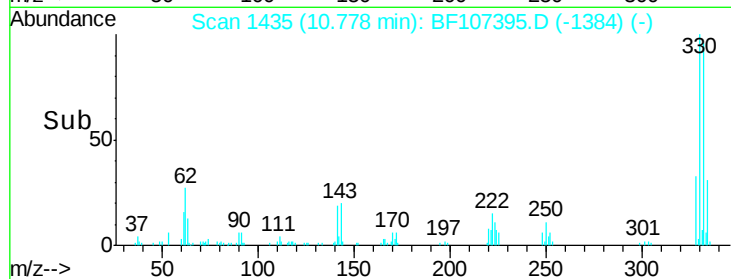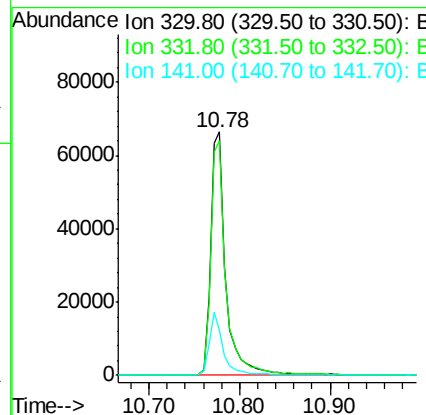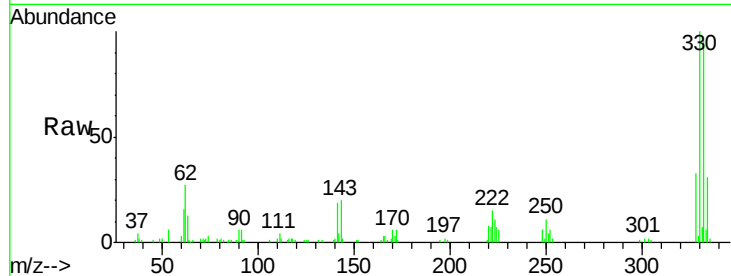

#44
 2-Fluorobiphenyl
 Concen: 111.001 ng
 RT: 9.28 min Scan# 1181
 Delta R.T. -0.01 min
 Lab File: BF107395.D
 Acq: 14 Jul 2018 4:54

Tgt Ion:172 Resp: 424483
 Ion Ratio Lower Upper
 172 100
 171 36.3 29.7 44.5
 170 24.2 19.6 29.4

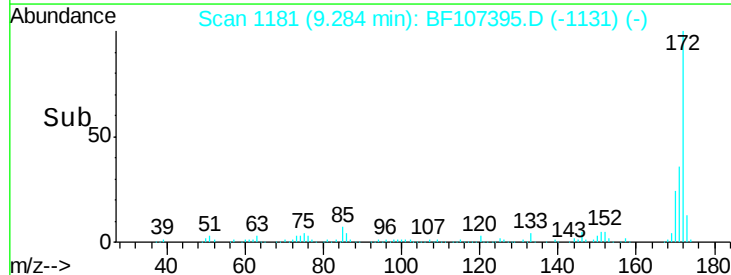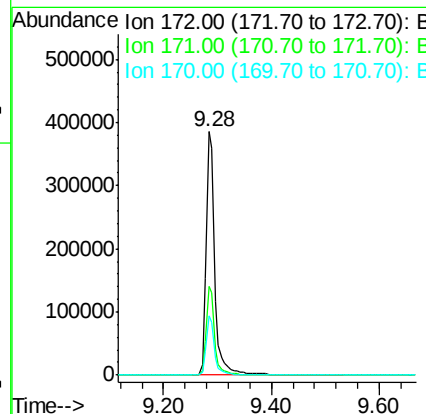

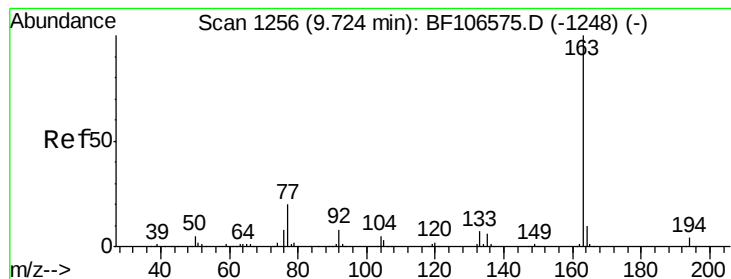

#49

Dimethylphthalate

Concen: 6.369 ng

RT: 9.68 min Scan# 1249

Delta R.T. -0.01 min

Lab File: BF107395.D

Acq: 14 Jul 2018 4:54

Instrument :

BNA_F

ClientSampleId :

071118-TIPC-F-U-B


Tgt Ion:163 Resp: 32232

Ion Ratio Lower Upper

163 100

194 3.6 2.7 4.1




164 10.8 8.2 12.2



Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

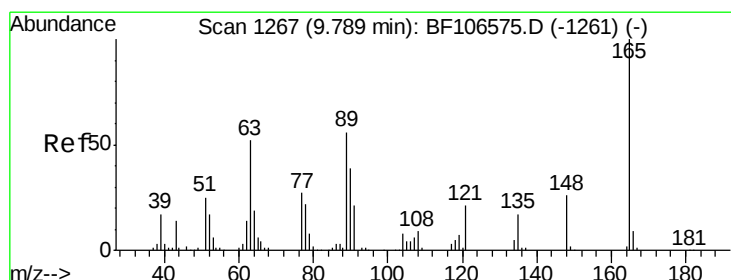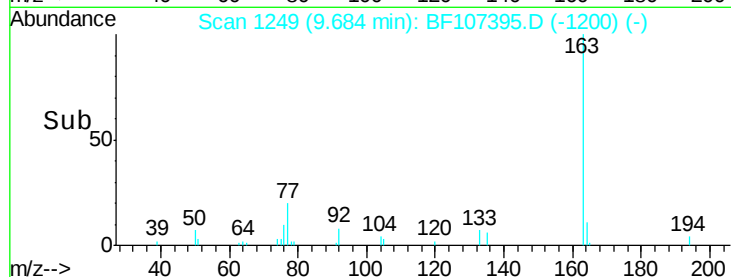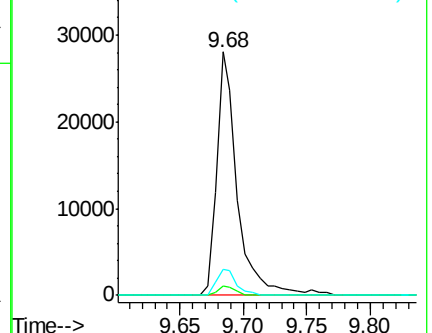

#50

2,6-Dinitrotoluene

Concen: 7.943 ng

RT: 9.98 min Scan# 1299

Delta R.T. 0.21 min

Lab File: BF107395.D

Acq: 14 Jul 2018 4:54


Tgt Ion:165 Resp: 8511

Ion Ratio Lower Upper

165 100

63 0.0 44.7 67.1#



89 0.0 44.0 66.0#




Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF1

Ion 89.00 (88.70 to 89.70): BF1



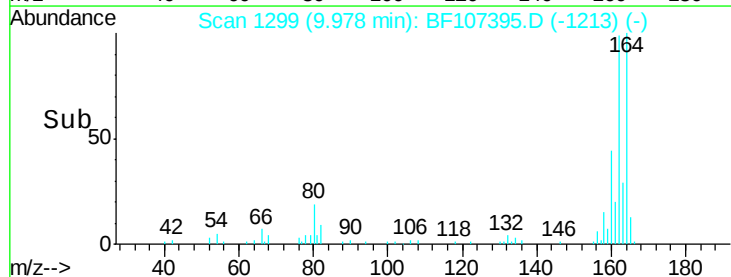
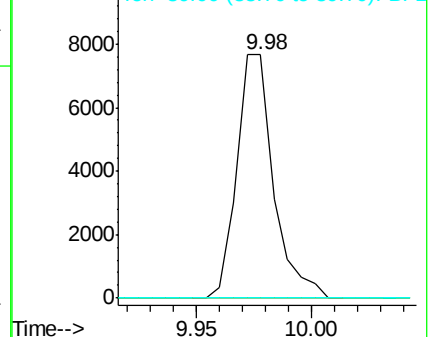


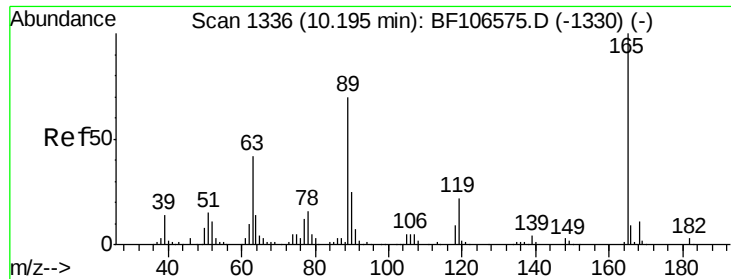

#56
 2,4-Dinitrotoluene
 Concen: 6.085 ng
 RT: 9.98 min Scan# 1299
 Delta R.T. -0.21 min
 Lab File: BF107395.D
 Acq: 14 Jul 2018 4:54




Instrument :
 BNA_F
 ClientSampleId :
 071118-TIPC-F-U-B


Tgt Ion:	165	Resp:	8511
Ion	Ratio	Lower	Upper
165	100		
63	0.0	36.4	54.6#
89	0.0	57.8	86.6#
182	0.0	1.6	2.4#

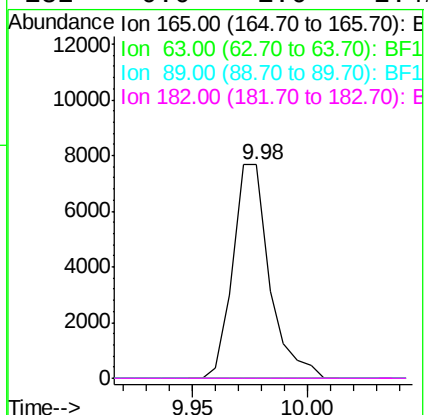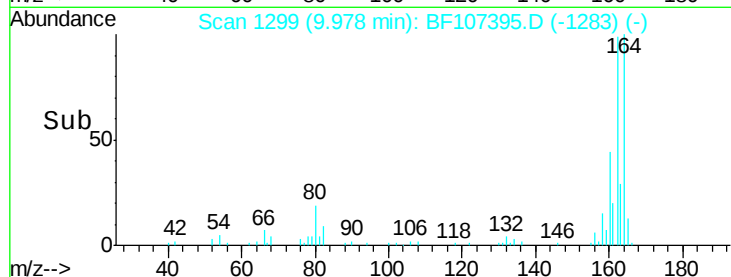

#63
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 11.47 min Scan# 1553
 Delta R.T. -0.01 min
 Lab File: BF107395.D
 Acq: 14 Jul 2018 4:54

Tgt Ion:	188	Resp:	145504
Ion	Ratio	Lower	Upper
188	100		
94	8.9	8.5	12.7
80	9.6	9.2	13.8

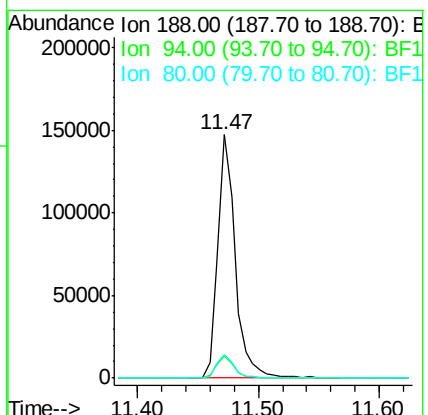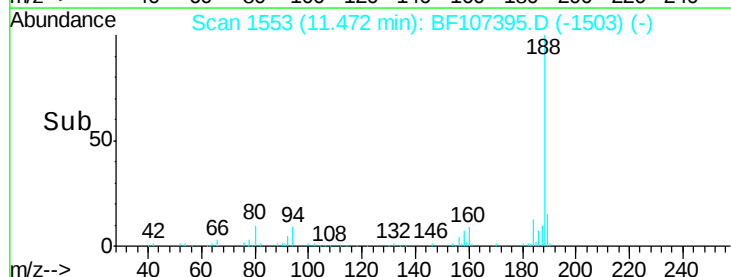


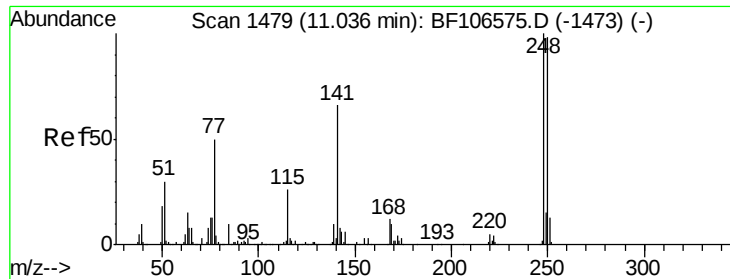




#66
4-Bromophenyl-phenylether
Concen: 2.641 ng
RT: 10.77 min Scan# 1434
Delta R.T. -0.24 min
Lab File: BF107395.D
Acq: 14 Jul 2018 4:54

Instrument :
BNA_F
ClientSampleId :
071118-TIPC-F-U-B

Tgt Ion:248 Resp: 4586
Ion Ratio Lower Upper
248 100
250 195.2 76.9 115.3#
141 412.8 74.4 111.6#

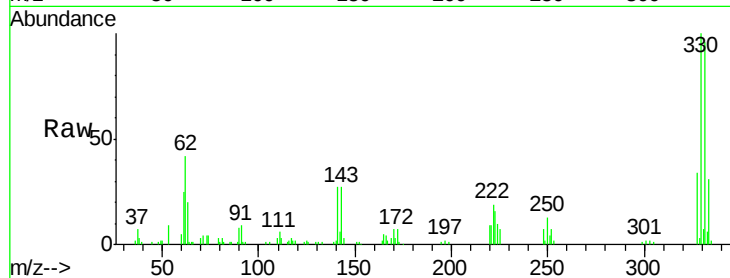


Abundance Ion 248.00 (247.70 to 248.70): E
Ion 250.00 (249.70 to 250.70): E
Ion 141.00 (140.70 to 141.70): E

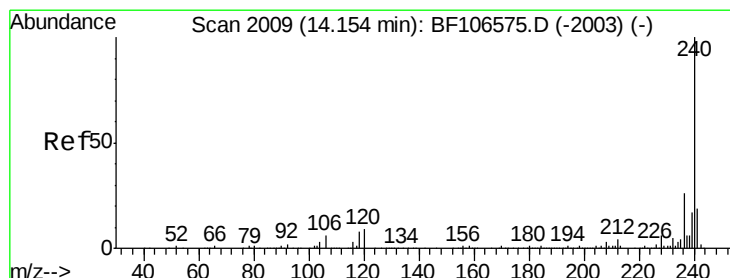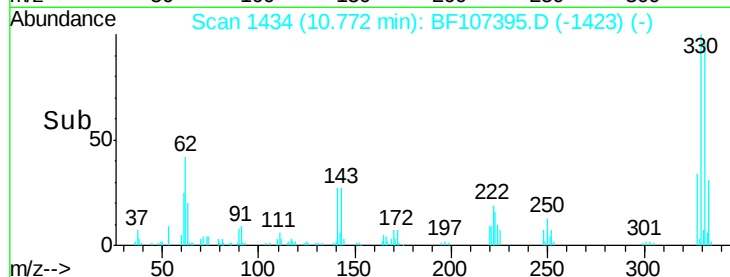
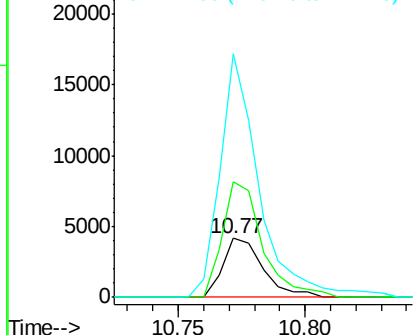



#75
Chrysene-d12
Concen: 20.000 ng
RT: 14.13 min Scan# 2005
Delta R.T. -0.01 min
Lab File: BF107395.D
Acq: 14 Jul 2018 4:54

Tgt Ion:240 Resp: 135563
Ion Ratio Lower Upper
240 100
120 9.6 9.5 14.3
236 24.9 20.7 31.1

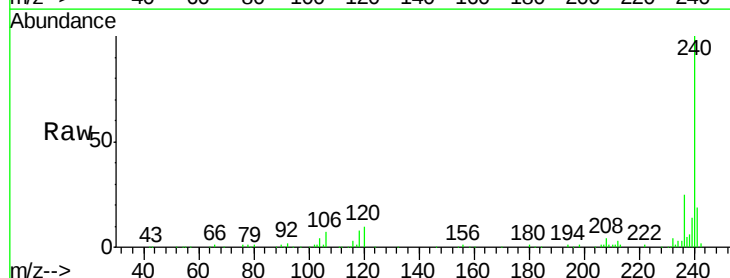

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

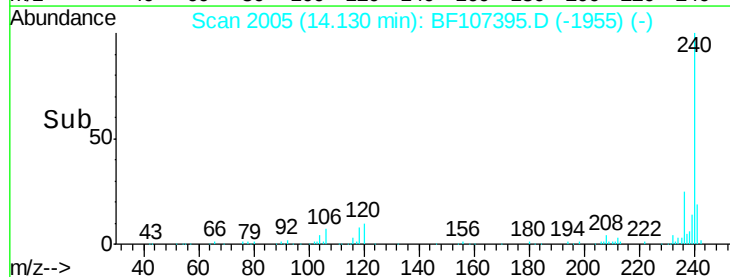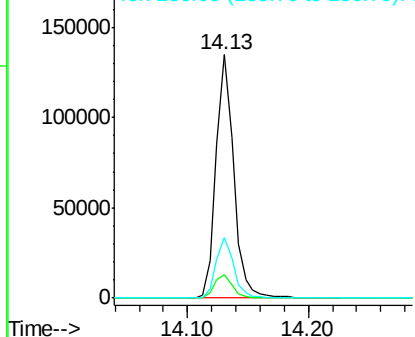

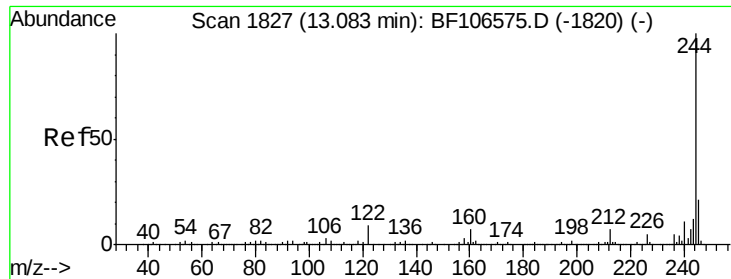

#78

Terphenyl-d14

Concen: 114.009 ng

RT: 13.06 min Scan# 1823

Delta R.T. 0.00 min

Lab File: BF107395.D

Acq: 14 Jul 2018 4:54

Instrument :

BNA_F

ClientSampleId :

071118-TIPC-F-U-B


Tgt Ion:244 Resp: 638046

Ion Ratio Lower Upper

244 100

212 6.6 5.4 8.0




122 8.0 11.0 16.4#

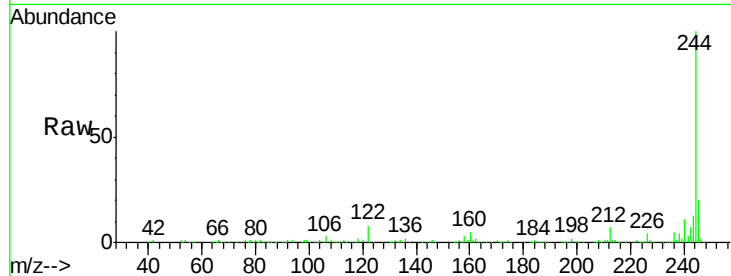

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

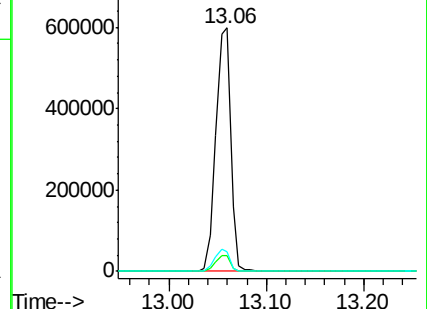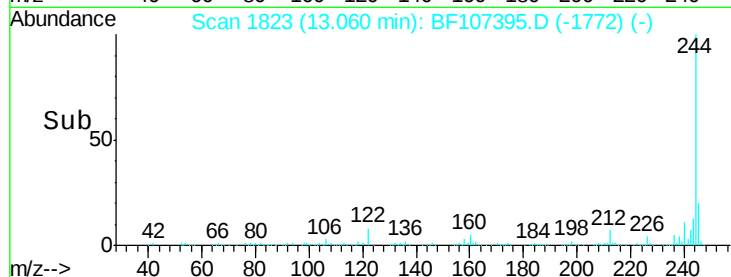

#86

Perylene-d12

Concen: 20.000 ng

RT: 15.67 min Scan# 2266

Delta R.T. 0.00 min

Lab File: BF107395.D

Acq: 14 Jul 2018 4:54


Tgt Ion:264 Resp: 93909

Ion Ratio Lower Upper

264 100

260 22.8 19.2 28.8

265 20.1 17.5 26.3



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

