
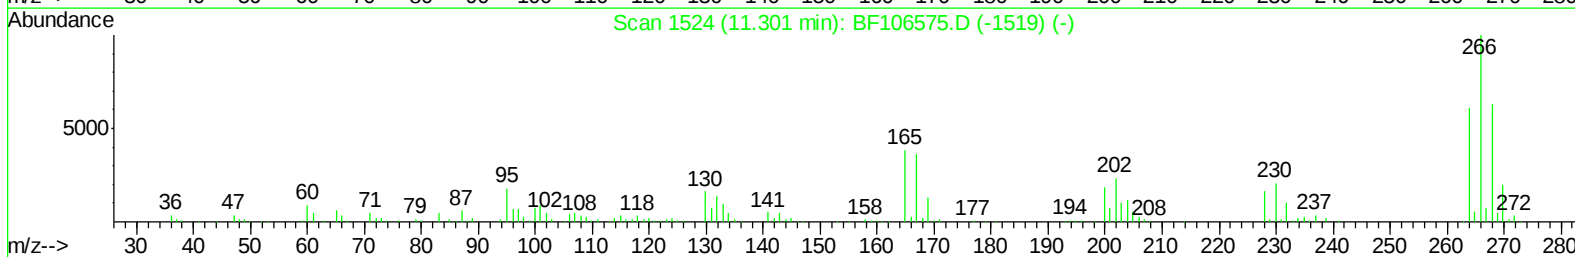
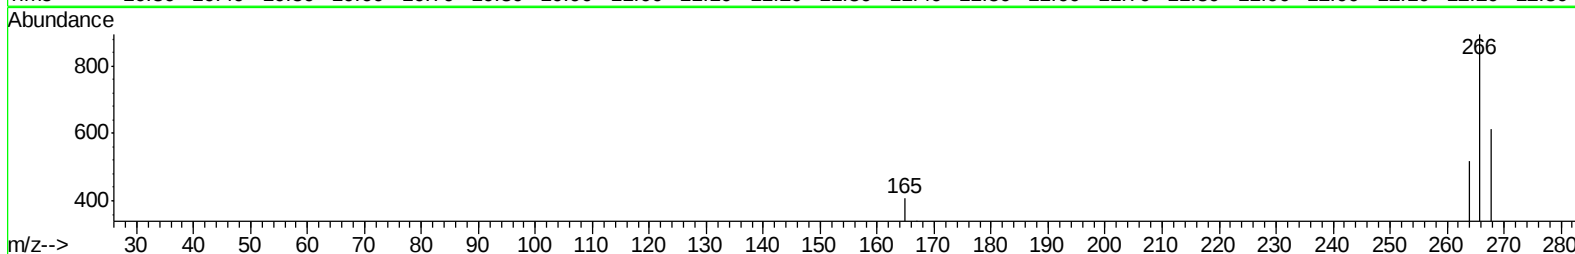


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071318\
Data File : BF107378.D
Acq On : 13 Jul 2018 21:02
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 16 02:01:11 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 13 11:54:53 2018
Response via : Initial Calibration

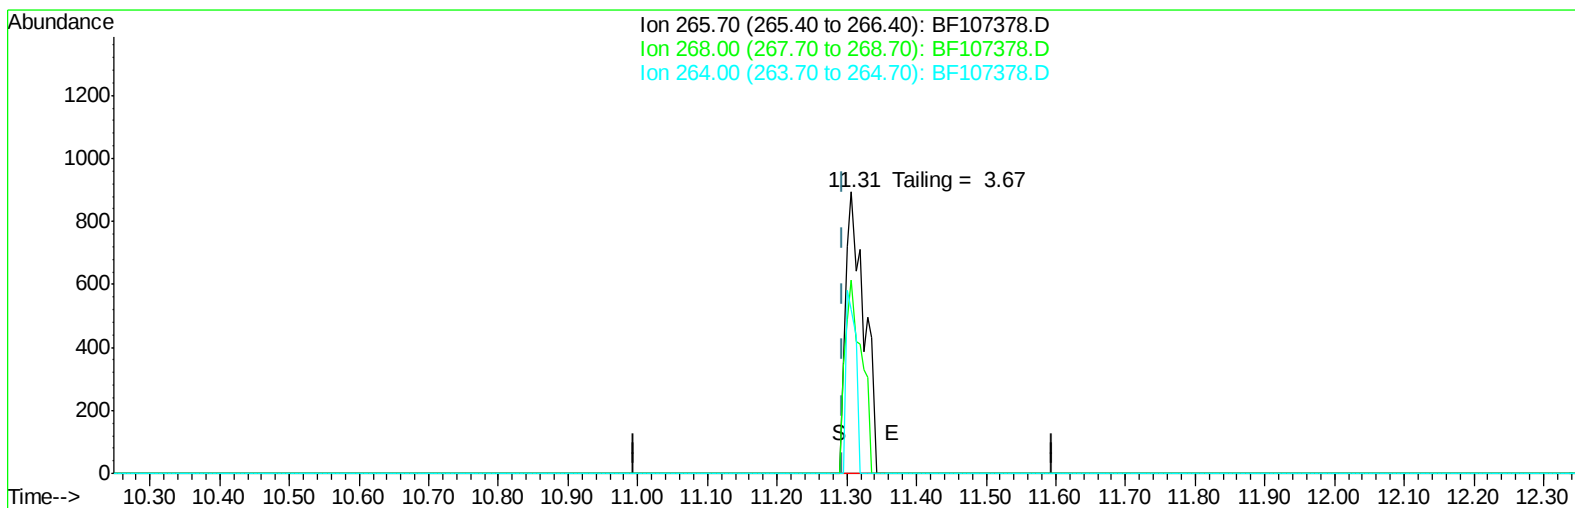

TIC: BF107378.D

(69) Pentachlorophenol (C)




11.307min (+0.012) 0.00ng m

response 1634

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	68.46
264.00	61.90	58.05
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071318\
 Data File : BF107378.D
 Acq On : 13 Jul 2018 21:02
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 16 02:01:11 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 13 11:54:53 2018
 Response via : Initial Calibration

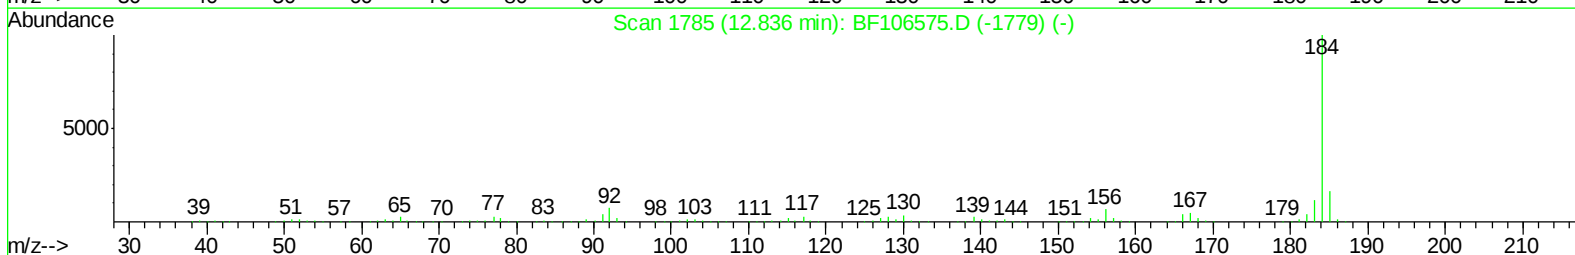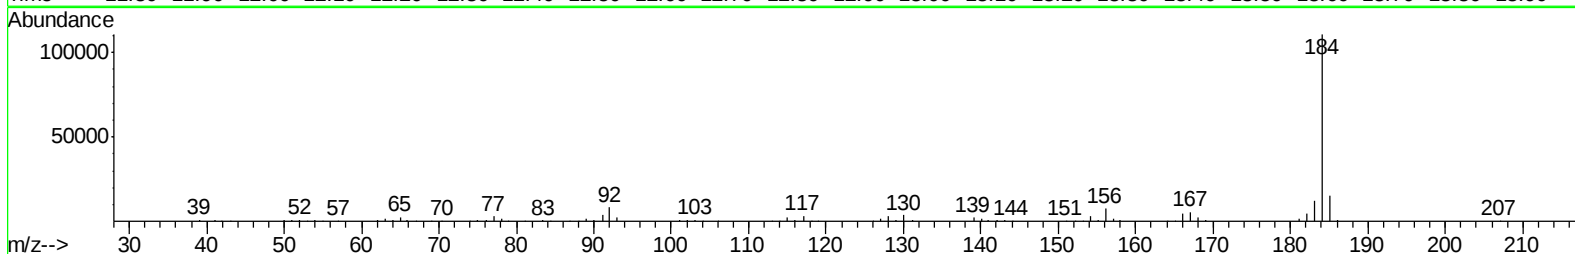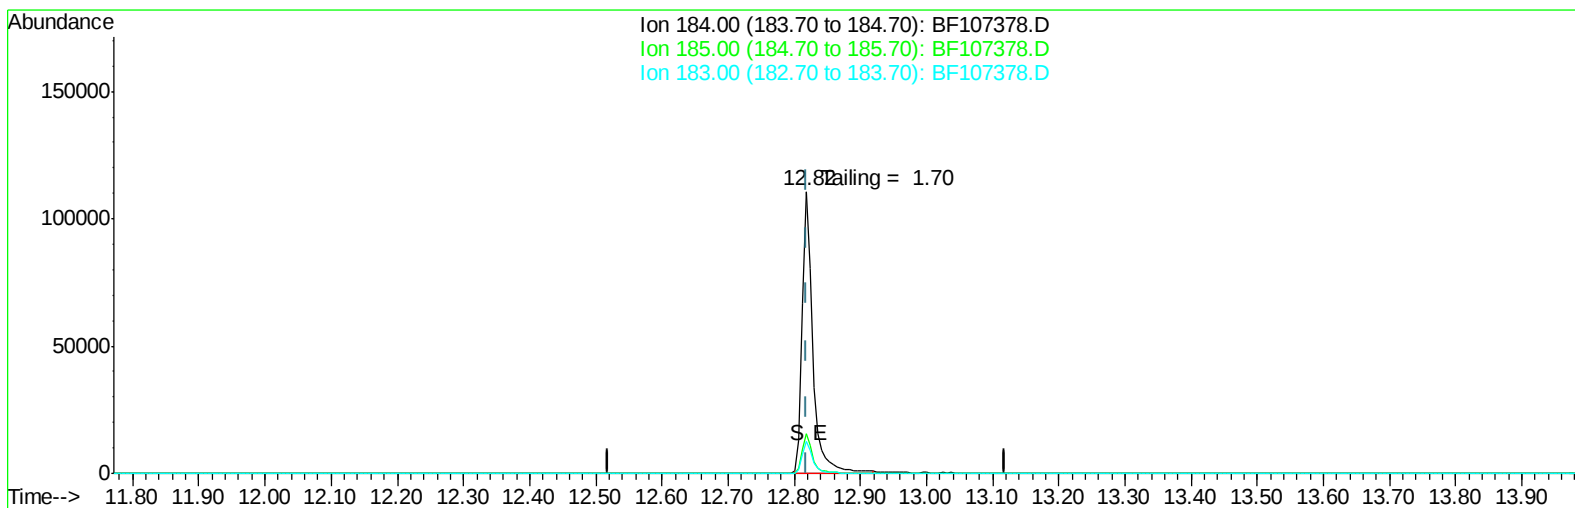

TIC: BF107378.D

(76) Benzidine

12.818min (-0.000) 0.00ng

response 127609

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	13.90
183.00	11.60	11.34
0.00	0.00	0.00