


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF071318\  
 Data File : BF107378.D  
 Acq On : 13 Jul 2018 21:02  
 Operator : JU/SJ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF061918.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Fri Jul 13 11:54:53 2018

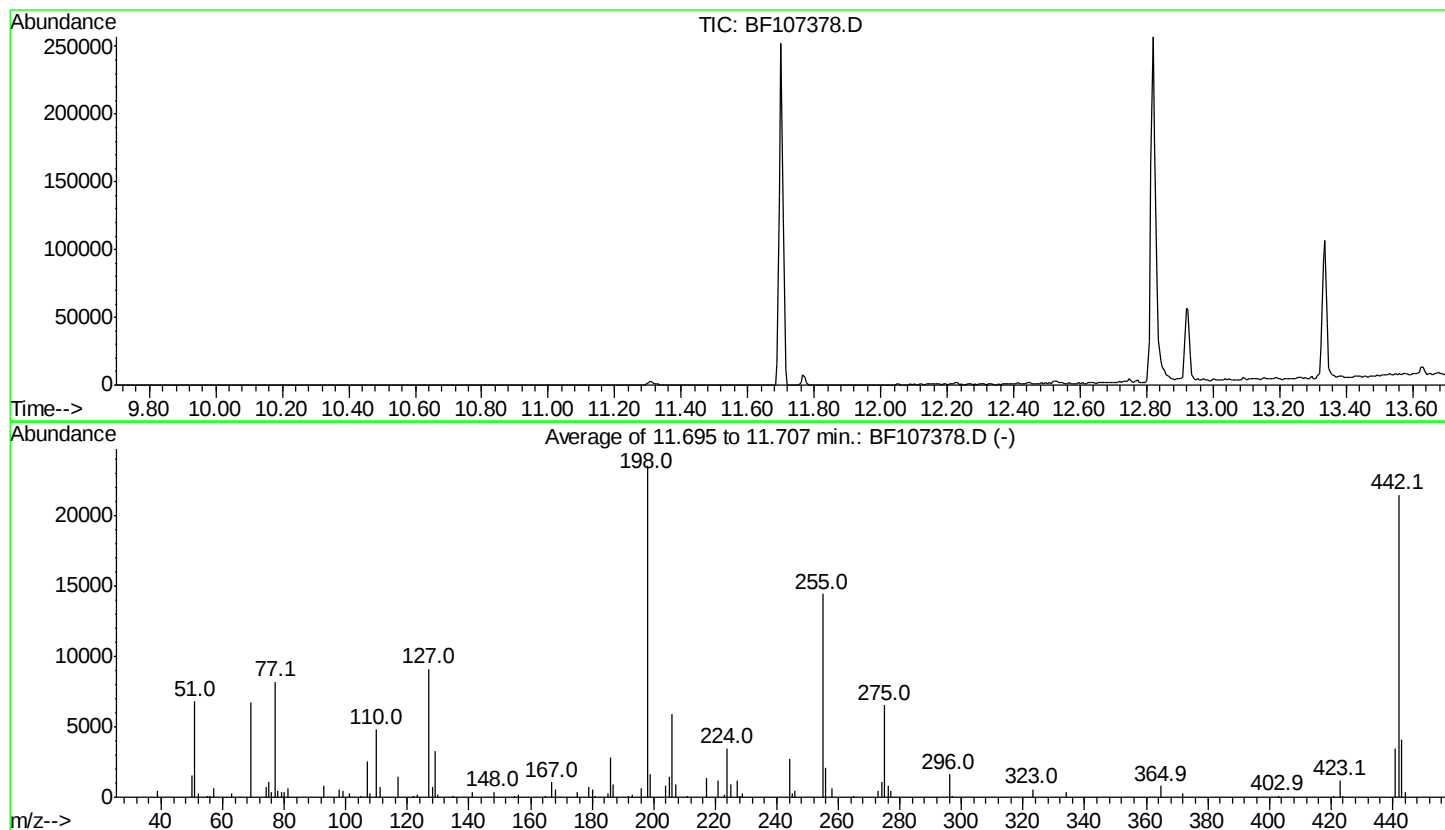

AutoFind: Scans 1591, 1592, 1593; Background Corrected with Scan 1587

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 28.9      | 6794    | PASS             |
| 68          | 69           | 0.00         | 2            | 0.0       | 0       | PASS             |
| 69          | 198          | 0.00         | 100          | 28.6      | 6725    | PASS             |
| 70          | 69           | 0.00         | 2            | 0.0       | 0       | PASS             |
| 127         | 198          | 10           | 80           | 38.8      | 9116    | PASS             |
| 197         | 198          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 23514   | PASS             |
| 199         | 198          | 5            | 9            | 6.9       | 1614    | PASS             |
| 275         | 198          | 10           | 60           | 27.6      | 6498    | PASS             |
| 365         | 198          | 1            | 100          | 3.3       | 781     | PASS             |
| 441         | 198          | 0.01         | 100          | 14.8      | 3479    | PASS             |
| 442         | 198          | 50           | 100          | 91.2      | 21439   | PASS             |
| 443         | 442          | 15           | 24           | 19.1      | 4087    | PASS             |