


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071320\
 Data File : BF120849.D
 Acq On : 13 Jul 2020 9:36
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070220.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 02 18:51:52 2020

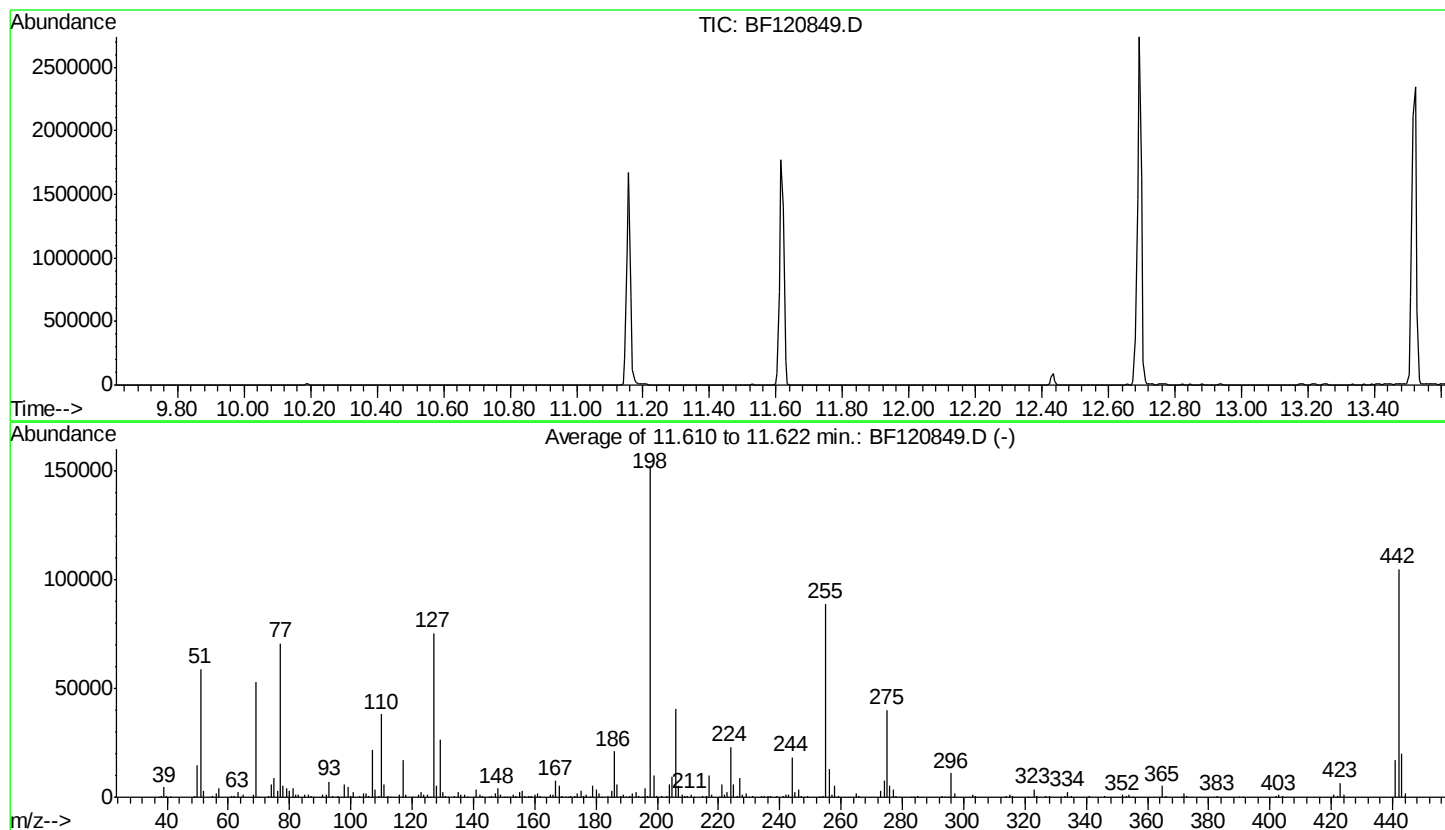

AutoFind: Scans 1619, 1620, 1621; Background Corrected with Scan 1614

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.7	58885	PASS
68	69	0.00	2	1.9	1007	PASS
69	198	0.00	100	34.9	53162	PASS
70	69	0.00	2	0.3	178	PASS
127	198	10	80	49.5	75306	PASS
197	198	0.00	2	0.5	778	PASS
198	198	100	100	100.0	152176	PASS
199	198	5	9	6.7	10137	PASS
275	198	10	60	26.3	39992	PASS
365	198	1	100	3.4	5136	PASS
441	198	0.01	100	11.1	16820	PASS
442	198	50	100	68.8	104757	PASS
443	442	15	24	19.0	19880	PASS