
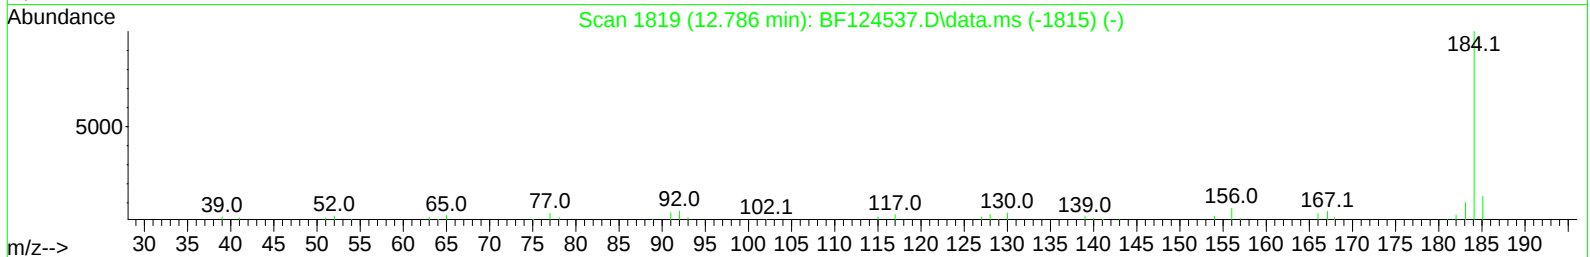
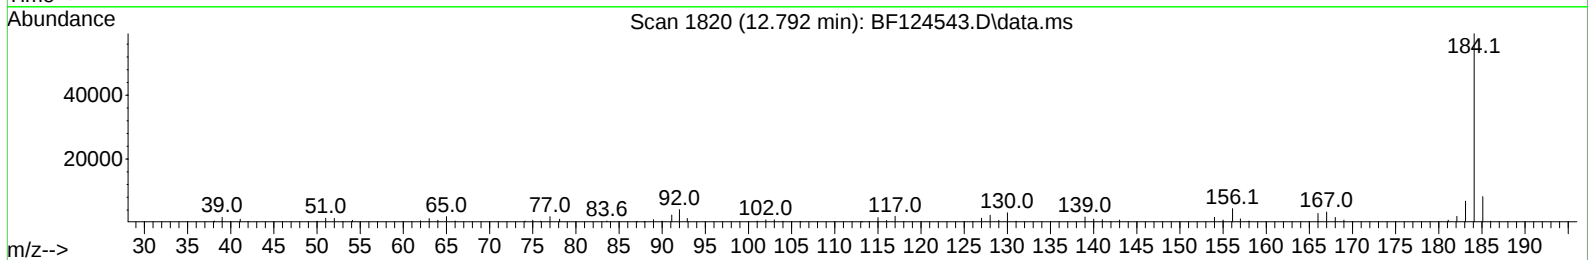


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071321\
 Data File : BF124543.D
 Acq On : 13 Jul 2021 11:44
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 13 12:50:57 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 08 07:49:42 2021
 Response via : Initial Calibration

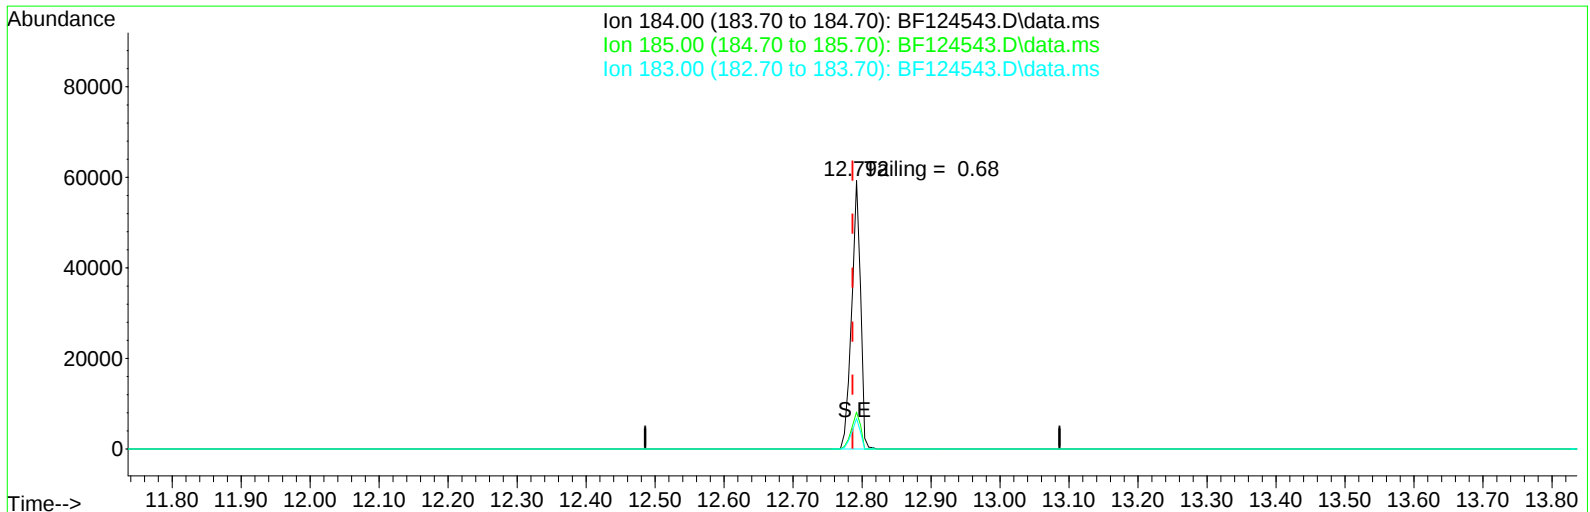

TIC: BF124543.D\data.ms

(77) Benzidine




12.792min (+ 0.006) 0.00 ng

response 53320

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	13.80
183.00	10.10	11.43
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071321\
Data File : BF124543.D
Acq On : 13 Jul 2021 11:44
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 13 12:50:57 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 08 07:49:42 2021
Response via : Initial Calibration

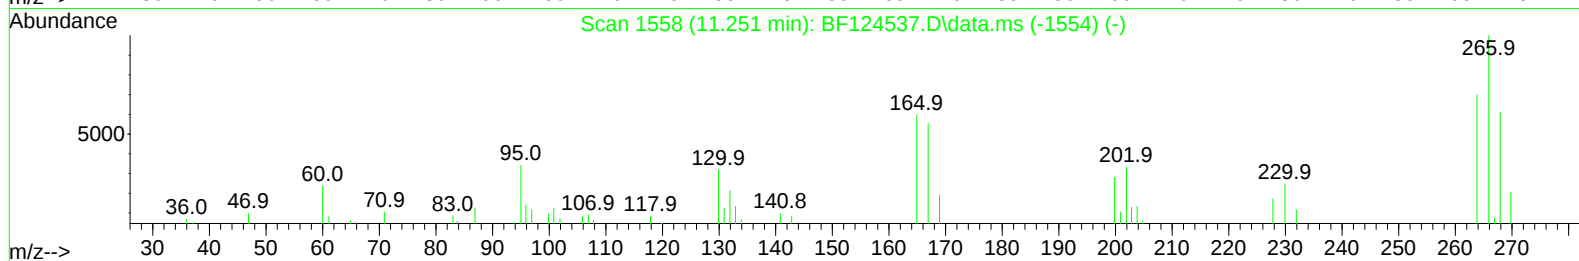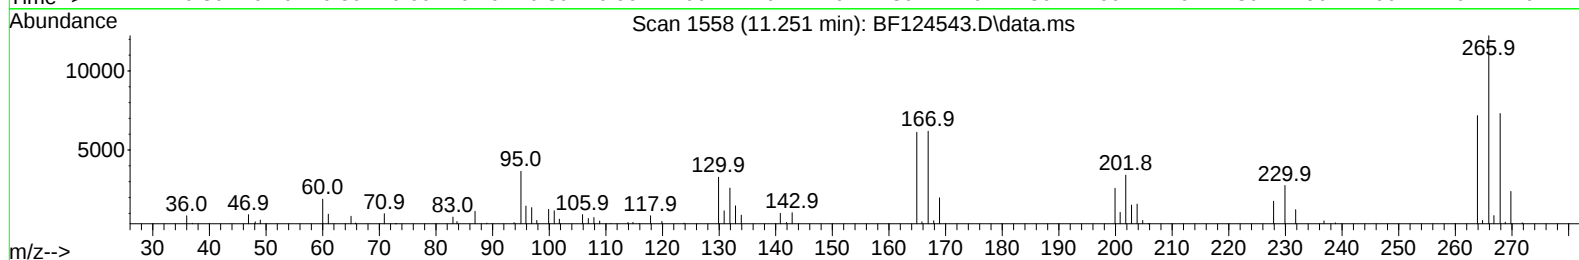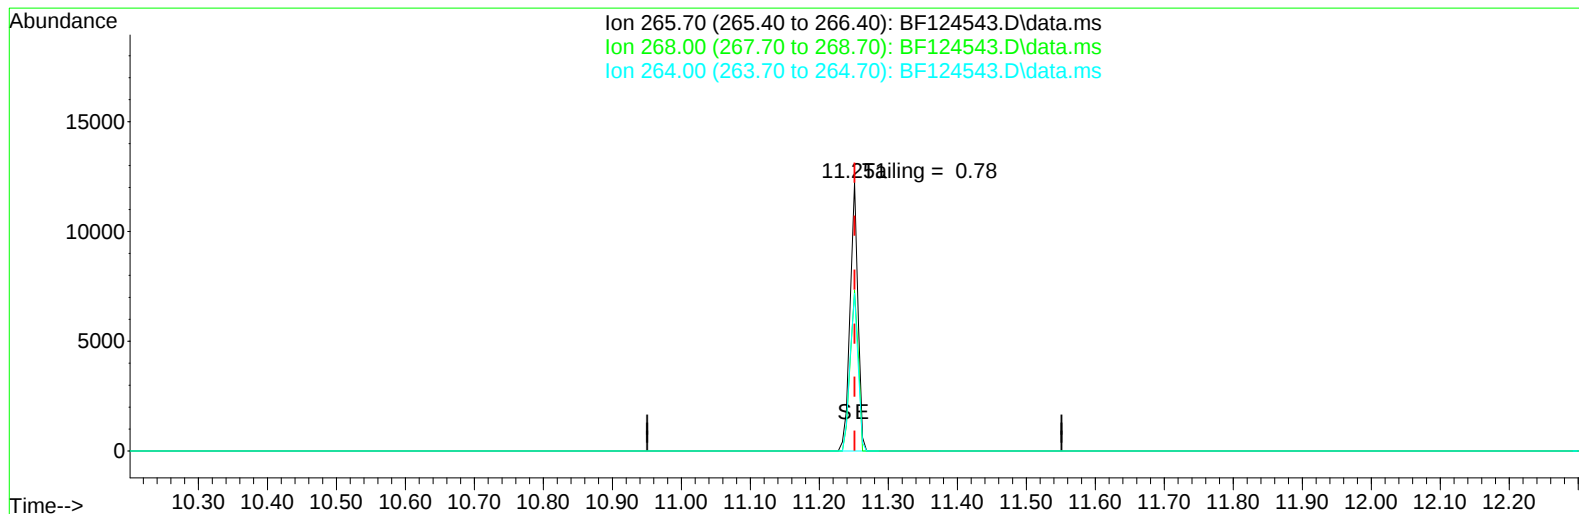

TIC: BF124543.D\data.ms

(70) Pentachlorophenol (C)

11.251min (+ 0.000) 0.00 ng

response 9783

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	59.80
264.00	69.90	58.71
0.00	0.00	0.00