

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071321\
Data File : BF124545.D
Acq On : 13 Jul 2021 14:03
Operator : JU/CG
Sample : PB137642BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB137642BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070721.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF124545.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.563	585	591	594	rBB	211264	228599	66.44%	12.497%
2	6.551	752	759	761	rBB	180423	232576	67.60%	12.715%
3	6.928	819	823	825	rBB	49711	44644	12.98%	2.441%
4	7.486	912	918	921	rBB	125361	152076	44.20%	8.314%
5	8.204	1036	1040	1044	rBB	66100	65312	18.98%	3.571%
6	9.286	1218	1224	1227	rBB	289666	308685	89.72%	16.876%
7	9.963	1334	1339	1342	rBB	80159	75776	22.02%	4.143%
8	10.757	1468	1474	1477	rBB	198575	185688	53.97%	10.152%
9	11.451	1588	1592	1596	rBB	91850	79075	22.98%	4.323%
10	13.051	1858	1864	1867	rBV	336347	344047	100.00%	18.809%
11	14.092	2038	2041	2045	rBB	72276	63356	18.41%	3.464%
12	15.592	2291	2296	2300	rBB2	41860	49325	14.34%	2.697%




Sum of corrected areas: 1829159

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071321\
Data File : BF124545.D
Acq On : 13 Jul 2021 14:03
Operator : JU/CG
Sample : PB137642BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB137642BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

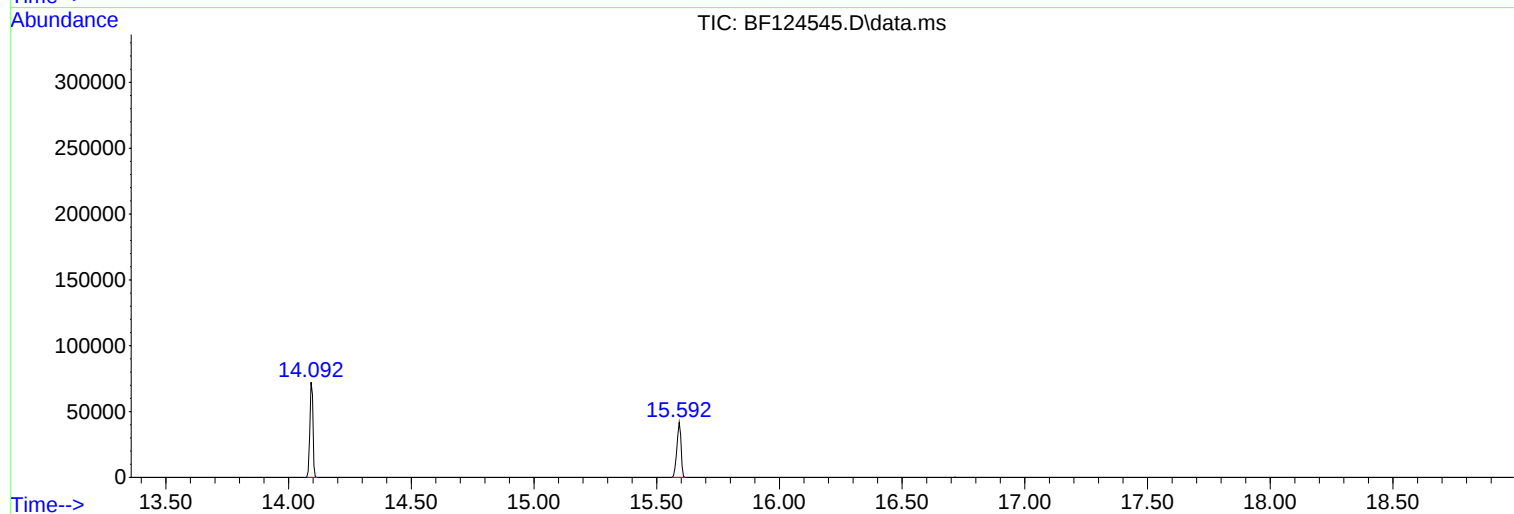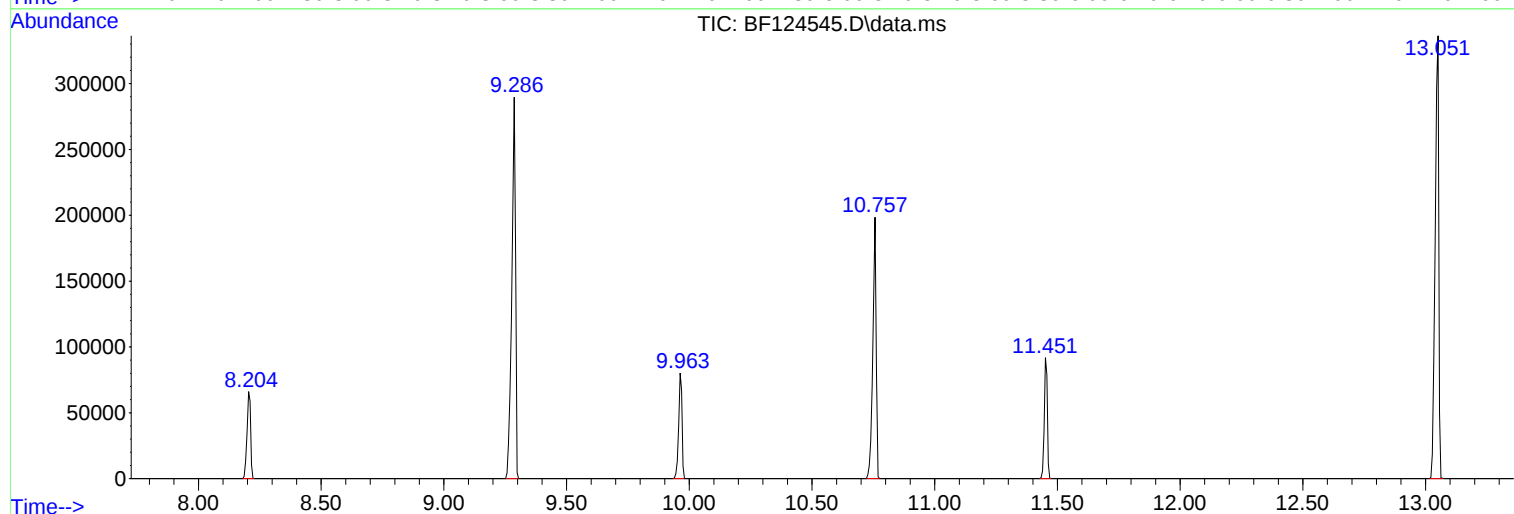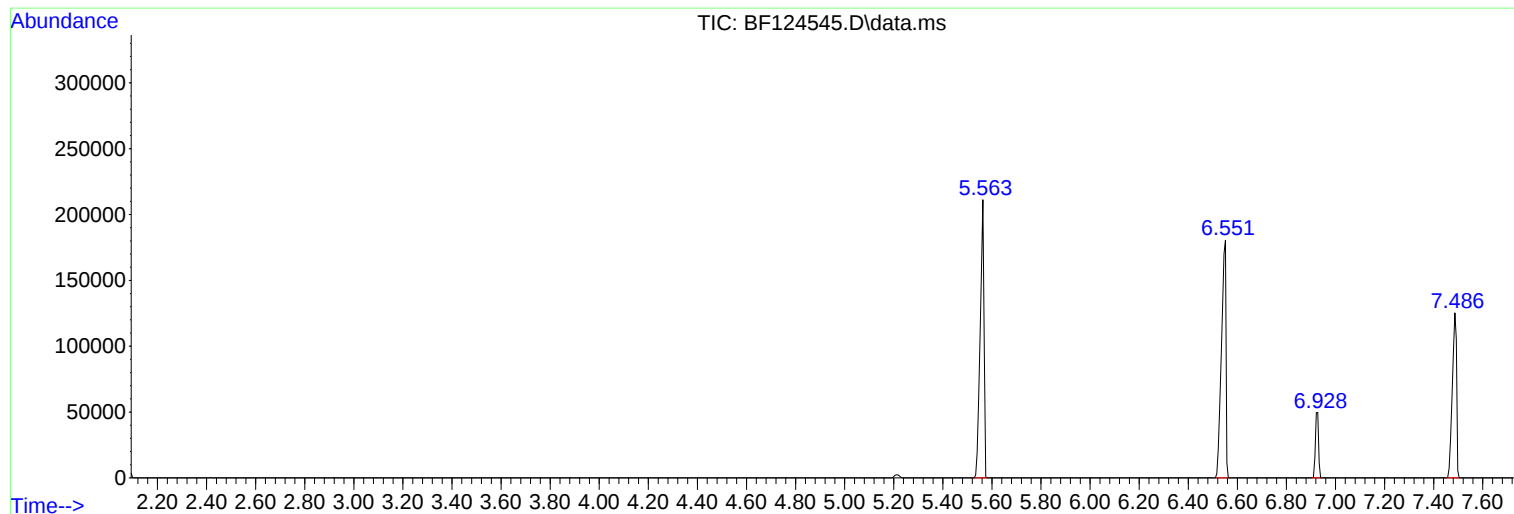

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071321\
Data File : BF124545.D
Acq On : 13 Jul 2021 14:03
Operator : JU/CG
Sample : PB137642BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB137642BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071321\
Data File : BF124545.D
Acq On : 13 Jul 2021 14:03
Operator : JU/CG
Sample : PB137642BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB137642BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------