
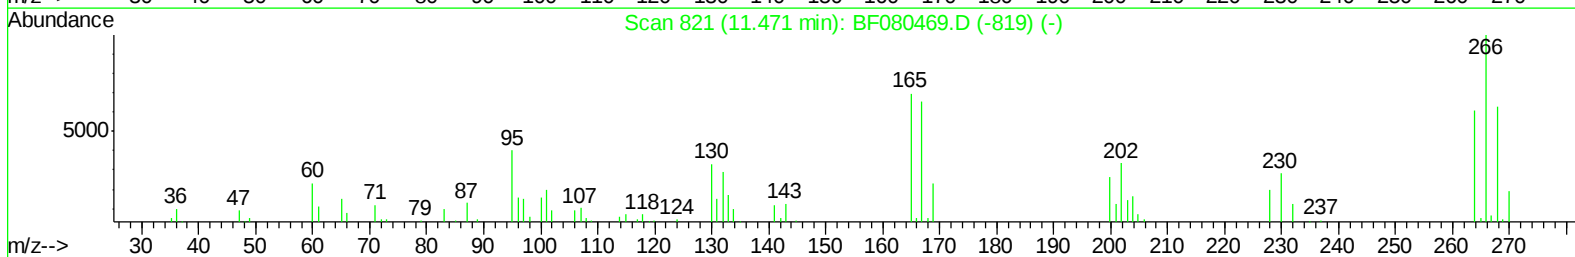
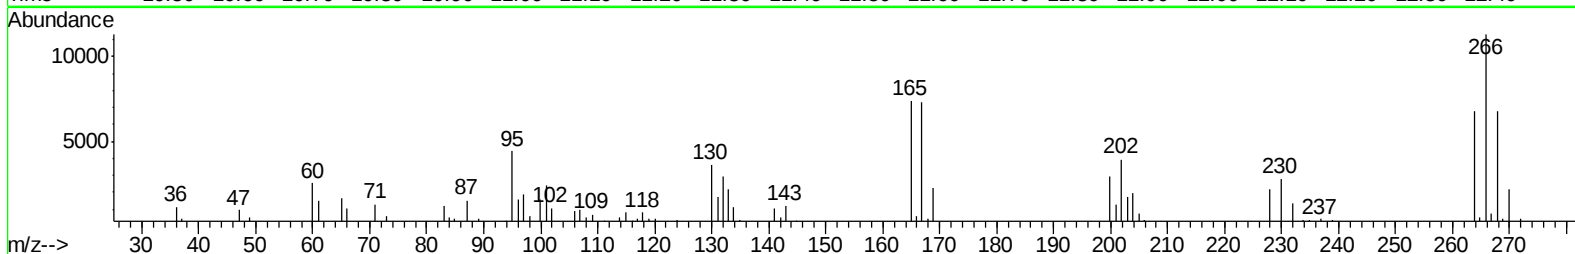


Data Path : Z:\HPCHEM1\BNA_F\Data\BF071415\
Data File : BF080465.D
Acq On : 14 Jul 2015 15:18
Operator : TP/UM
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 15 08:56:10 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF071415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 15 03:58:42 2015
Response via : Initial Calibration

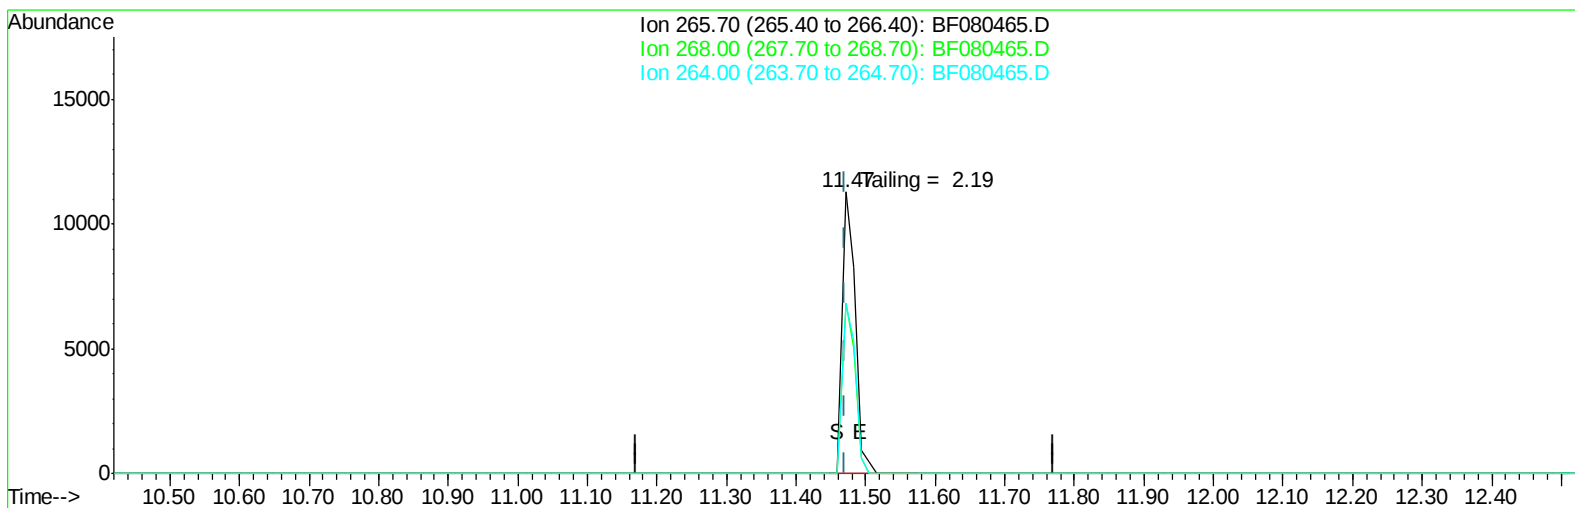

TIC: BF080465.D

(69) Pentachlorophenol (C)




11.471min (+0.001) 0.00ng m

response 14341

Ion	Exp%	Act%
265.70	100	100
268.00	62.90	60.31
264.00	60.70	60.13
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF071415\
Data File : BF080465.D
Acq On : 14 Jul 2015 15:18
Operator : TP/UM
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 15 08:56:10 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF071415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 15 03:58:42 2015
Response via : Initial Calibration

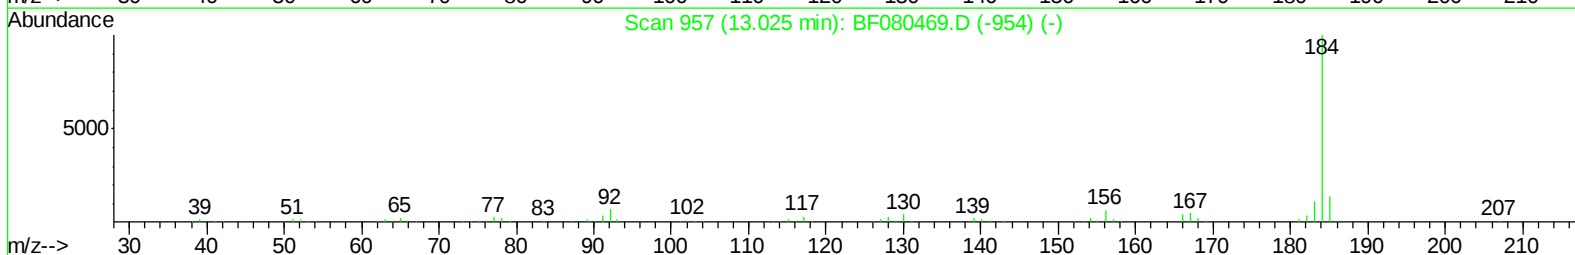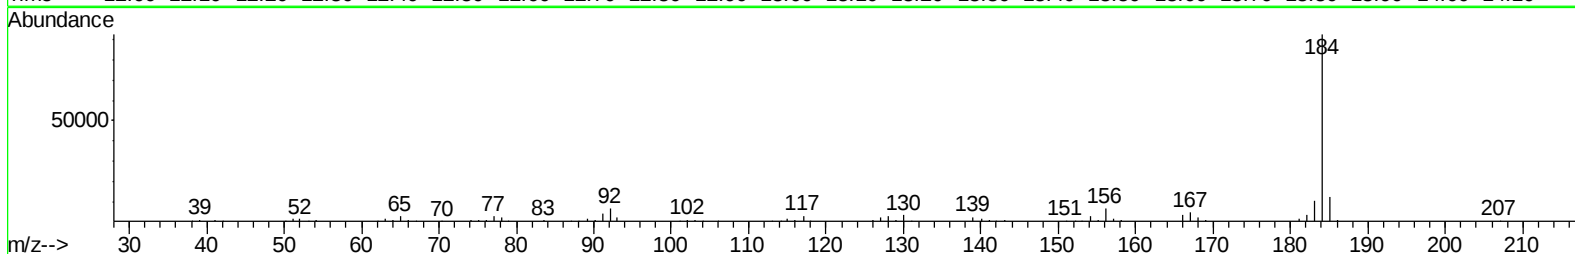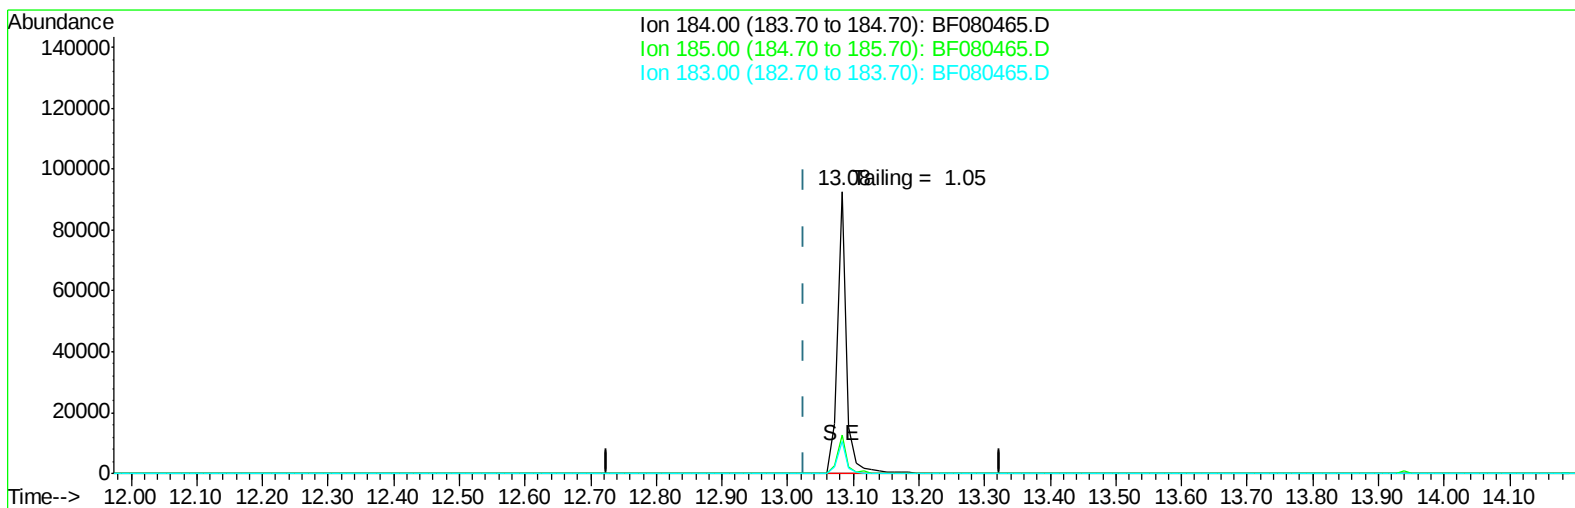

TIC: BF080465.D

(76) Benzidine

13.082min (+0.057) 0.00ng

response 91536

Ion	Exp%	Act%
184.00	100	100
185.00	14.00	13.65
183.00	11.60	11.44
0.00	0.00	0.00