


Data Path : Z:\HPCHEM1\BNA\_F\DATA\BF071415\  
 Data File : BF080465.D  
 Acq On : 14 Jul 2015 15:18  
 Operator : TP/UM  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF071415.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Wed Jul 15 03:58:42 2015

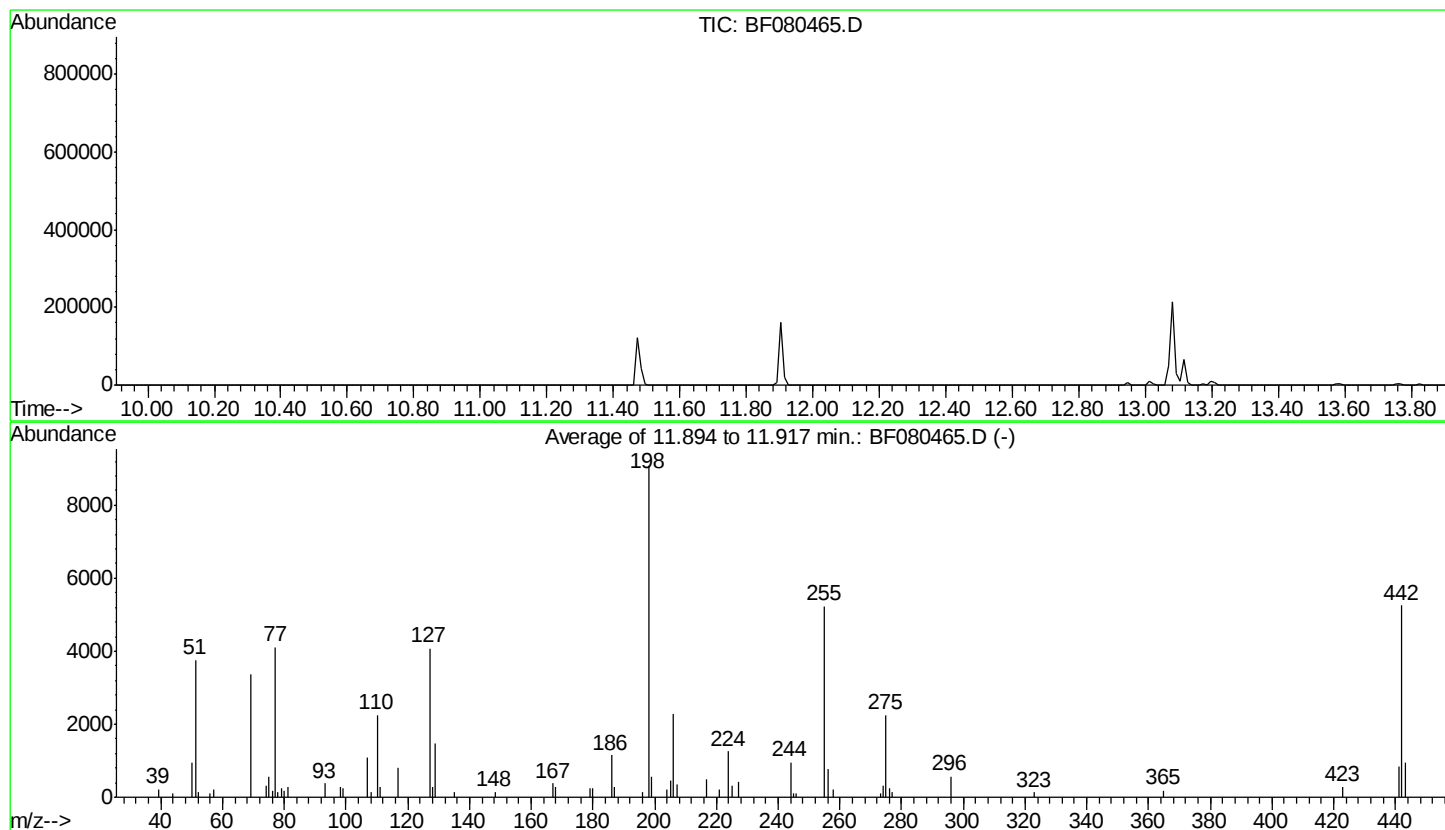

AutoFind: Scans 858, 859, 860; Background Corrected with Scan 855

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 41.5      | 3767    | PASS             |
| 68          | 69           | 0.00         | 2            | 0.0       | 0       | PASS             |
| 69          | 198          | 0.00         | 100          | 37.2      | 3378    | PASS             |
| 70          | 69           | 0.00         | 2            | 0.0       | 0       | PASS             |
| 127         | 198          | 10           | 80           | 44.9      | 4079    | PASS             |
| 197         | 198          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 9080    | PASS             |
| 199         | 198          | 5            | 9            | 6.2       | 561     | PASS             |
| 275         | 198          | 10           | 60           | 24.9      | 2258    | PASS             |
| 365         | 198          | 1            | 100          | 1.9       | 177     | PASS             |
| 441         | 442          | 0.01         | 24           | 15.8      | 830     | PASS             |
| 442         | 198          | 50           | 100          | 57.9      | 5256    | PASS             |
| 443         | 442          | 15           | 24           | 17.9      | 943     | PASS             |