


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF071415\
 Data File : BF080474.D
 Acq On : 15 Jul 2015 4:30
 Operator : TP/UM
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF071415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jul 15 03:58:42 2015

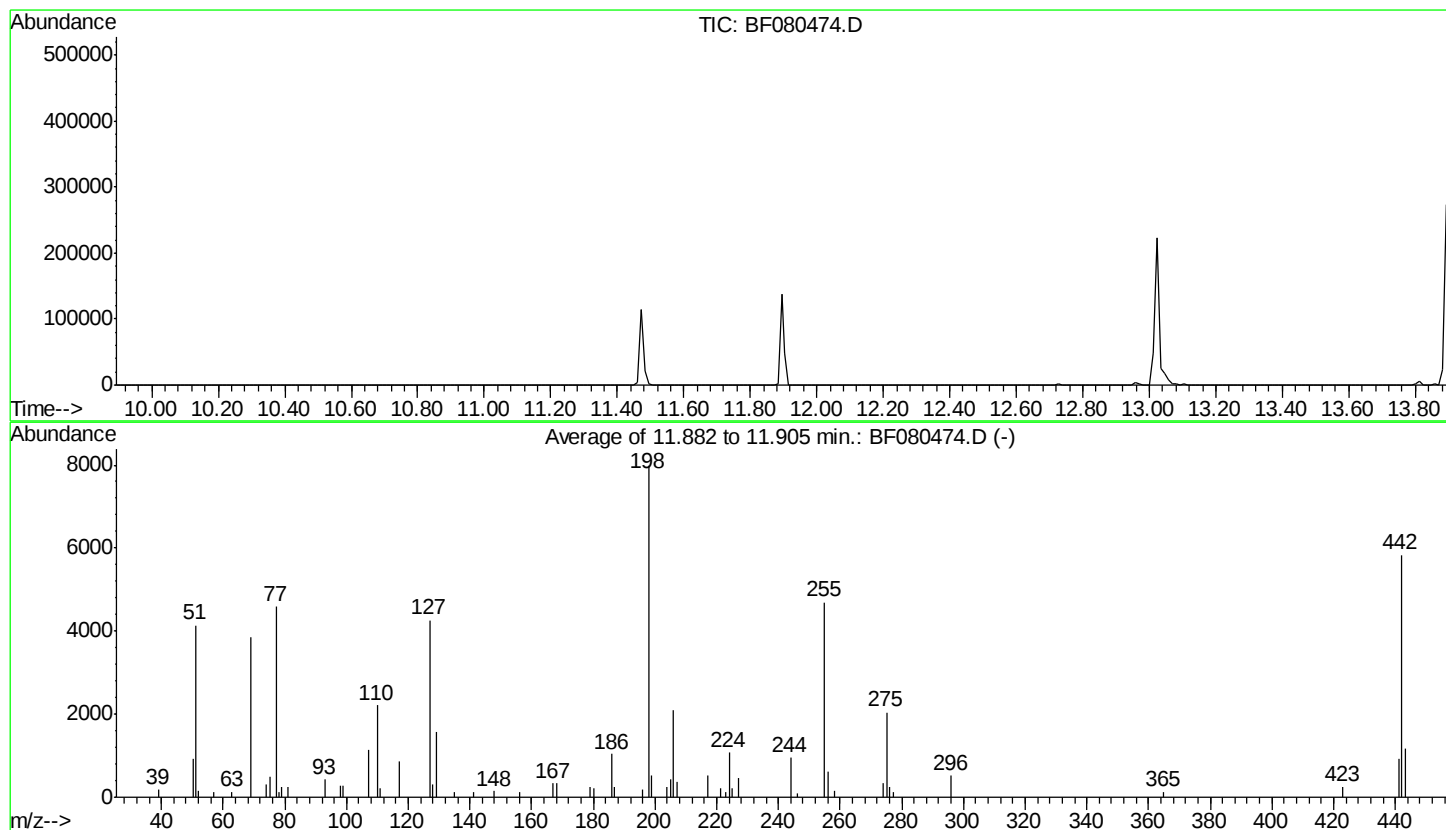

AutoFind: Scans 857, 858, 859; Background Corrected with Scan 855

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	51.9	4143	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	48.4	3862	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.5	4269	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	7986	PASS
199	198	5	9	6.7	534	PASS
275	198	10	60	25.5	2040	PASS
365	198	1	100	1.7	134	PASS
441	442	0.01	24	15.8	923	PASS
442	198	50	100	73.1	5838	PASS
443	442	15	24	20.1	1176	PASS