


Data Path : Z:\HPCHEM1\BNA F\DATA\BF071416\
 Data File : BF088981.D
 Acq On : 14 Jul 2016 11:55
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jul 11 18:13:32 2016

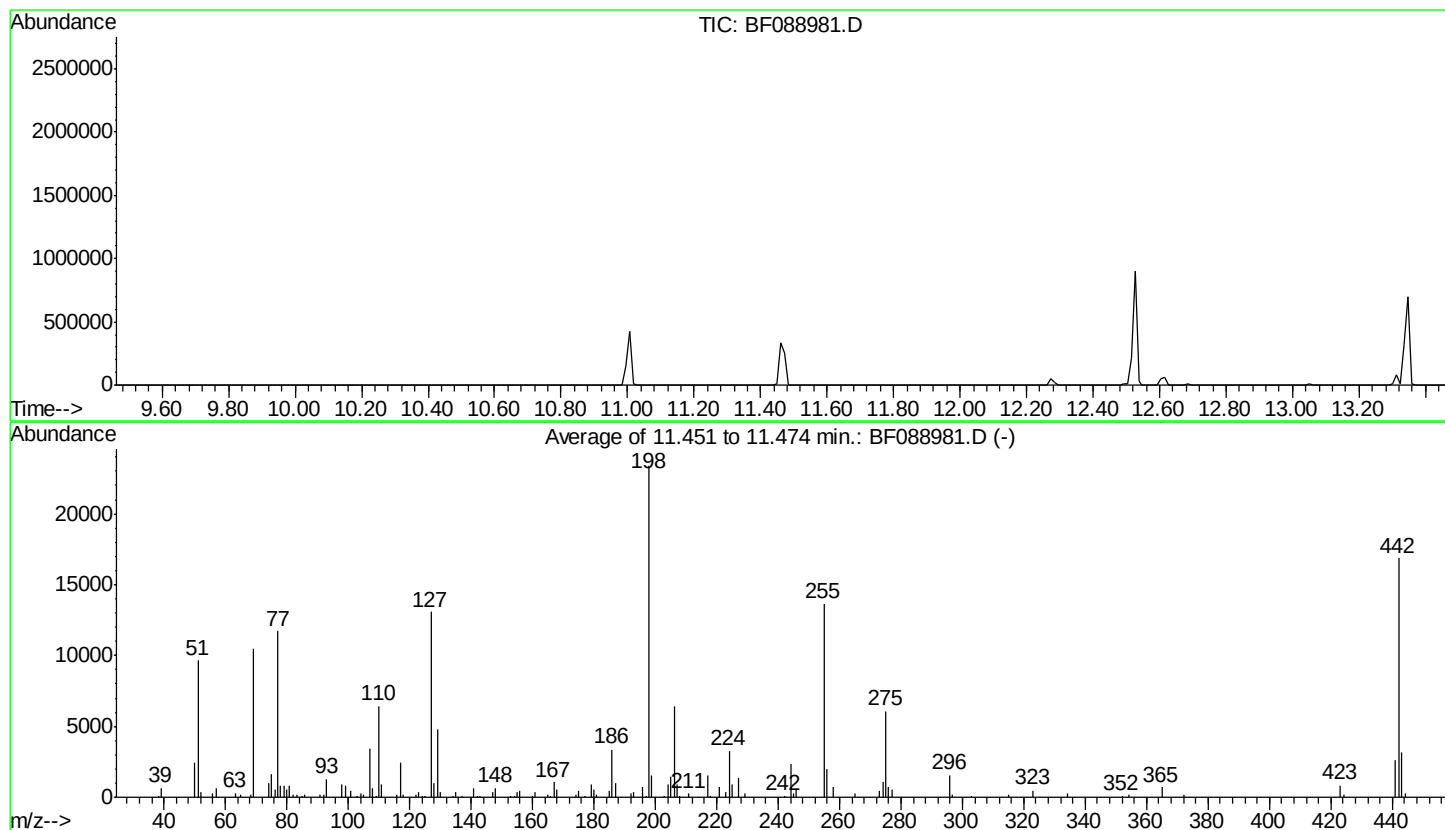

AutoFind: Scans 863, 864, 865; Background Corrected with Scan 860

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.2	9628	PASS
68	69	0.00	2	1.6	168	PASS
69	198	0.00	100	45.0	10519	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	55.9	13071	PASS
197	198	0.00	2	0.5	108	PASS
198	198	100	100	100.0	23397	PASS
199	198	5	9	6.7	1558	PASS
275	198	10	60	26.0	6087	PASS
365	198	1	100	3.0	711	PASS
441	442	0.01	24	15.7	2649	PASS
442	198	50	100	72.2	16882	PASS
443	442	15	24	18.8	3182	PASS