

Data Path : Z:\HPCHEM1\BNA F\DATA\BF071417\
 Data File : BF096806.D
 Acq On : 15 Jul 2017 7:49
 Operator : SJ/JU
 Sample : I4172-14 20X
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Jul 17 00:49:42 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF071317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 13 14:49:34 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.62	152	75135	20.00	ng	-0.01
21) Naphthalene-d8	7.90	136	281665	20.00	ng	-0.02
38) Acenaphthene-d10	9.66	164	101927	20.00	ng	-0.01
63) Phenanthrene-d10	11.13	188	167992	20.00	ng	-0.01
75) Chrysene-d12	13.76	240	191664	20.00	ng	-0.02
86) Perylene-d12	15.14	264	137225	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.23	112	42464	8.50	ng	0.00
7) Phenol-d6	6.27	99	46893	7.82	ng	-0.01
23) Nitrobenzene-d5	7.18	82	23313	5.13	ng	-0.02
41) 2,4,6-Tribromophenol	10.44	330	6779	7.79	ng	-0.02
44) 2-Fluorobiphenyl	8.98	172	41530	6.44	ng	-0.02
78) Terphenyl-d14	12.71	244	37511	3.39	ng	-0.02
Target Compounds						
25) Isophorone	7.18	82	23312	2.76	ng	# 67
50) 2,6-Dinitrotoluene	9.66	165	13520	8.13	ng	# 33
56) 2,4-Dinitrotoluene	9.66	165	13520	6.33	ng	# 33
70) Phenanthrene	11.16	178	91214	9.99	ng	98
74) Fluoranthene	12.34	202	121476	13.89	ng	99
77) Pyrene	12.56	202	109762	6.31	ng	100
80) Benzo(a)anthracene	13.75	228	39245	3.29	ng	99
82) Chrysene	13.79	228	39875	3.39	ng	95
85) Indeno(1,2,3-cd)pyrene	16.43	276	11376	4.33	ng	96
87) Benzo(b)fluoranthene	14.76	252	49707	6.01	ng	# 92
88) Benzo(k)fluoranthene	14.76	252	49707	6.34	ng	95
89) Benzo(a)pyrene	15.08	252	24903	3.28	ng	# 93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF071417\
Data File : BF096806.D
Acq On : 15 Jul 2017 7:49
Operator : SJ/JU
Sample : I4172-14 20X
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Jul 17 00:49:42 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF071317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 13 14:49:34 2017
Response via : Initial Calibration

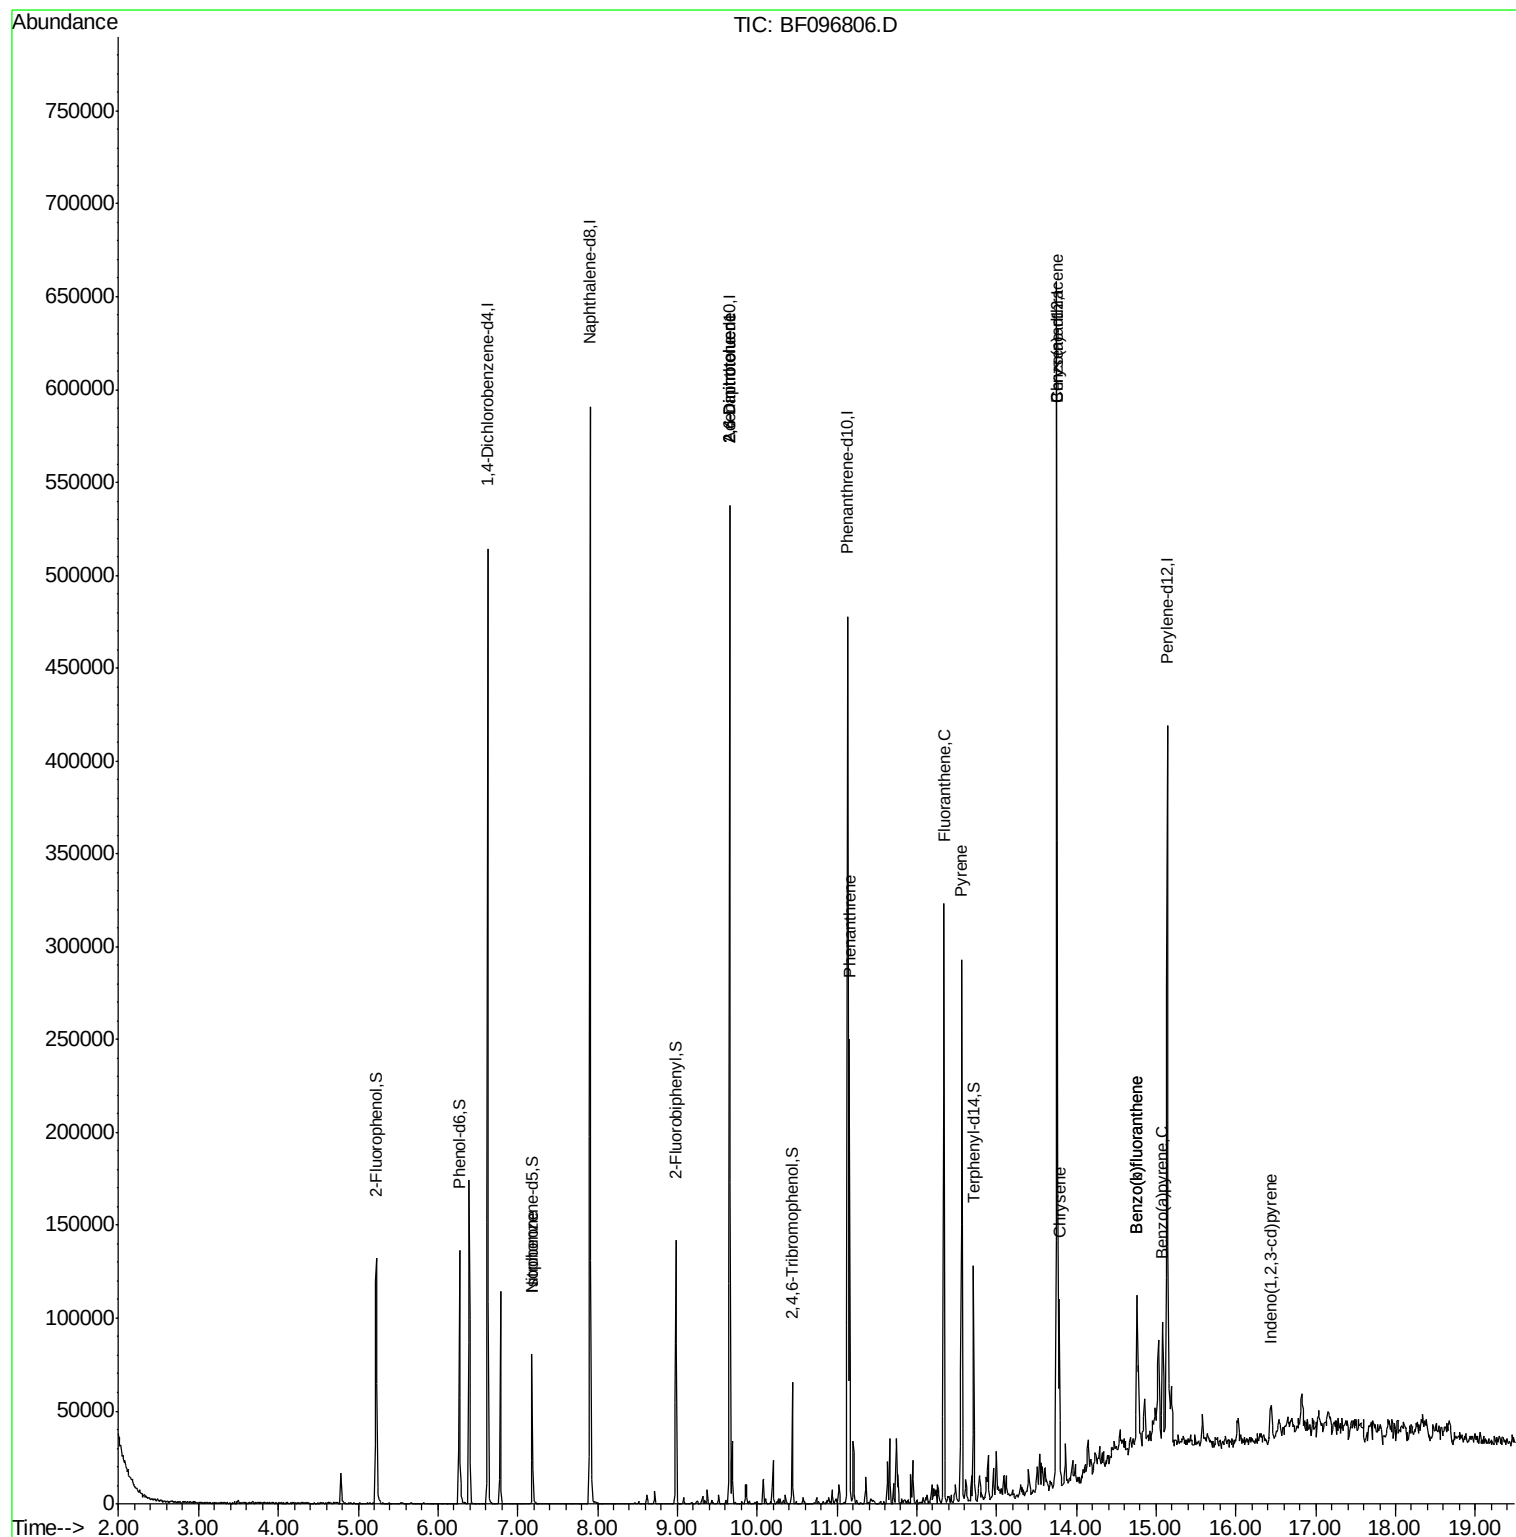

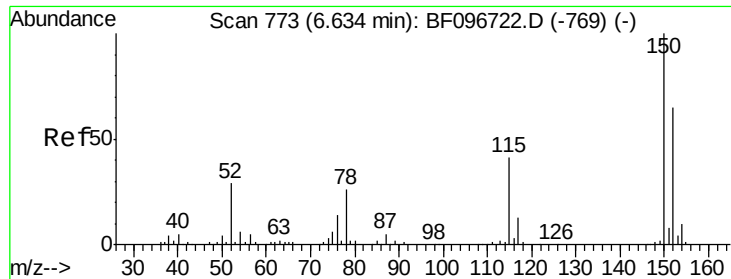


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 6.62 min Scan# 788
Delta R.T. -0.01 min
Lab File: BF096806.D
Acq: 15 Jul 2017 7:49

Instrument :
BNA_F
ClientSampleId :

Tot Ion:152 Resp: 75135
Ion Ratio Lower Upper
152 100
150 154.9 126.2 189.2
115 70.5 52.2 78.2

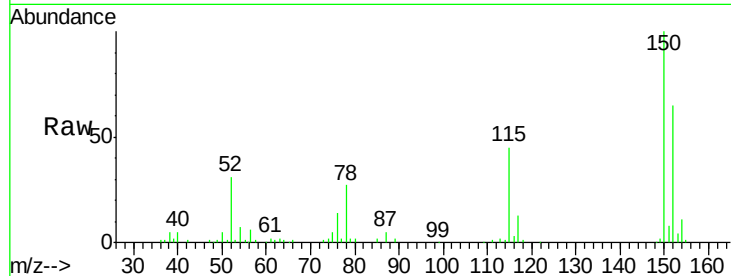


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

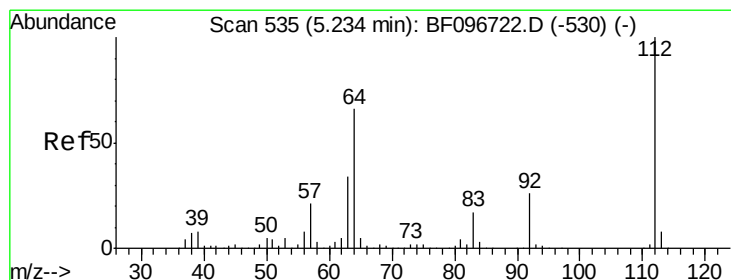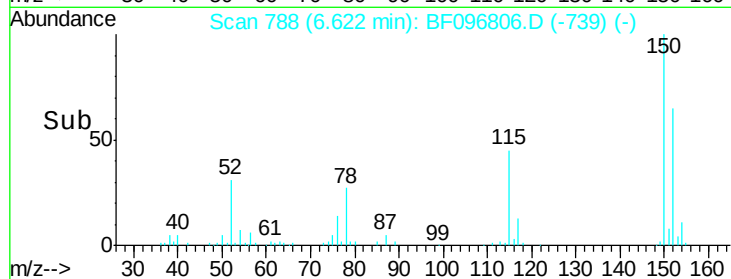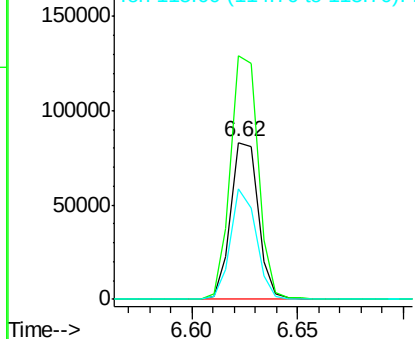



#5


2-Fluorophenol
Concen: 8.50 ng
RT: 5.23 min Scan# 551
Delta R.T. -0.01 min
Lab File: BF096806.D
Acq: 15 Jul 2017 7:49

Tgt Ion:112 Resp: 42464
Ion Ratio Lower Upper
112 100
64 60.9 46.0 69.0
63 28.9 23.4 35.0



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

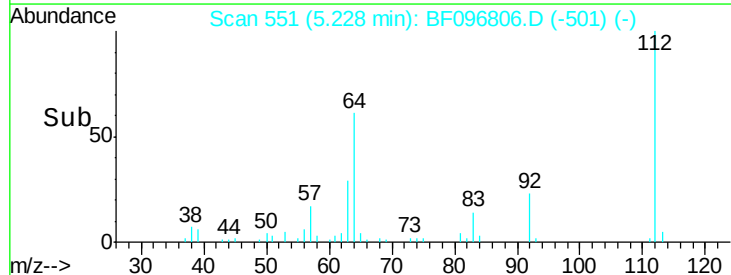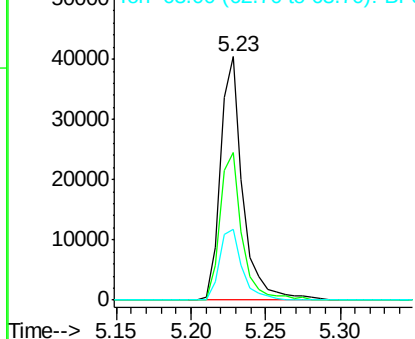

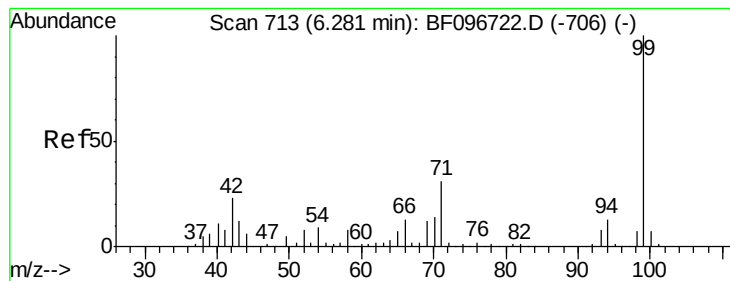

#7

Phenol-d6

Concen: 7.82 ng

RT: 6.27 min Scan# 728

Delta R.T. -0.01 min

Lab File: BF096806.D

Acq: 15 Jul 2017 7:49





Instrument :

BNA_F

ClientSampleId :

Tot Ion: 99 Resp: 46893

Ion	Ratio	Lower	Upper
99	100		
42	22.8	13.5	20.3#
71	30.7	24.5	36.7

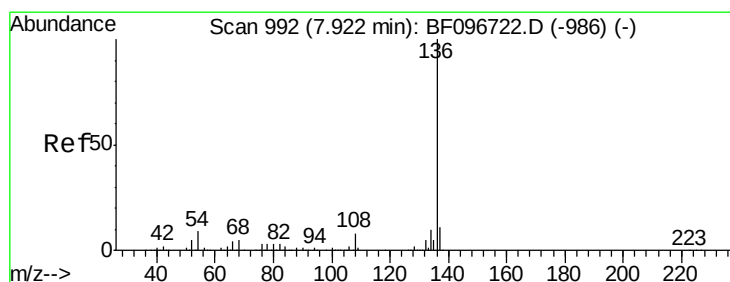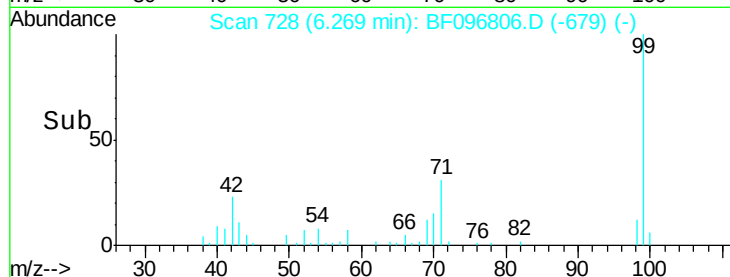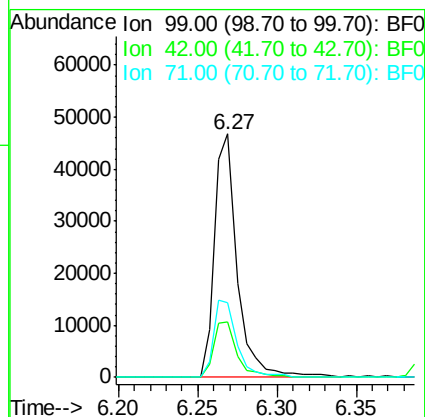

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 7.90 min Scan# 1006




Delta R.T. -0.02 min


Lab File: BF096806.D

Acq: 15 Jul 2017 7:49

Tgt Ion: 136 Resp: 281665

Ion	Ratio	Lower	Upper
136	100		
137	10.8	8.5	12.7
54	9.5	4.9	7.3#
68	4.9	4.1	6.1


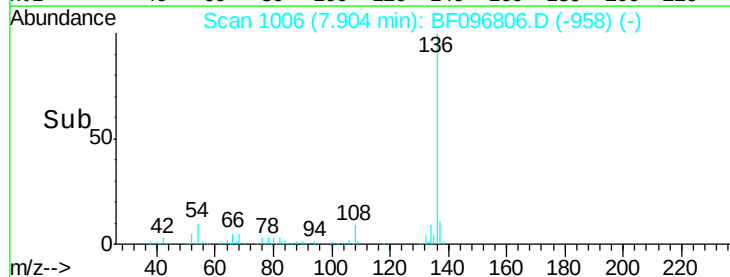
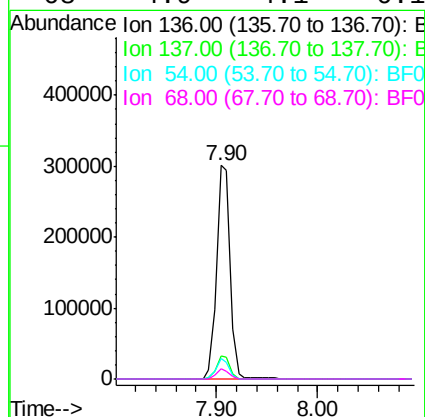
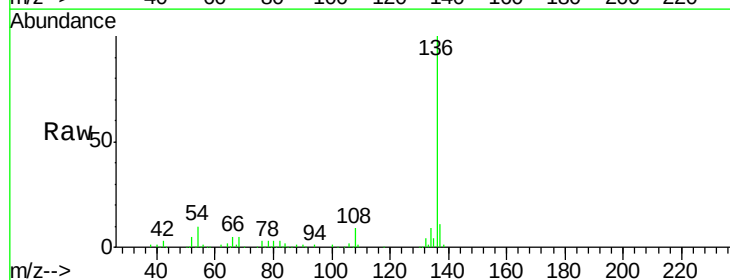


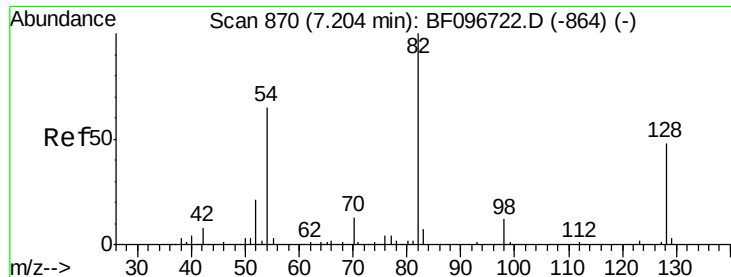

#23
 Nitrobenzene-d5
 Concen: 5.13 ng
 RT: 7.18 min Scan# 883
 Delta R.T. -0.02 min
 Lab File: BF096806.D
 Acq: 15 Jul 2017 7:49




Instrument :
 BNA_F
 ClientSampleId :


Tot Ion	82	Resp	23313
Ion Ratio	Lower	Upper	
82	100		
128	39.8	34.0	51.0
54	67.1	42.2	63.2#

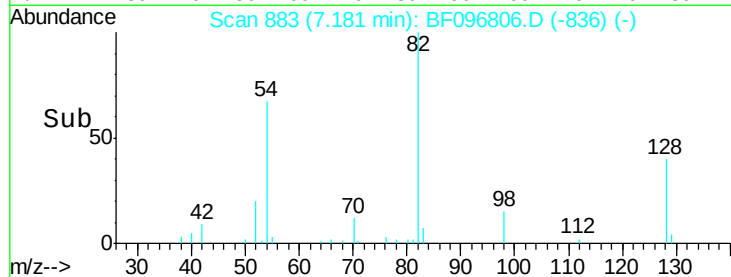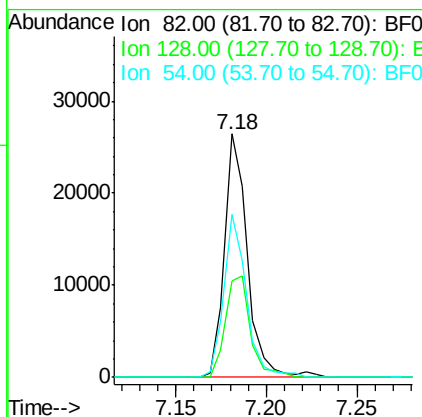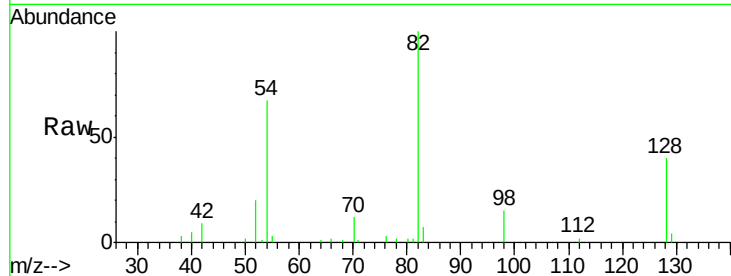

#25
 Isophorone
 Concen: 2.76 ng
 RT: 7.18 min Scan# 883
 Delta R.T. -0.29 min
 Lab File: BF096806.D
 Acq: 15 Jul 2017 7:49

Tgt Ion	82	Resp	23312
Ion Ratio	Lower	Upper	
82	100		
95	0.0	5.3	7.9#
138	0.0	13.1	19.7#

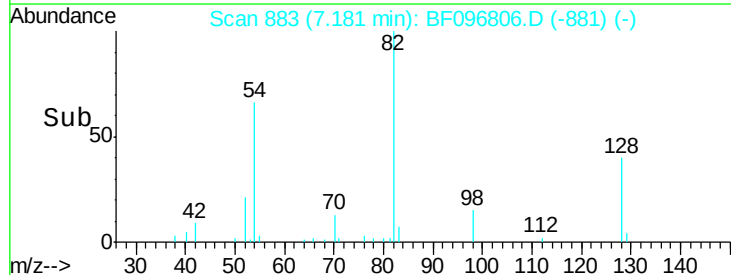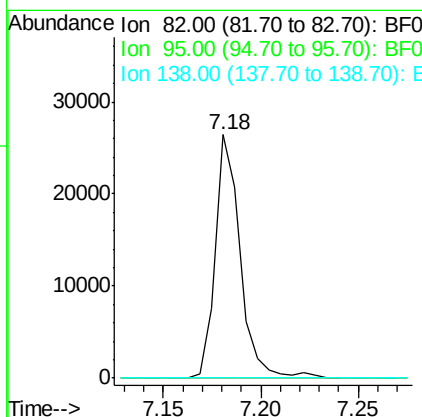

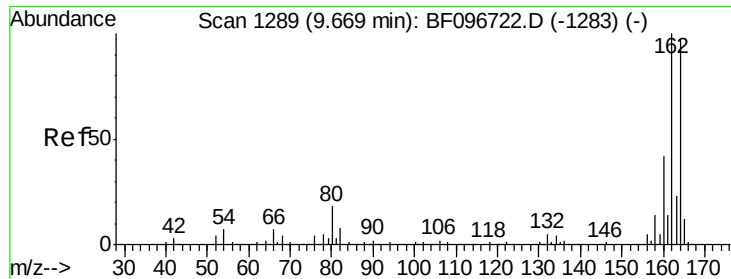

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 9.66 min Scan# 1304

Delta R.T. -0.01 min

Lab File: BF096806.D

Acq: 15 Jul 2017 7:49

Instrument :

BNA_F

ClientSampleId :


Tot Ion:164 Resp: 101927

Ion Ratio Lower Upper

164 100

162 104.4 82.6 123.8




160 45.3 36.2 54.2



Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

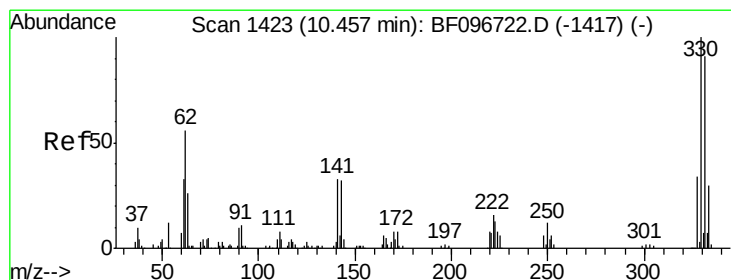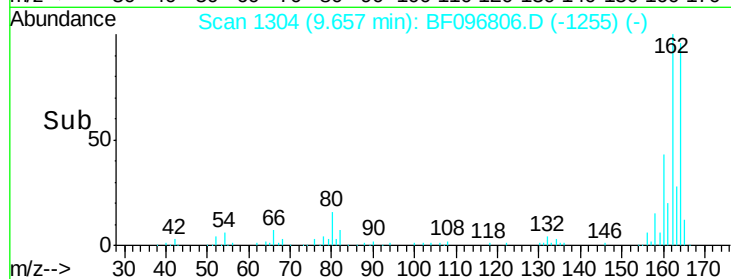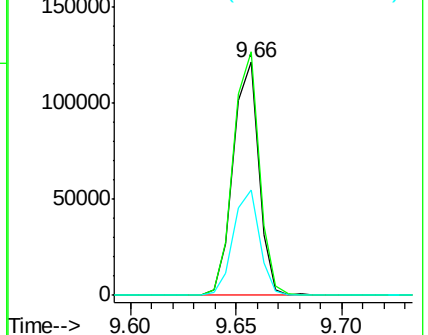

#41

2,4,6-Tribromophenol

Concen: 7.79 ng

RT: 10.44 min Scan# 1437

Delta R.T. -0.02 min

Lab File: BF096806.D

Acq: 15 Jul 2017 7:49


Tgt Ion:330 Resp: 6779

Ion Ratio Lower Upper

330 100

332 100.5 76.6 115.0



141 39.2 31.4 47.2

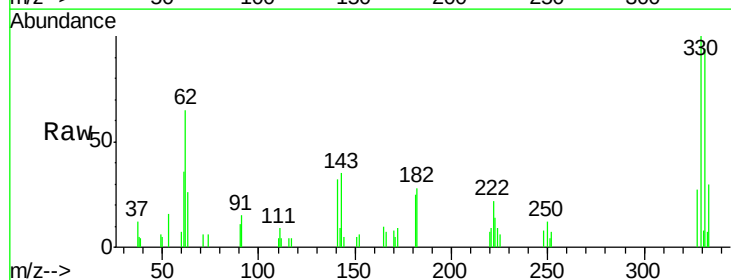


Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



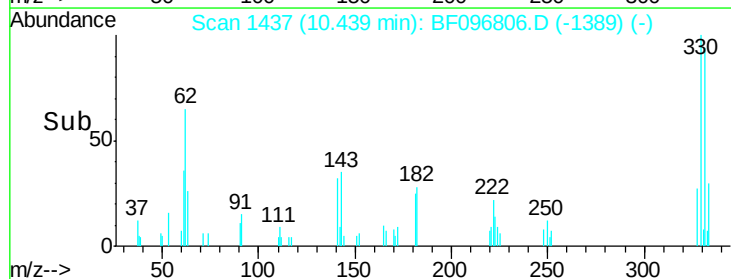
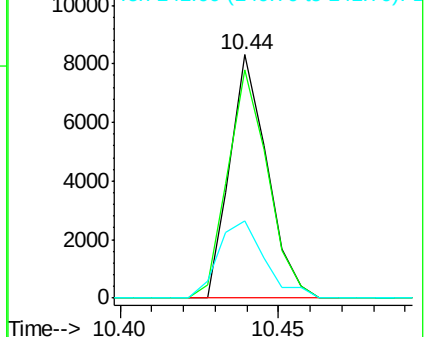


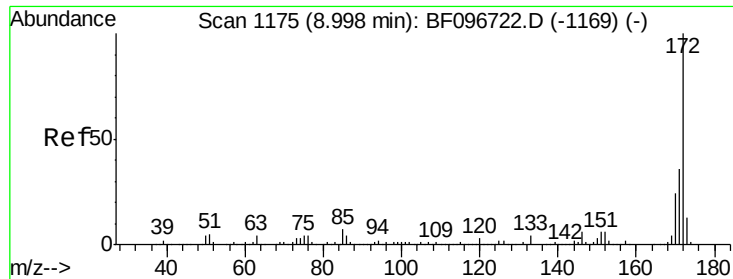

#44
 2-Fluorobiphenyl
 Concen: 6.44 ng
 RT: 8.98 min Scan# 1189
 Delta R.T. -0.02 min
 Lab File: BF096806.D
 Acq: 15 Jul 2017 7:49




Instrument :
 BNA_F
 ClientSampleId :


Tot Ion:172 Resp: 41530
 Ion Ratio Lower Upper
 172 100
 171 34.6 29.6 44.4
 170 23.2 19.8 29.8

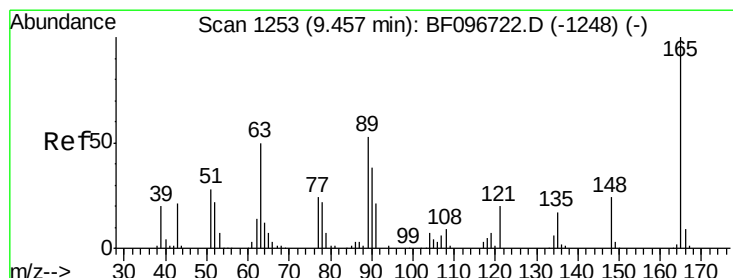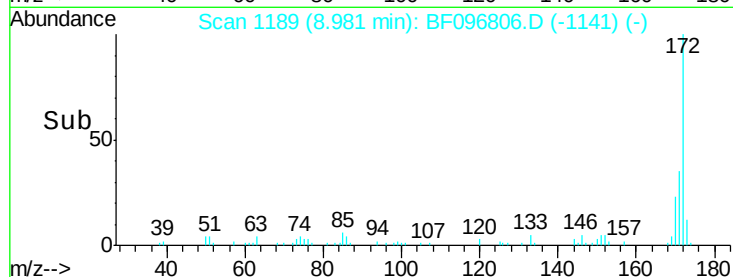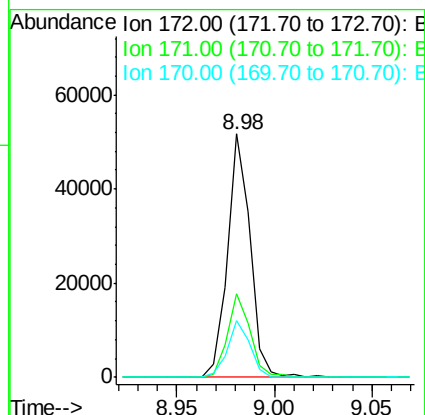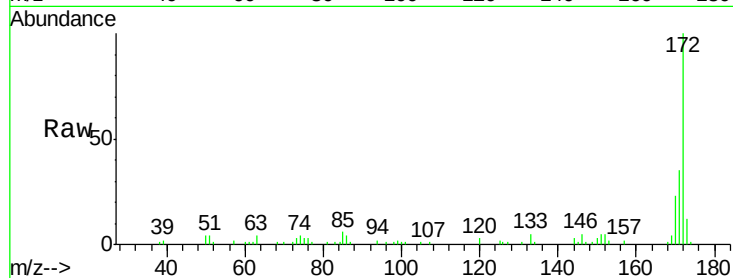

#50
 2,6-Dinitrotoluene
 Concen: 8.13 ng
 RT: 9.66 min Scan# 1304
 Delta R.T. 0.20 min
 Lab File: BF096806.D
 Acq: 15 Jul 2017 7:49

Tgt Ion:165 Resp: 13520
 Ion Ratio Lower Upper
 165 100
 63 0.0 34.3 51.5#
 89 2.1 37.1 55.7#


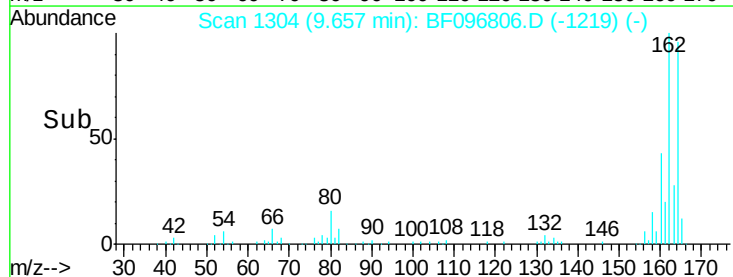
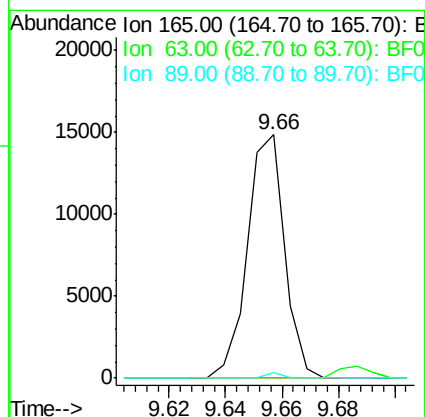
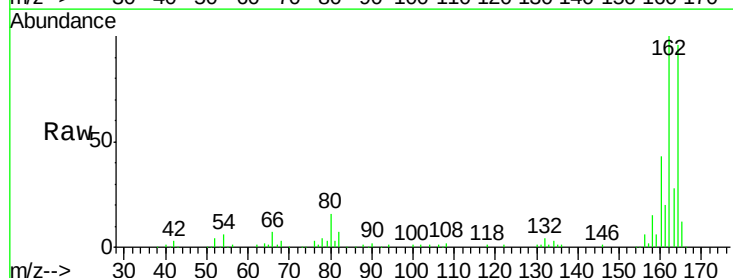


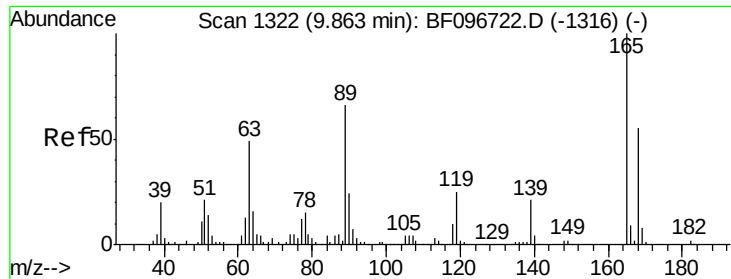

#56
 2,4-Dinitrotoluene
 Concen: 6.33 ng
 RT: 9.66 min Scan# 1304
 Delta R.T. -0.21 min
 Lab File: BF096806.D
 Acq: 15 Jul 2017 7:49




Instrument :
 BNA_F
 ClientSampleId :


Tot Ion:	165	Resp:	13520
Ion Ratio	Lower	Upper	
165	100		
63	0.0	25.4	38.0#
89	2.1	46.4	69.6#
182	0.0	1.8	2.6#

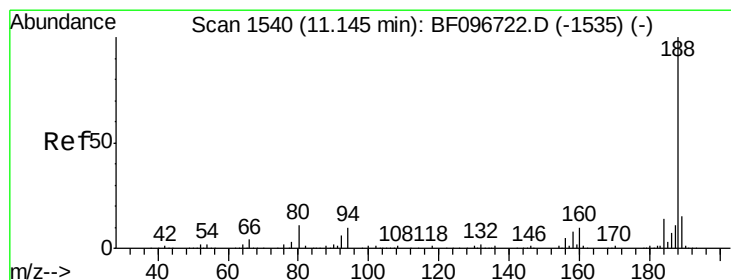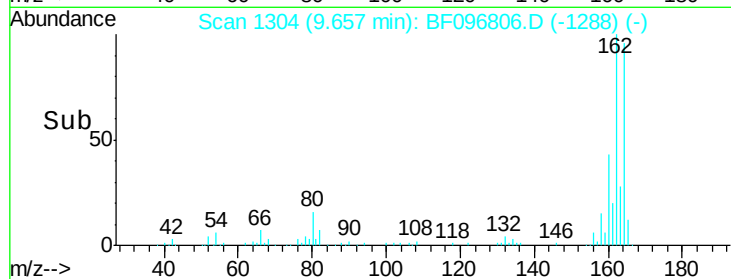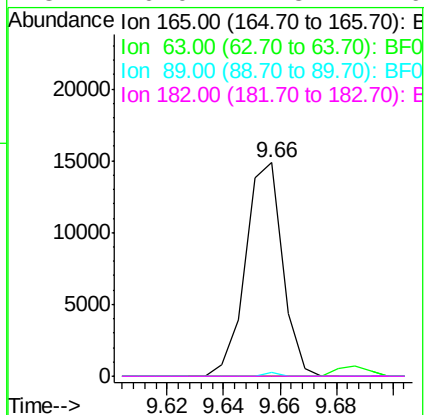

#63
 Phenanthrene-d10
 Concen: 20.00 ng
 RT: 11.13 min Scan# 1555
 Delta R.T. -0.01 min
 Lab File: BF096806.D
 Acq: 15 Jul 2017 7:49

Tgt Ion:	188	Resp:	167992
Ion Ratio	Lower	Upper	
188	100		
94	9.6	9.4	14.2
80	9.5	10.2	15.2#

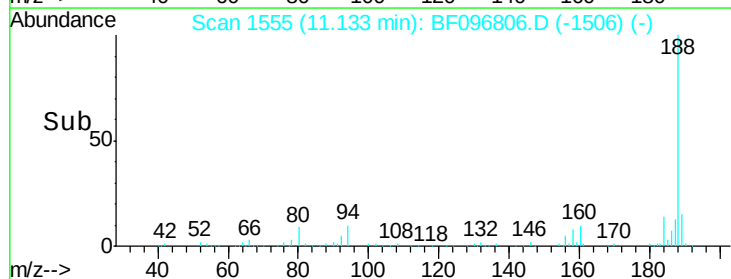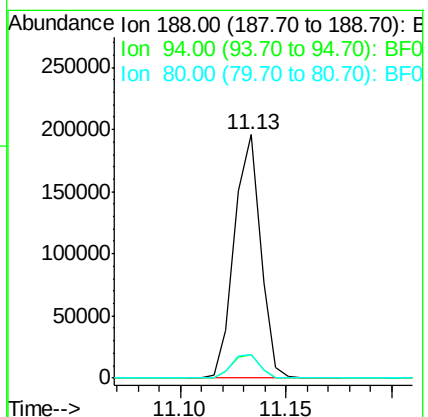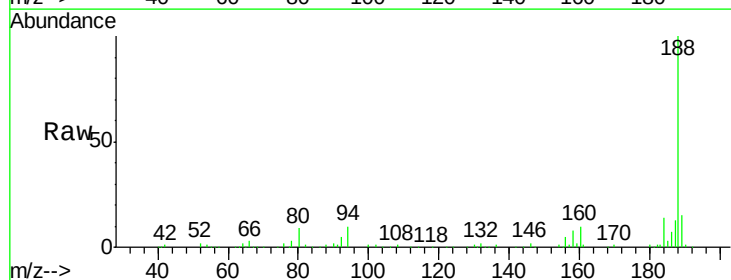

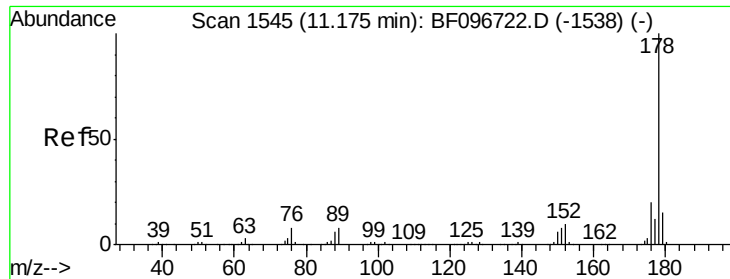

#70

Phenanthrene

Concen: 9.99 ng

RT: 11.16 min Scan# 1559

Delta R.T. -0.02 min

Lab File: BF096806.D

Acq: 15 Jul 2017 7:49

Instrument :

BNA_F

ClientSampleId :


Tot Ion:178 Resp: 91214

Ion Ratio Lower Upper

178 100

176 19.6 16.2 24.4




179 14.4 12.6 19.0



Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E

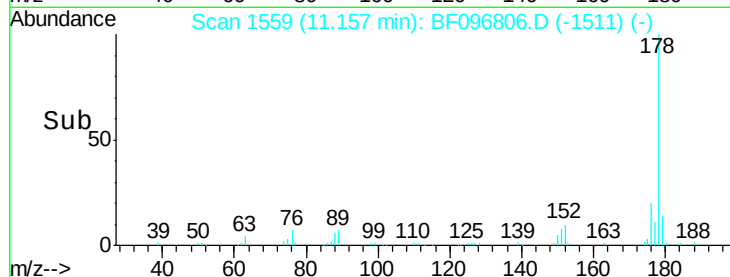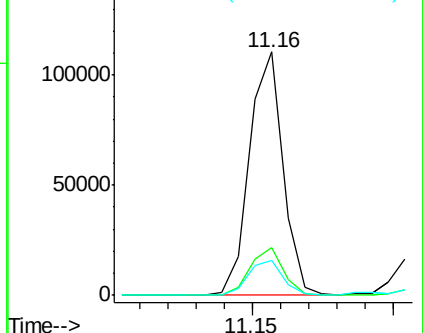

#74

Fluoranthene

Concen: 13.89 ng

RT: 12.34 min Scan# 1760

Delta R.T. -0.02 min

Lab File: BF096806.D

Acq: 15 Jul 2017 7:49


Tgt Ion:202 Resp: 121476

Ion Ratio Lower Upper

202 100

101 12.4 0.0 33.2



203 18.6 0.0 38.1




Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 203.00 (202.70 to 203.70): E

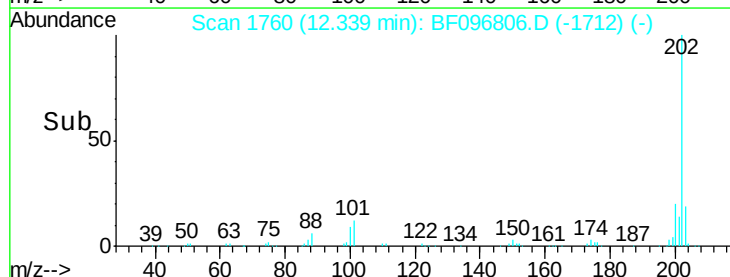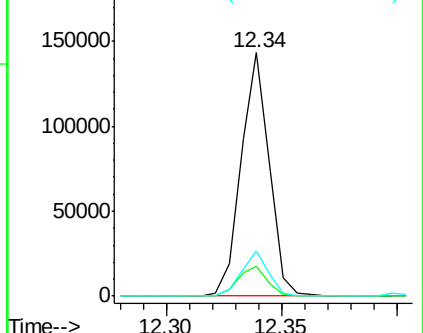

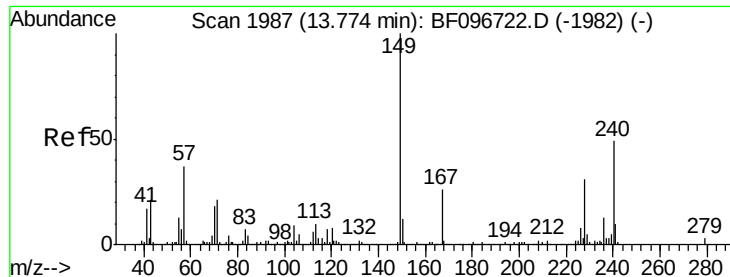

#75

Chrysene-d12

Concen: 20.00 ng

RT: 13.76 min Scan# 2001

Delta R.T. -0.02 min

Lab File: BF096806.D

Acq: 15 Jul 2017 7:49

Instrument :

BNA_F

ClientSampleId :


Tot Ion:240 Resp: 191664

Ion Ratio Lower Upper

240 100

120 16.7 5.8 8.8#




236 25.0 20.5 30.7



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

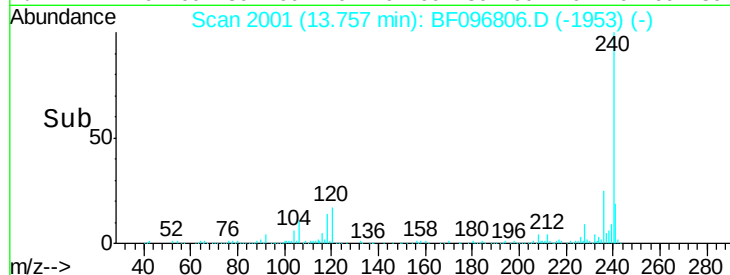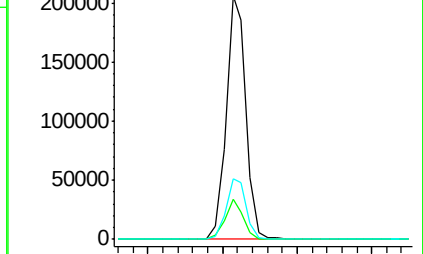

#77

Pyrene

Concen: 6.31 ng

RT: 12.56 min Scan# 1798

Delta R.T. -0.02 min

Lab File: BF096806.D

Acq: 15 Jul 2017 7:49


Tgt Ion:202 Resp: 109762

Ion Ratio Lower Upper

202 100

200 22.2 17.6 26.4



203 18.0 14.4 21.6




Abundance Ion 202.00 (201.70 to 202.70): E

Ion 200.00 (199.70 to 200.70): E

Ion 203.00 (202.70 to 203.70): E

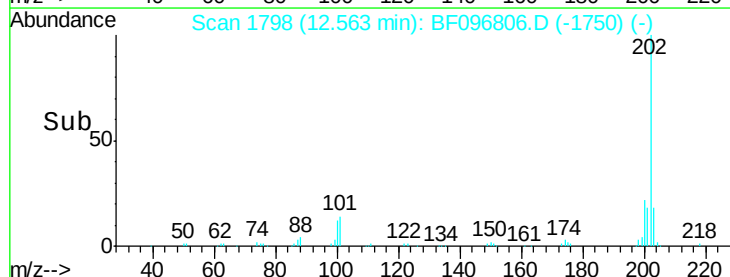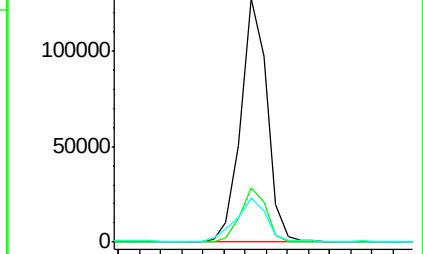

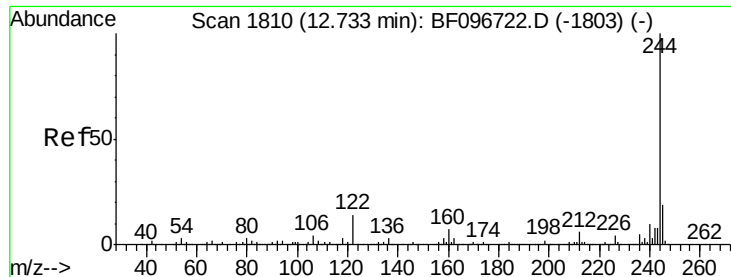

#78

Terphenyl-d14

Concen: 3.39 ng

RT: 12.71 min Scan# 1823

Delta R.T. -0.02 min

Lab File: BF096806.D

Acq: 15 Jul 2017 7:49

Instrument :

BNA_F

ClientSampled :


Tot Ion:244 Resp: 37511

Ion Ratio Lower Upper

244 100

212 7.0 6.0 9.0




122 18.2 10.3 15.5#



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

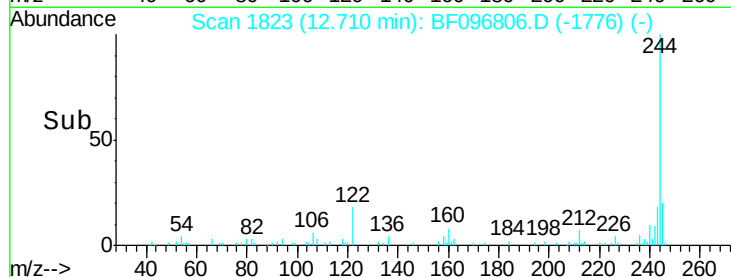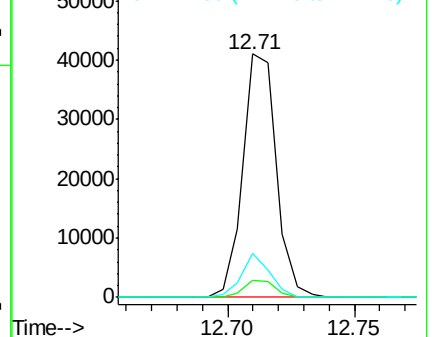

#80

Benzo(a)anthracene

Concen: 3.29 ng

RT: 13.75 min Scan# 2000

Delta R.T. -0.01 min

Lab File: BF096806.D

Acq: 15 Jul 2017 7:49


Tgt Ion:228 Resp: 39245

Ion Ratio Lower Upper

228 100

226 29.3 22.6 33.8



229 20.1 16.3 24.5




Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

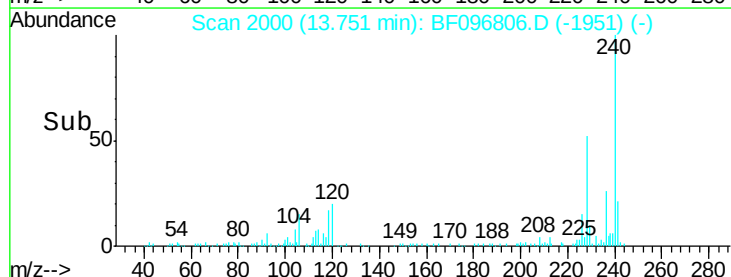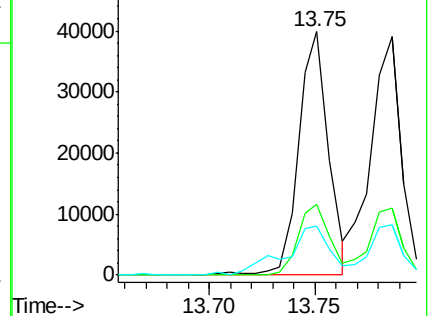

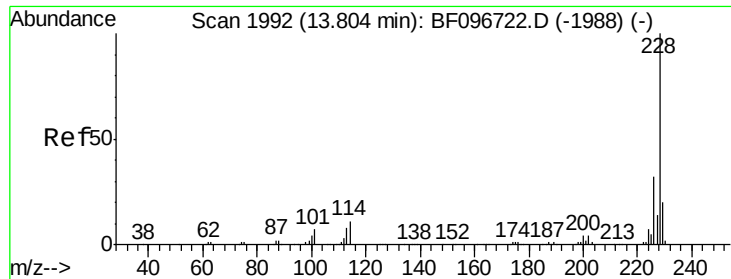

#82

Chrysene

Concen: 3.39 ng

RT: 13.79 min Scan# 2006

Delta R.T. -0.02 min

Lab File: BF096806.D

Acq: 15 Jul 2017 7:49

Instrument :

BNA_F

ClientSampled :


Tot Ion:228 Resp: 39875

Ion Ratio Lower Upper

228 100

226 27.9 24.9 37.3




229 21.1 15.8 23.6

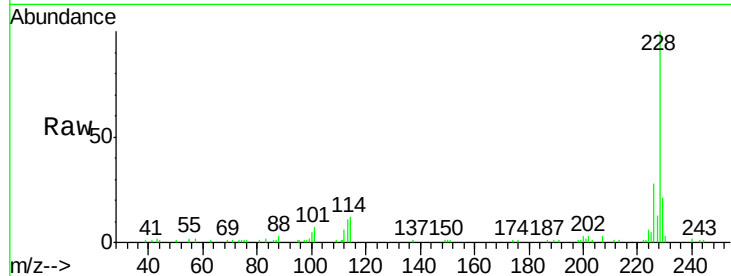

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

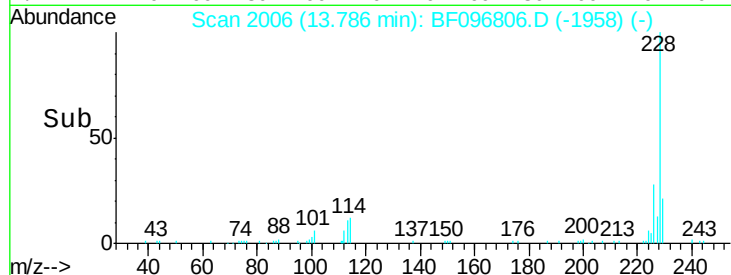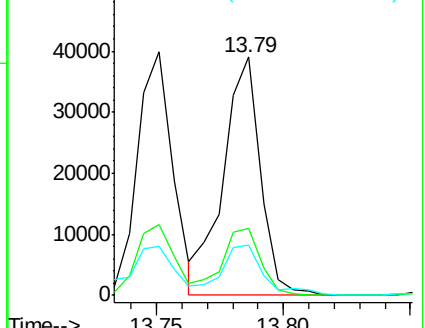

#85

Indeno(1,2,3-cd)pyrene

Concen: 4.33 ng

RT: 16.43 min Scan# 2456

Delta R.T. -0.03 min

Lab File: BF096806.D

Acq: 15 Jul 2017 7:49


Tgt Ion:276 Resp: 11376

Ion Ratio Lower Upper

276 100

138 31.6 27.8 41.6



277 26.9 20.2 30.4




Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

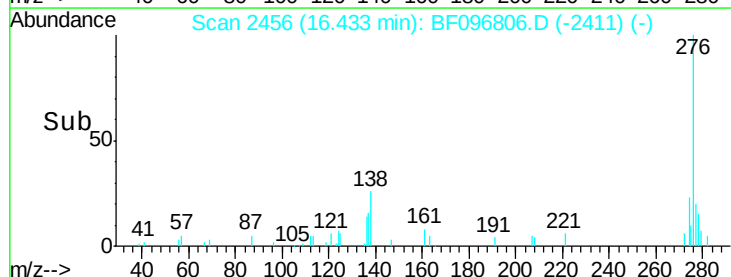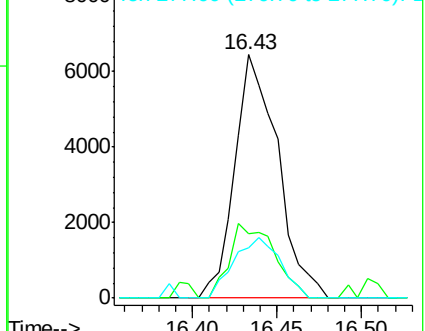




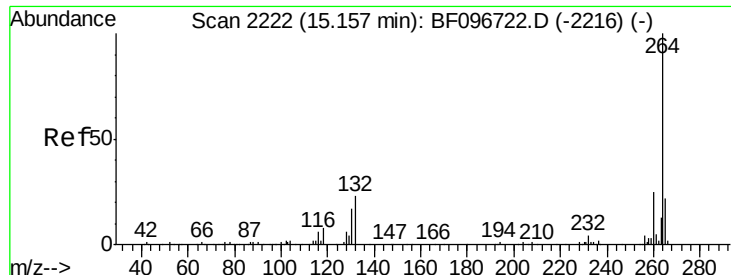


#86
Pervlene-d12
Concen: 20.00 ng
RT: 15.14 min Scan# 2236
Delta R.T. -0.02 min
Lab File: BF096806.D
Acq: 15 Jul 2017 7:49

Instrument :
BNA_F
ClientSampleId :

Tot Ion:264 Resp: 137225




Ion	Ratio	Lower	Upper
264	100		
260	23.2	19.5	29.3
265	21.3	17.2	25.8

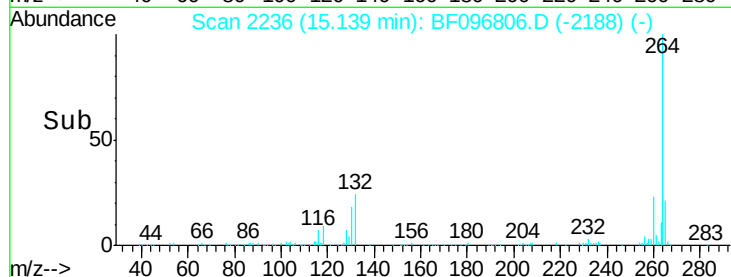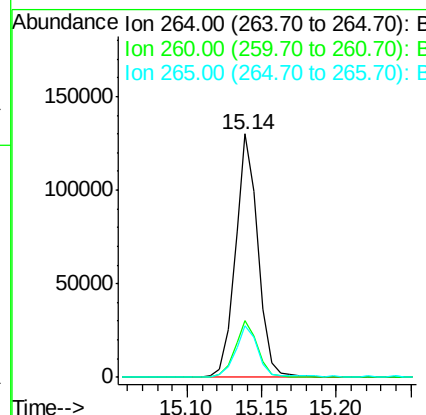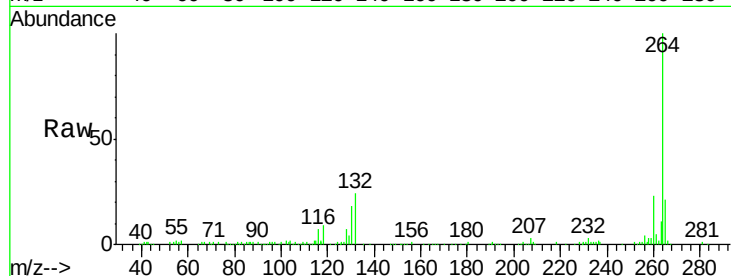


#87
Benzo(b)fluoranthene
Concen: 6.01 ng
RT: 14.76 min Scan# 2171
Delta R.T. -0.02 min
Lab File: BF096806.D
Acq: 15 Jul 2017 7:49

Tgt Ion:252 Resp: 49707

Ion	Ratio	Lower	Upper
252	100		
253	20.7	18.1	27.1
125	18.4	9.8	14.8#

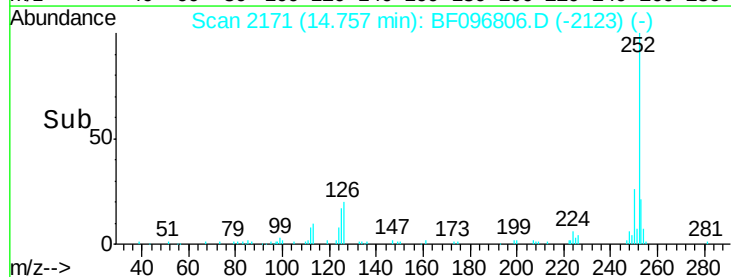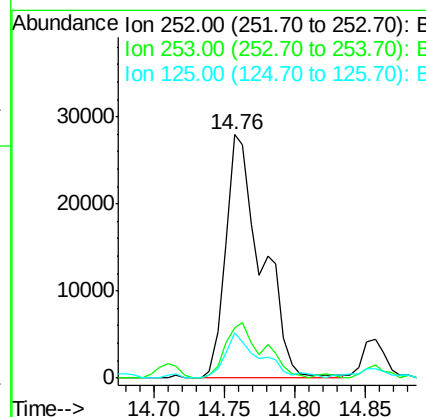


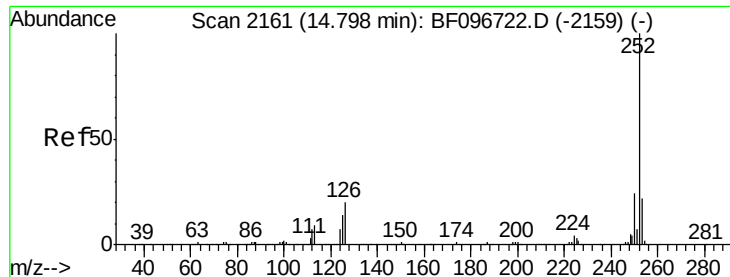




#88
Benzo(k)fluoranthene
Concen: 6.34 ng
RT: 14.76 min Scan# 2171
Delta R.T. -0.04 min
Lab File: BF096806.D
Acq: 15 Jul 2017 7:49

Instrument :
BNA_F
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
252	100		
253	20.7	18.4	27.6
125	18.4	13.1	19.7




Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

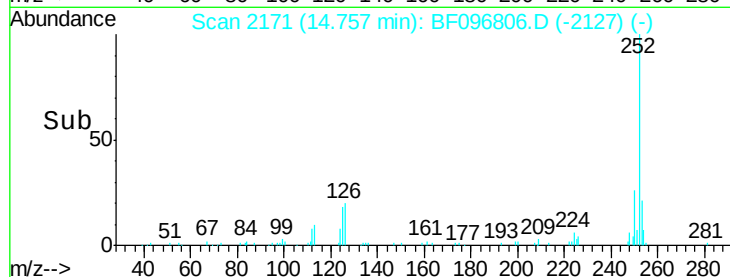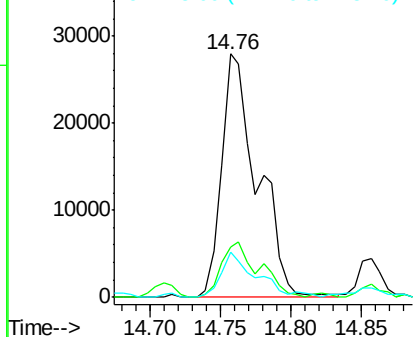

#89
Benzo(a)pyrene
Concen: 3.28 ng
RT: 15.08 min Scan# 2226
Delta R.T. -0.02 min
Lab File: BF096806.D
Acq: 15 Jul 2017 7:49

Tgt Ion	Ratio	Lower	Upper
252	100		
253	23.6	17.5	26.3
125	18.8	11.0	16.4



Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

