
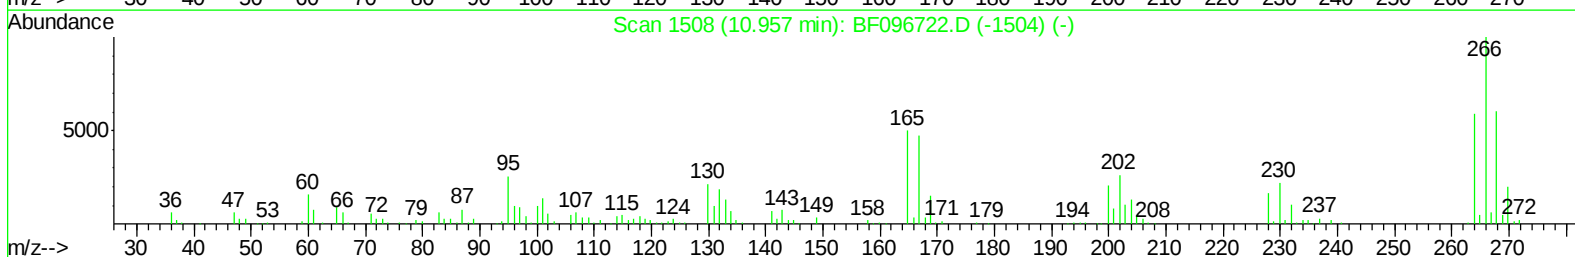
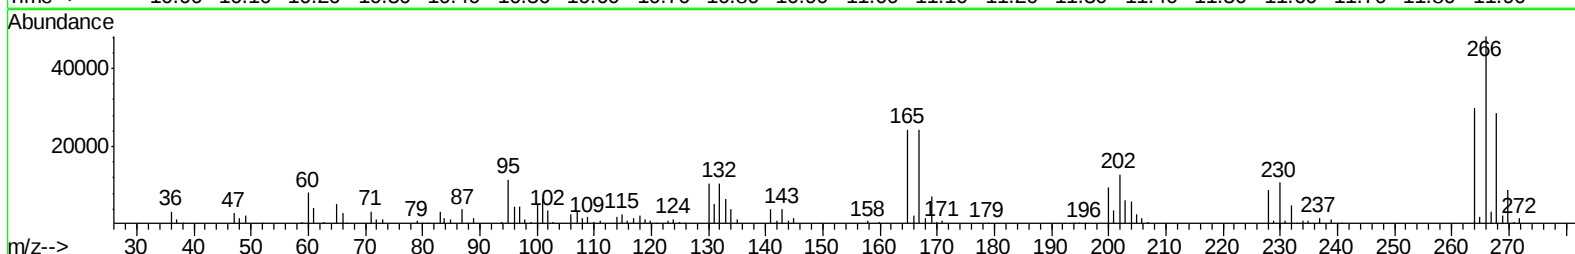


Data Path : Z:\HPCHEM1\BNA F\DATA\BF071417\
Data File : BF096804.D
Acq On : 15 Jul 2017 6:54
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Jul 15 07:27:09 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF071317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 13 14:49:34 2017
Response via : Initial Calibration

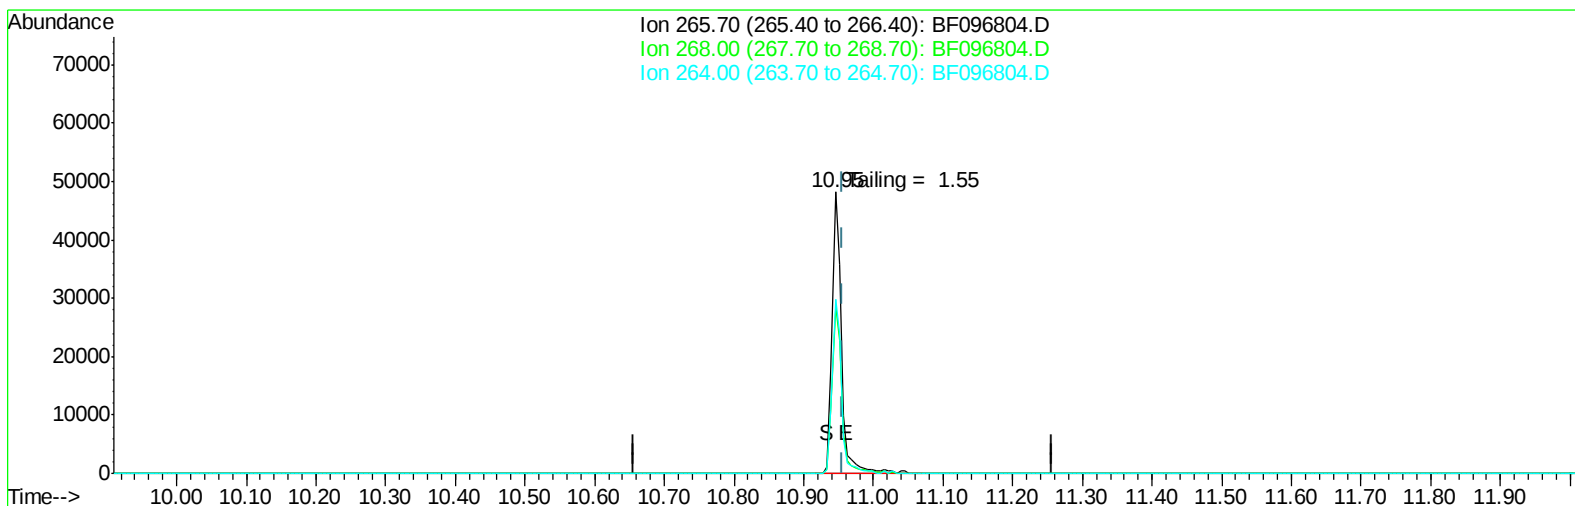

TIC: BF096804.D

(69) Pentachlorophenol (C)

10.945min (-0.012) 0.00ng




response 43632

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	59.10
264.00	64.60	61.67
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF071417\
 Data File : BF096804.D
 Acq On : 15 Jul 2017 6:54
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Jul 15 07:27:09 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF071317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 13 14:49:34 2017
 Response via : Initial Calibration

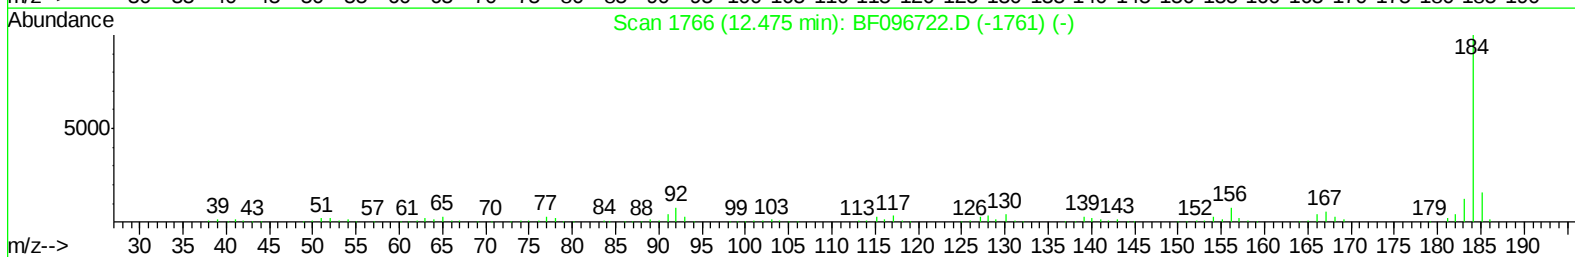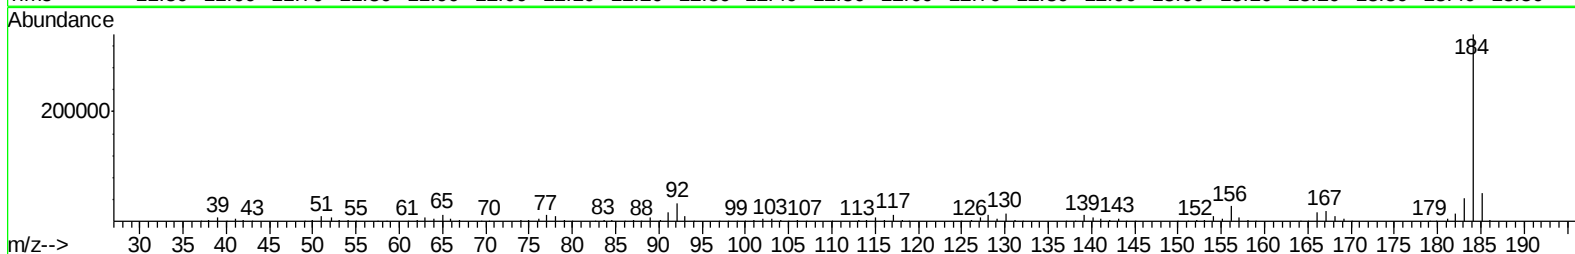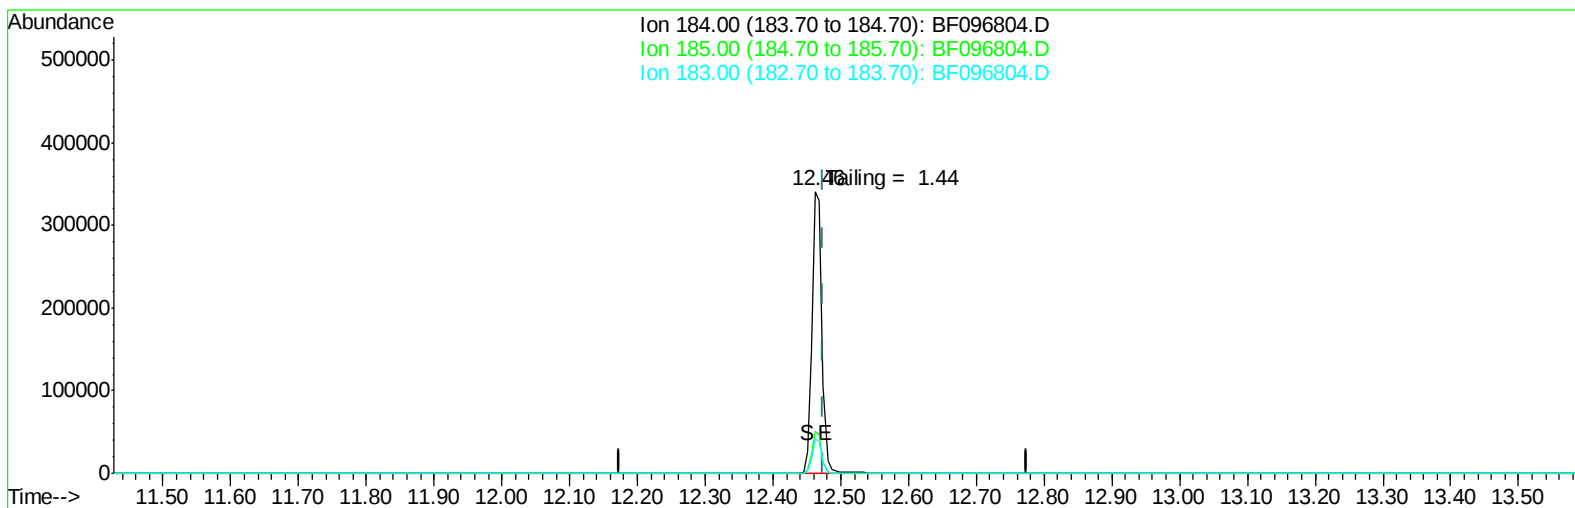

TIC: BF096804.D

(76) Benzidine

12.463min (-0.012) 0.00ng




response 350043

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	15.08#
183.00	12.20	12.12
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF071417\
Data File : BF096804.D
Acq On : 15 Jul 2017 6:54
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Jul 15 07:27:09 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF071317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 13 14:49:34 2017
Response via : Initial Calibration

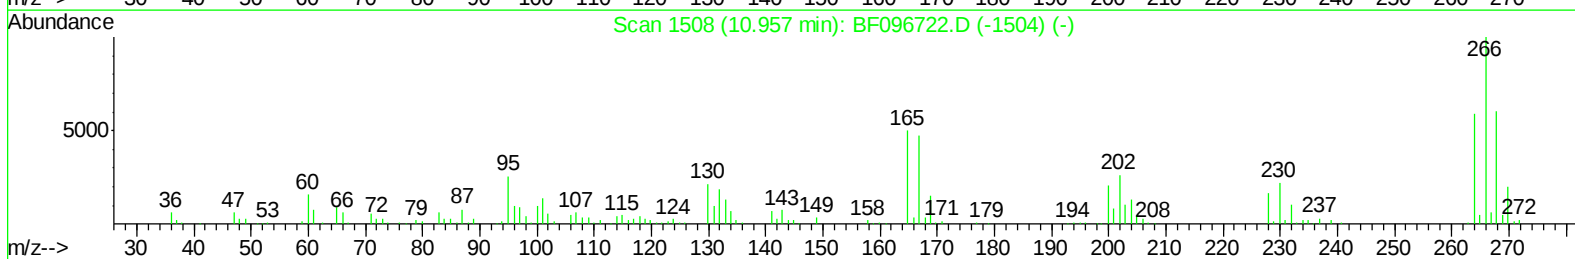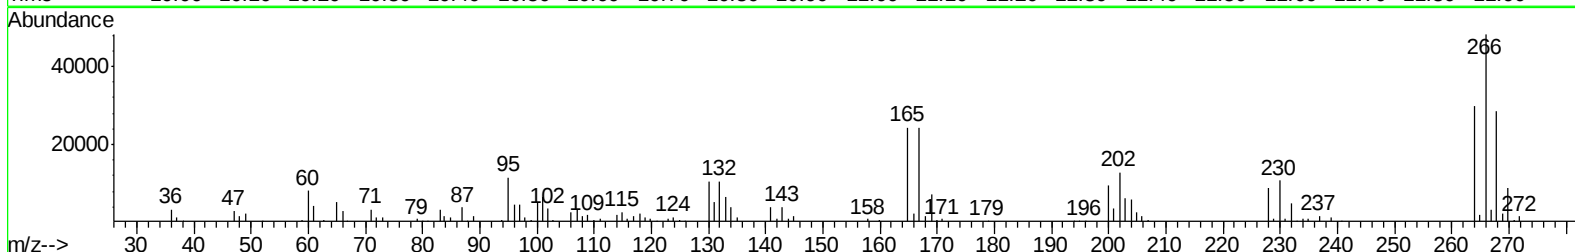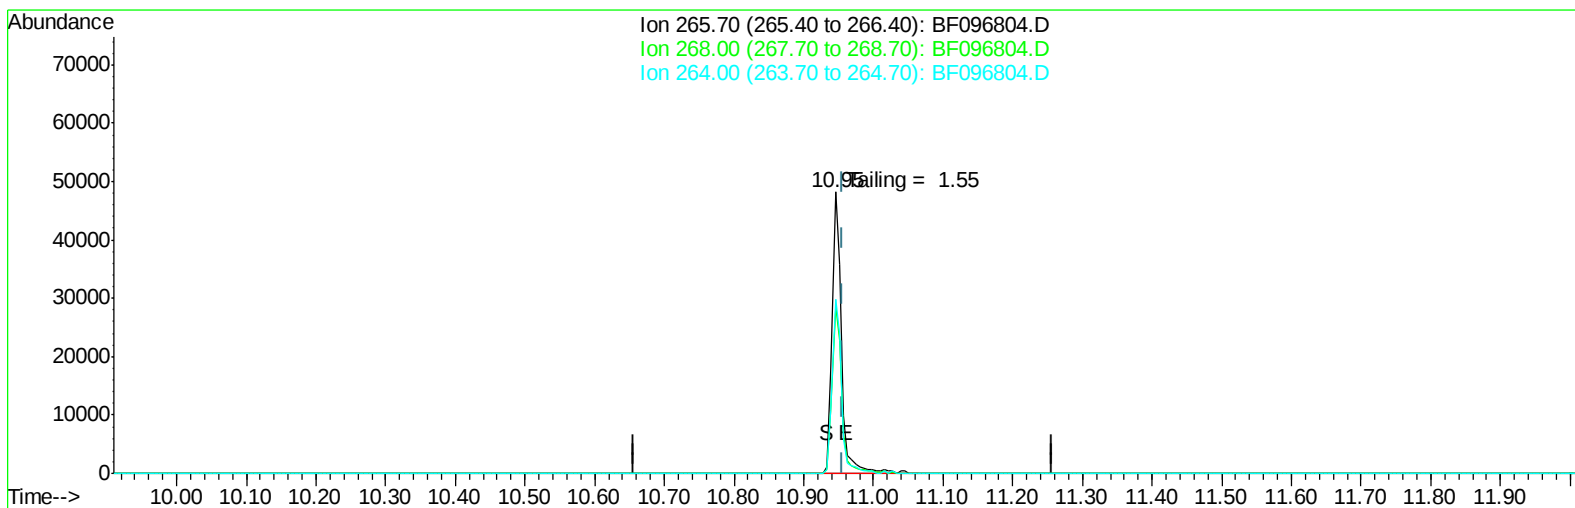

TIC: BF096804.D

(69) Pentachlorophenol (C)




10.945min (-0.012) 0.00ng

response 43632

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	59.10
264.00	64.60	61.67
0.00	0.00	0.00

```
Data Path : Z:\HPCHEM1\BNA F\DATA\BF071417\  
Data File : BF096804.D  
Acq On    : 15 Jul 2017    6:54  
Operator  : SJ/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Jul 15 07:27:09 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF071317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 13 14:49:34 2017
Response via : Initial Calibration

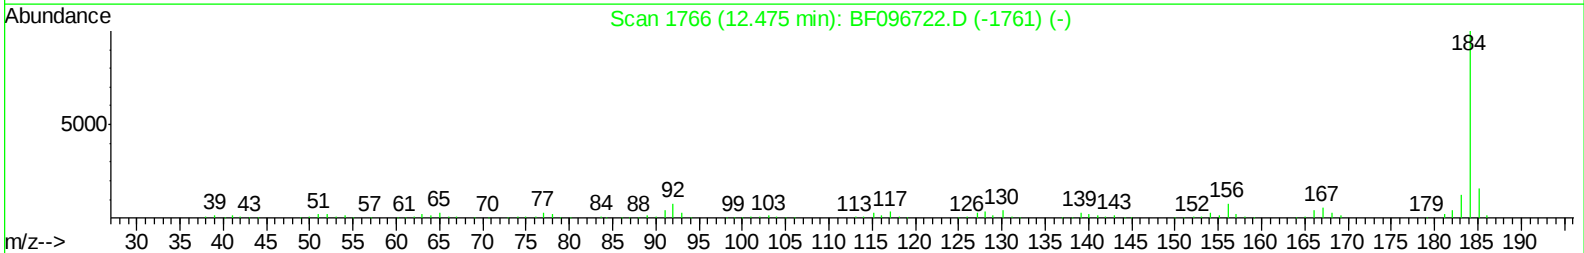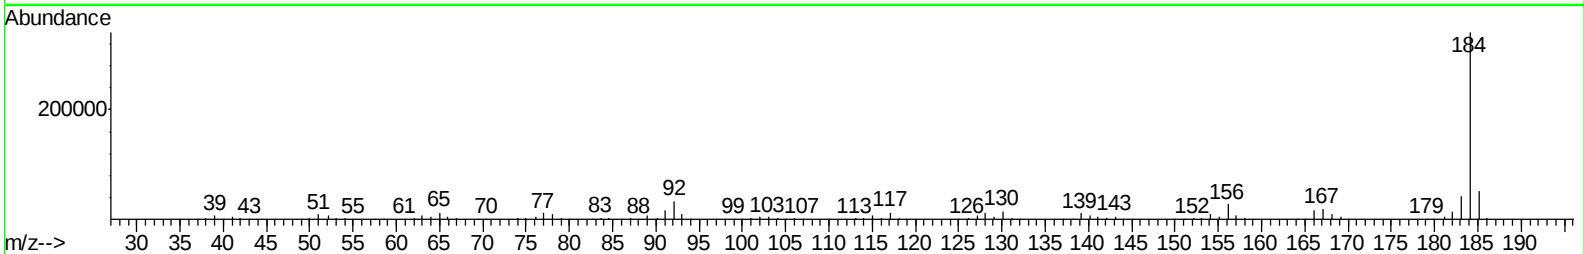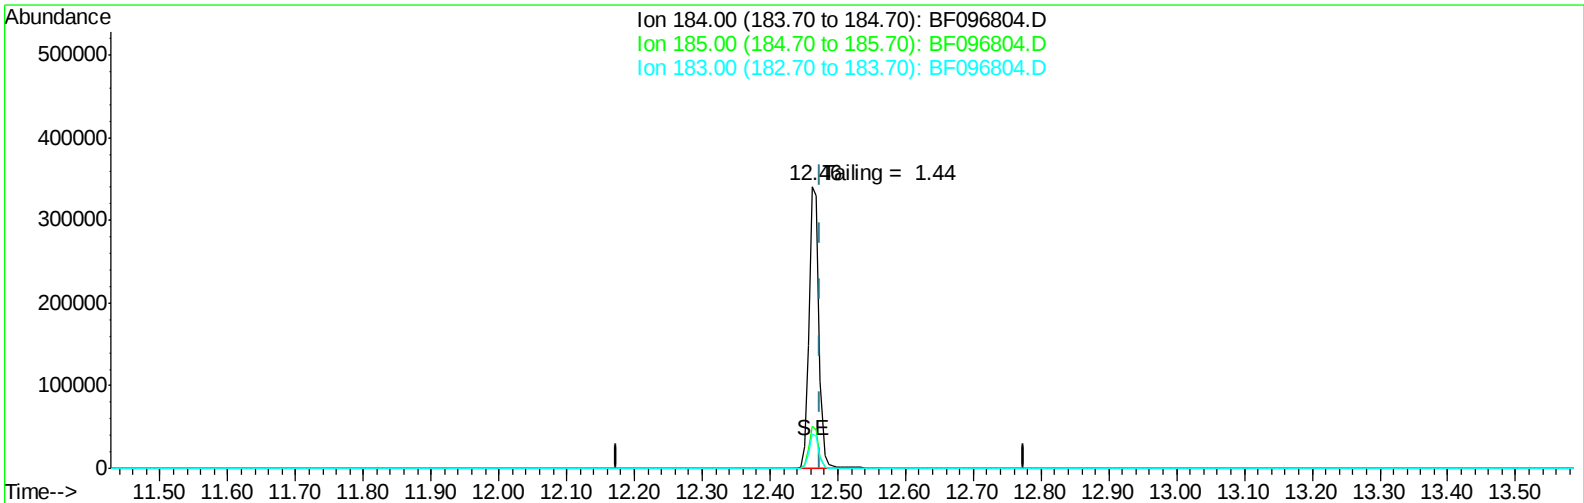

TIC: BF096804.D

(76) Benzidine

12.463min (-0.012) 0.00ng



response 350043

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	15.08#
183.00	12.20	12.12
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF071417\
Data File : BF096804.D
Acq On : 15 Jul 2017 6:54
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Jul 17 01:46:50 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF071317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 13 14:49:34 2017
Response via : Initial Calibration

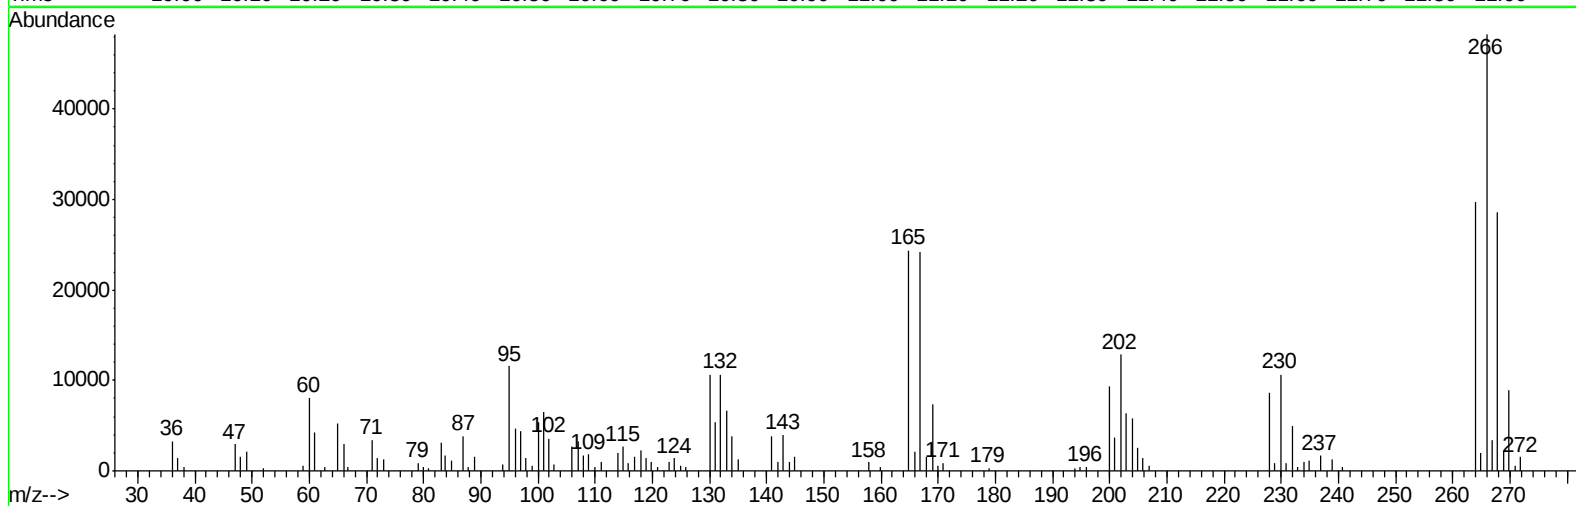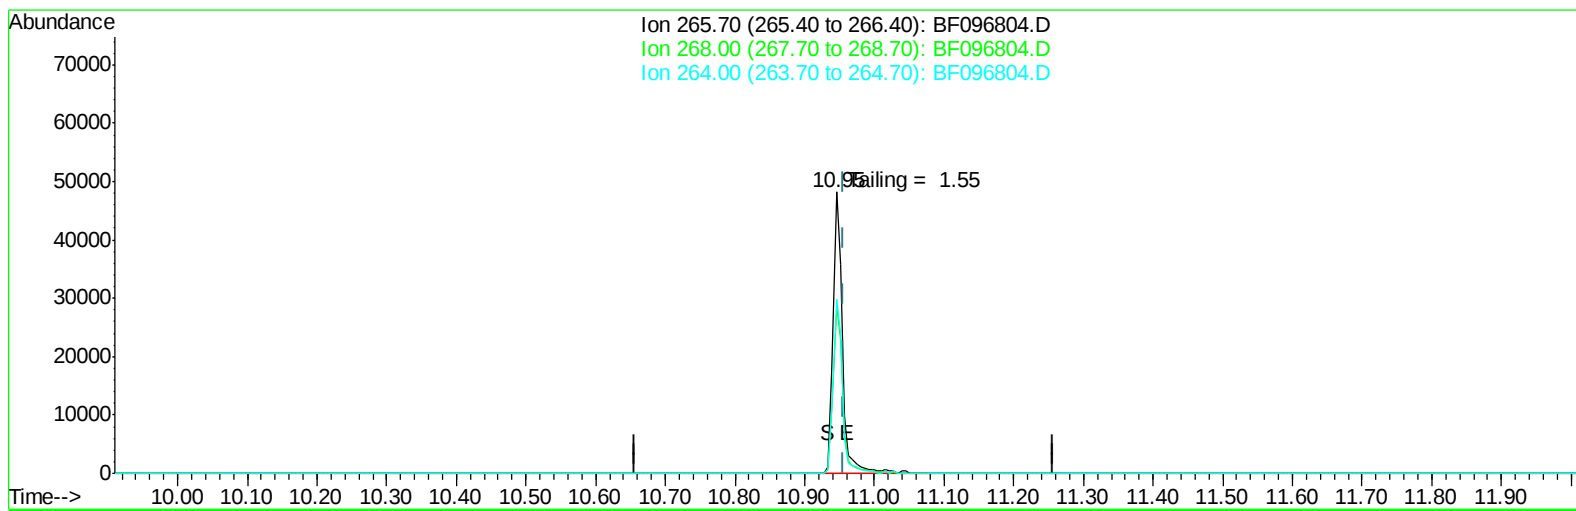

TIC: BF096804.D

(69) Pentachlorophenol (C)

10.945min (-0.012) 0.00ng



response 43632

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	59.10
264.00	64.60	61.67
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF071417\
Data File : BF096804.D
Acq On : 15 Jul 2017 6:54
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Jul 17 01:46:50 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF071317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 13 14:49:34 2017
Response via : Initial Calibration

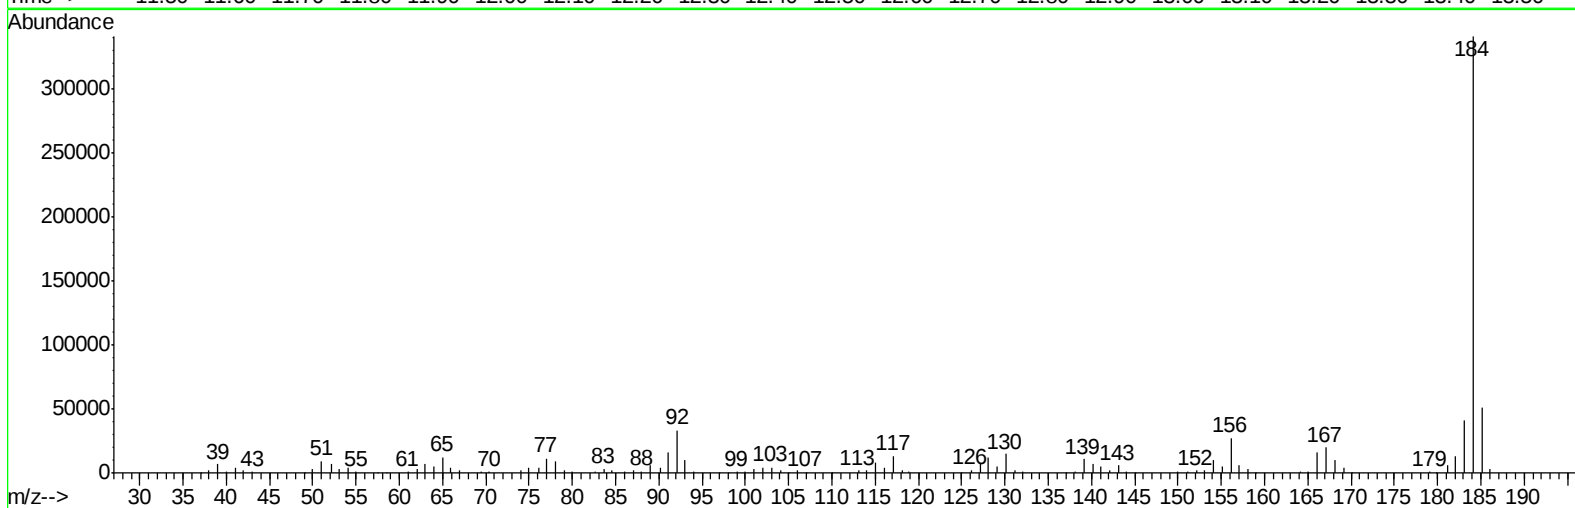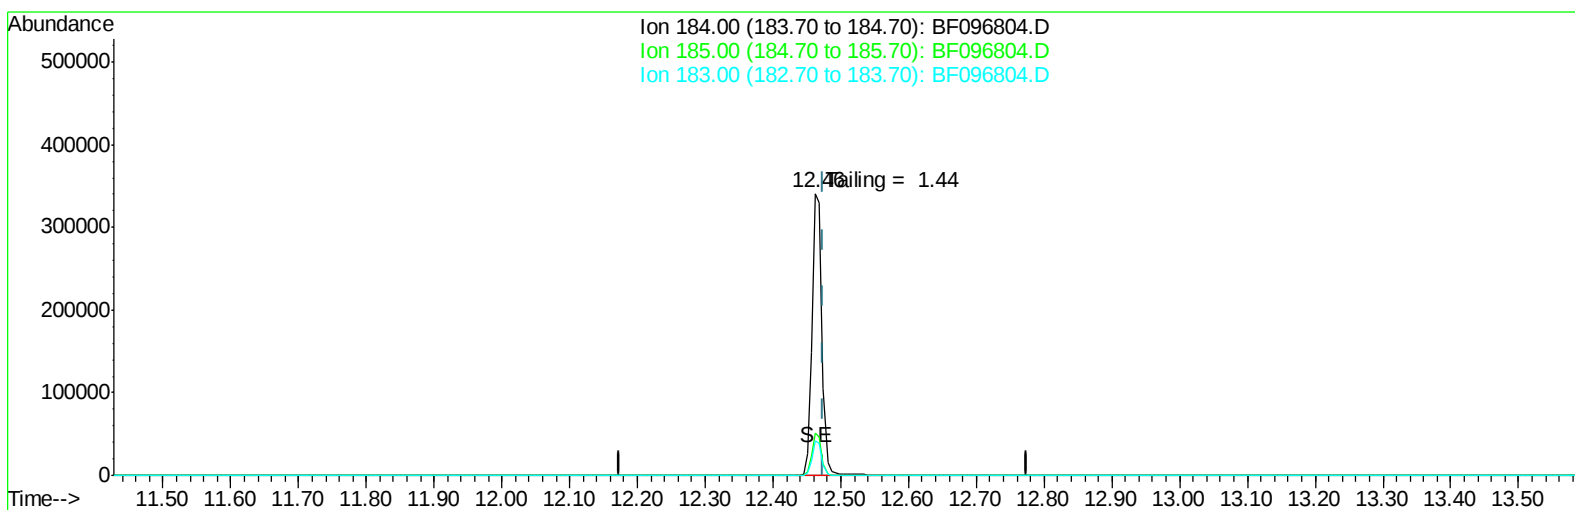

TIC: BF096804.D

(76) Benzidine

12.463min (-0.012) 0.00ng

response 350043

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	15.08#
183.00	12.20	12.12
0.00	0.00	0.00