
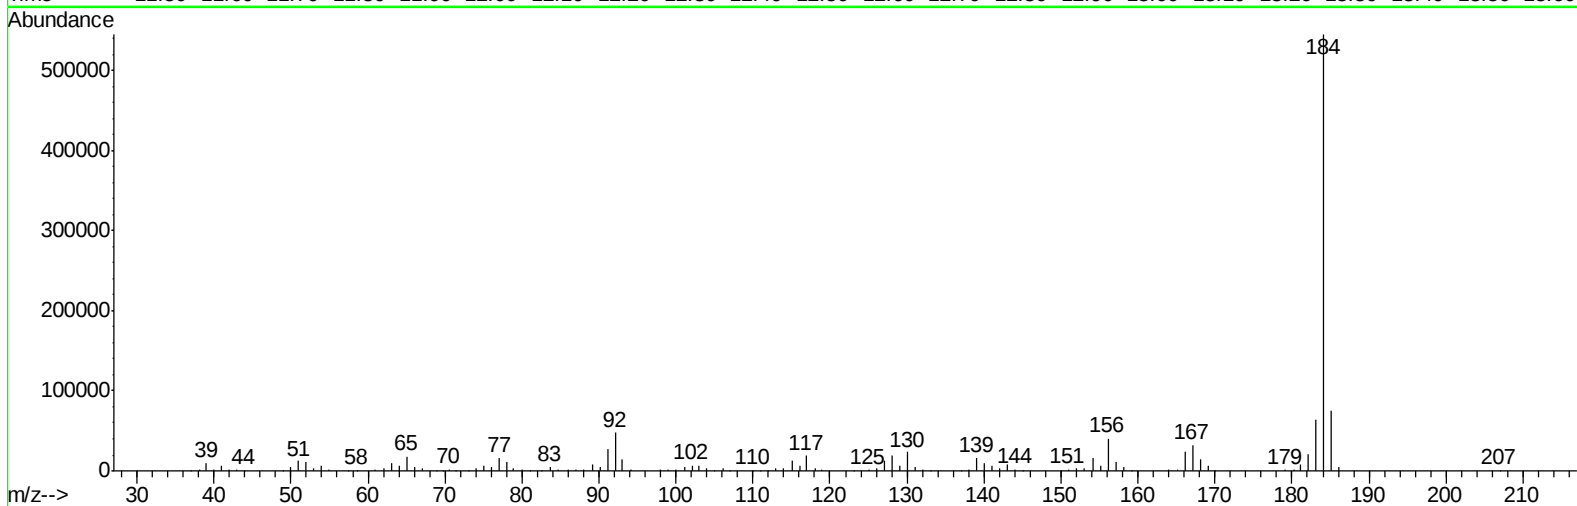


Data Path : Z:\HPCHEM1\BNA F\DATA\BF071417\
Data File : BF096764.D
Acq On : 14 Jul 2017 9:41
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 15 06:01:54 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF071317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 13 14:49:34 2017
Response via : Initial Calibration

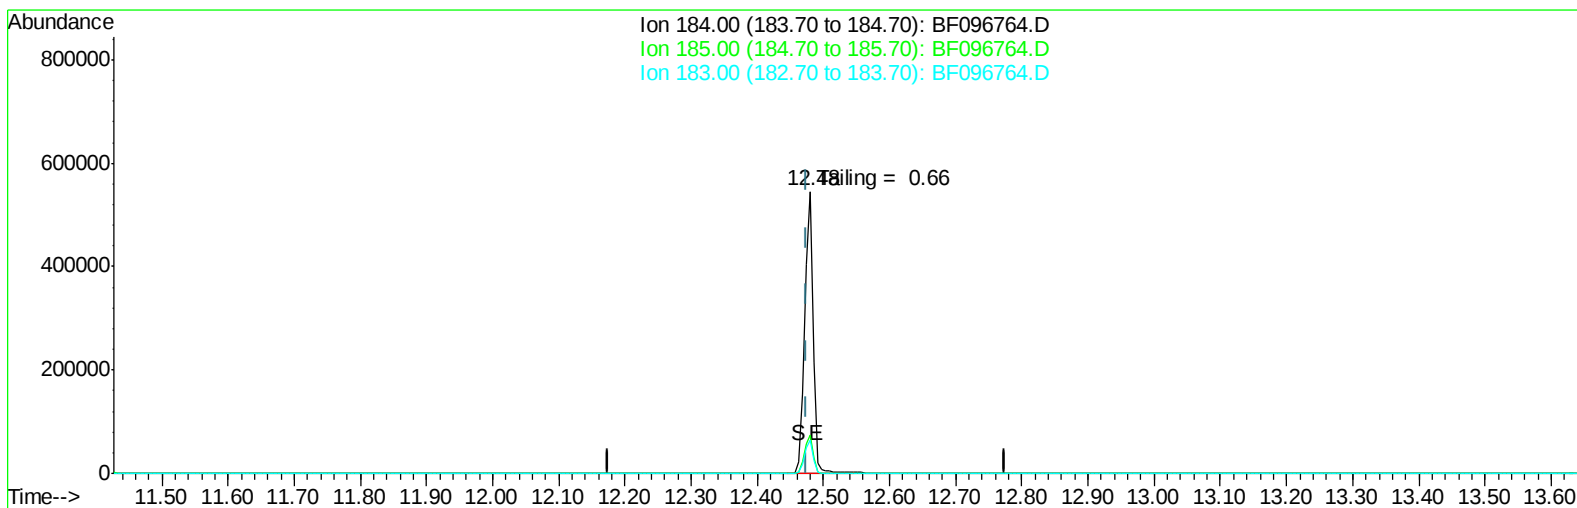

TIC: BF096764.D

(76) Benzidine



12.480min (+0.006) 36718.61ng

response 495602

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	13.83#
183.00	12.20	11.74
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF071417\
Data File : BF096764.D
Acq On : 14 Jul 2017 9:41
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 15 06:01:54 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF071317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 13 14:49:34 2017
Response via : Initial Calibration

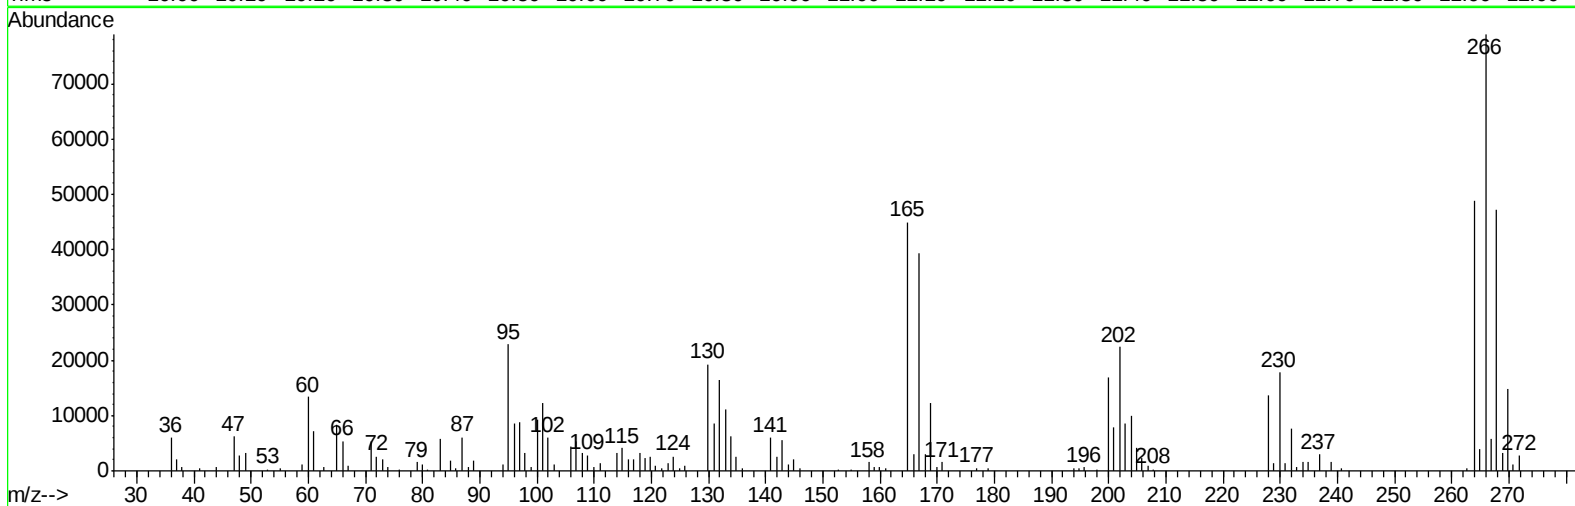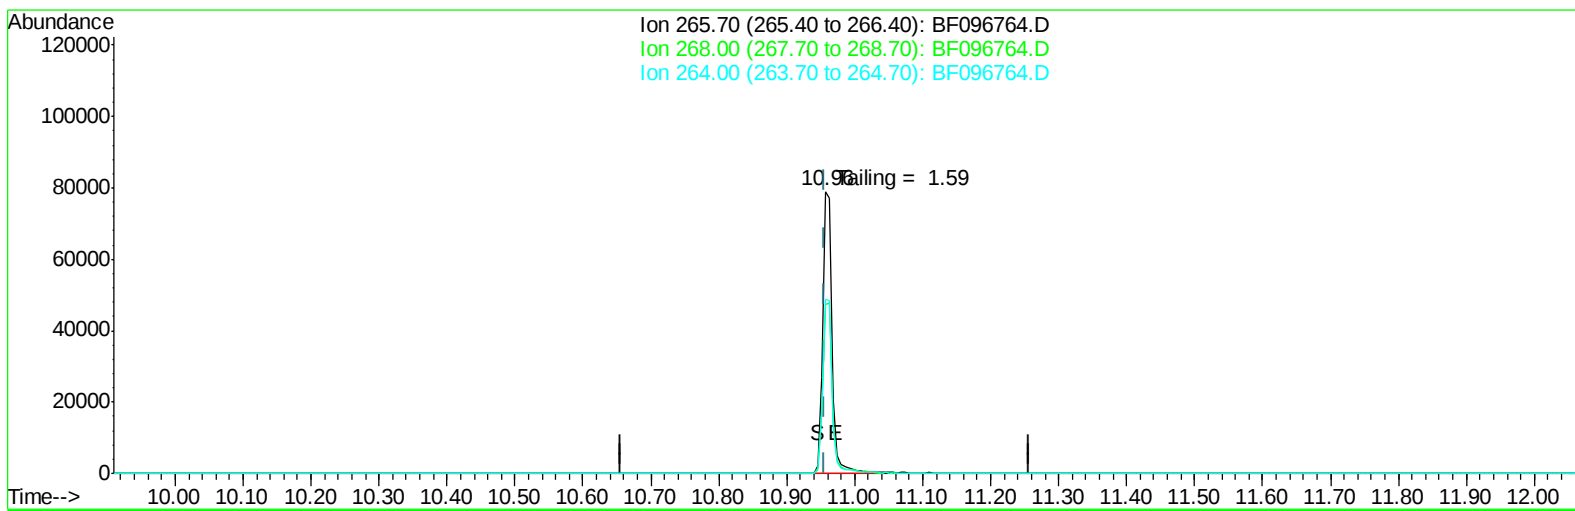

TIC: BF096764.D

(69) Pentachlorophenol (C)

10.957min (-0.000) 0.00ng

response 78652

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	59.92
264.00	64.60	61.77
0.00	0.00	0.00