


Data Path : Z:\HPCHEM1\BNA_F\Data\BF071417\
 Data File : BF096764.D
 Acq On : 14 Jul 2017 9:41
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF071317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 18 13:33:22 2017

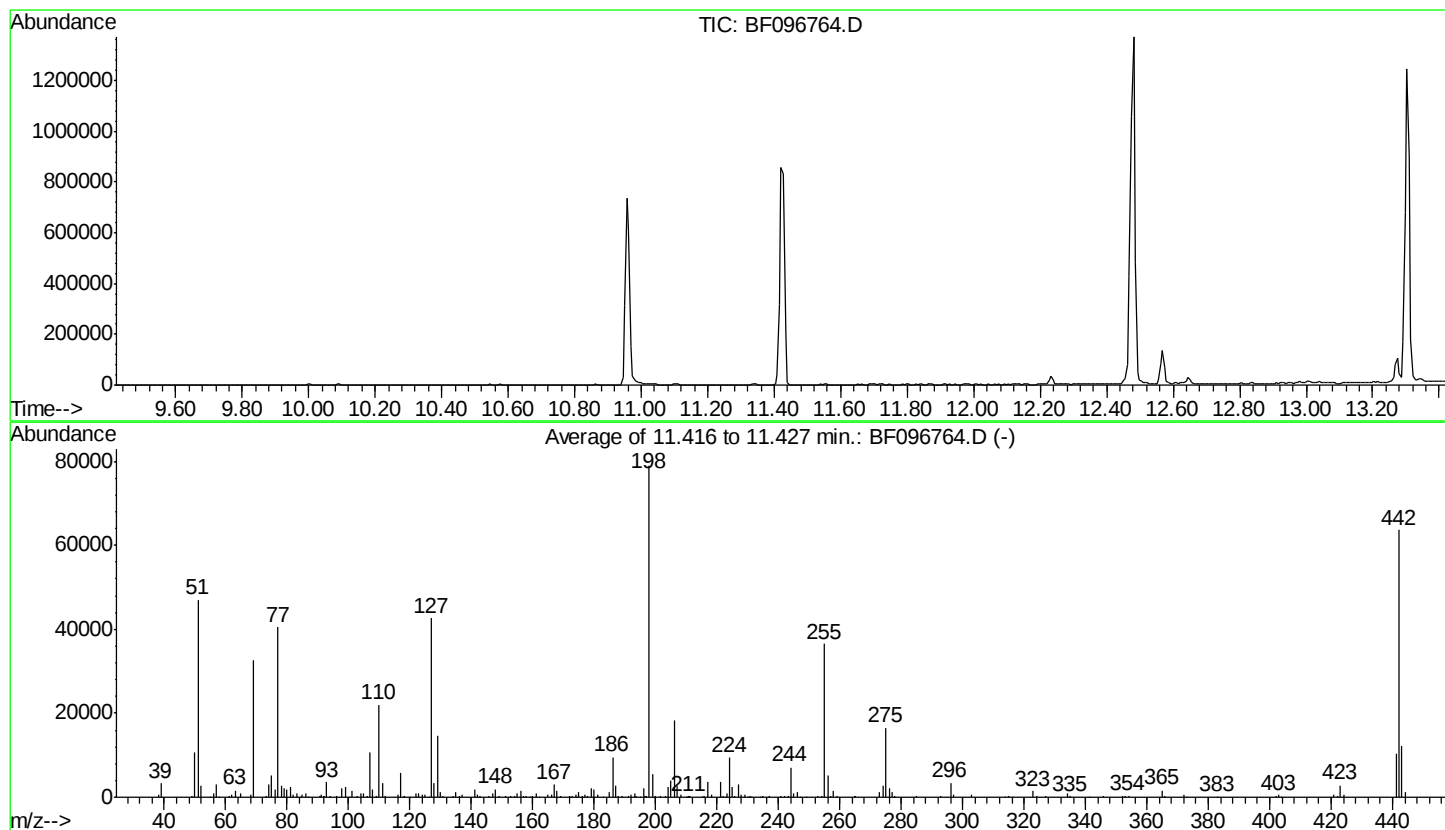

AutoFind: Scans 1603, 1604, 1605; Background Corrected with Scan 1598

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	59.5	46986	PASS
68	69	0.00	2	2.0	656	PASS
69	198	0.00	100	41.3	32602	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	54.0	42674	PASS
197	198	0.00	2	0.5	398	PASS
198	198	100	100	100.0	78989	PASS
199	198	5	9	7.0	5534	PASS
275	198	10	60	20.9	16540	PASS
365	198	1	100	2.1	1670	PASS
441	442	0.01	24	16.4	10453	PASS
442	198	50	100	80.6	63700	PASS
443	442	15	24	19.4	12333	PASS