


Data Path : Z:\HPCHEM1\BNA_F\Data\BF071417\
Data File : BF096778.D
Acq On : 14 Jul 2017 18:16
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF071317.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jul 13 14:49:34 2017

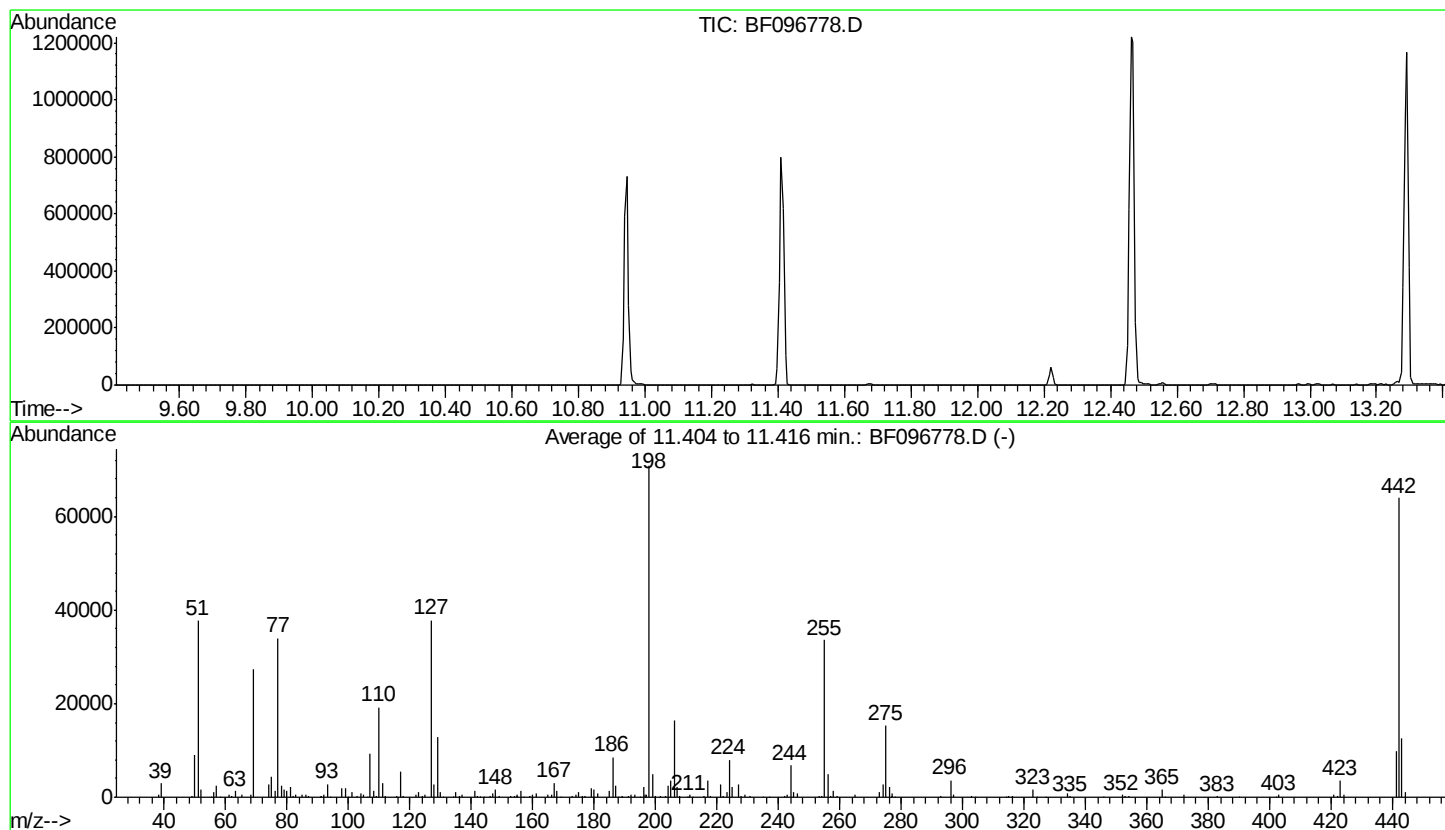

AutoFind: Scans 1601, 1602, 1603; Background Corrected with Scan 1596

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	53.2	37722	PASS
68	69	0.00	2	1.8	493	PASS
69	198	0.00	100	38.6	27373	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.4	37842	PASS
197	198	0.00	2	0.7	466	PASS
198	198	100	100	100.0	70861	PASS
199	198	5	9	6.9	4865	PASS
275	198	10	60	21.5	15221	PASS
365	198	1	100	2.2	1581	PASS
441	442	0.01	24	15.6	9948	PASS
442	198	50	100	90.2	63938	PASS
443	442	15	24	19.8	12660	PASS