


Data Path : Z:\HPCHEM1\BNA_F\Data\BF071417\
 Data File : BF096804.D
 Acq On : 15 Jul 2017 6:54
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF071317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 13 14:49:34 2017

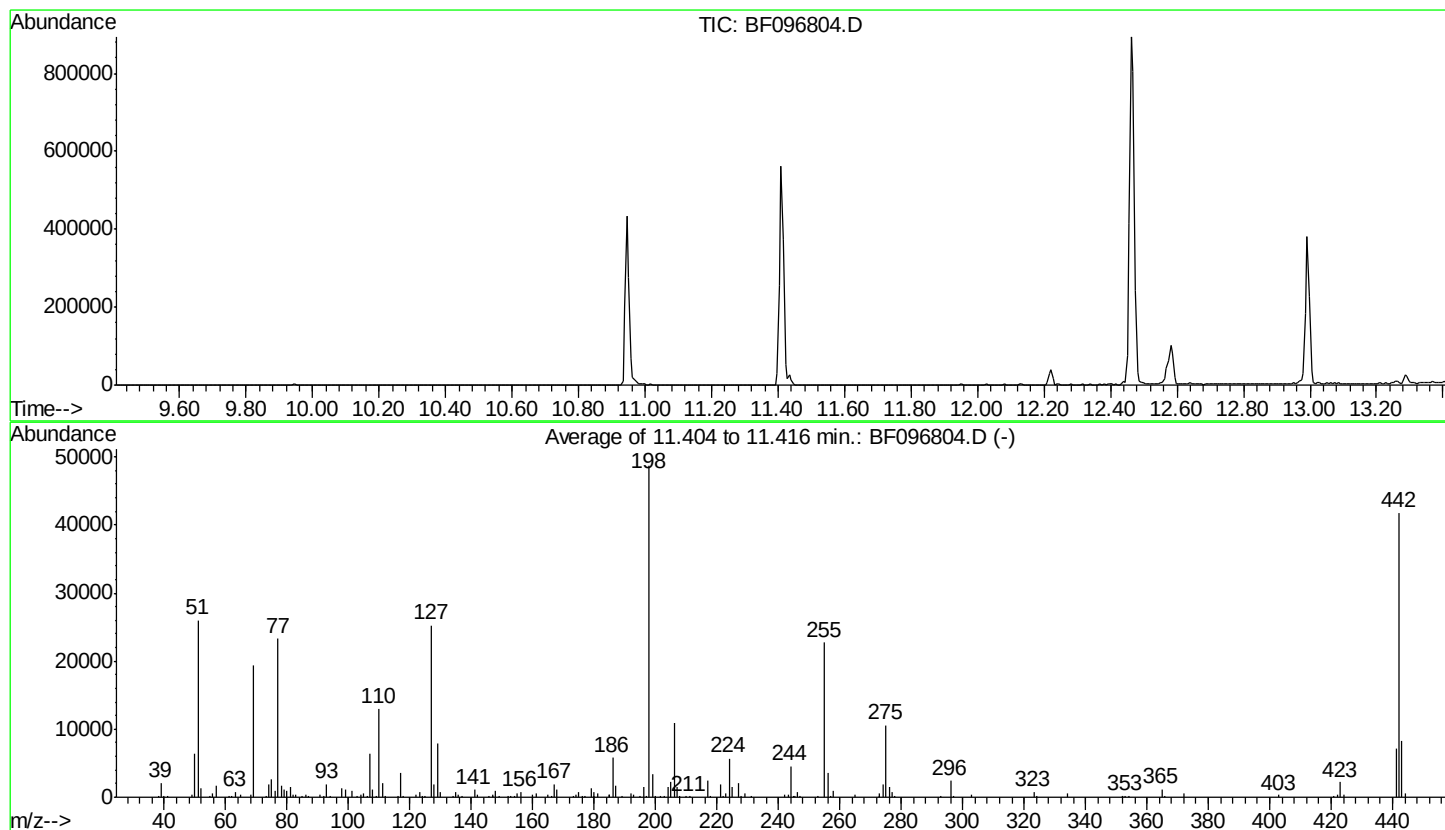

AutoFind: Scans 1601, 1602, 1603; Background Corrected with Scan 1597

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	53.4	26026	PASS
68	69	0.00	2	2.0	394	PASS
69	198	0.00	100	39.7	19338	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.9	25272	PASS
197	198	0.00	2	0.2	114	PASS
198	198	100	100	100.0	48722	PASS
199	198	5	9	6.9	3354	PASS
275	198	10	60	21.7	10581	PASS
365	198	1	100	2.3	1135	PASS
441	442	0.01	24	17.1	7161	PASS
442	198	50	100	85.8	41816	PASS
443	442	15	24	19.8	8288	PASS