
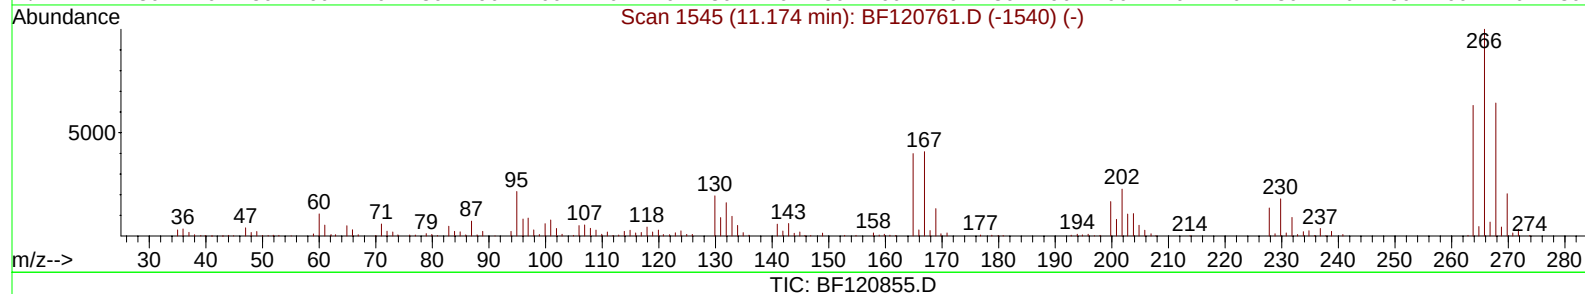
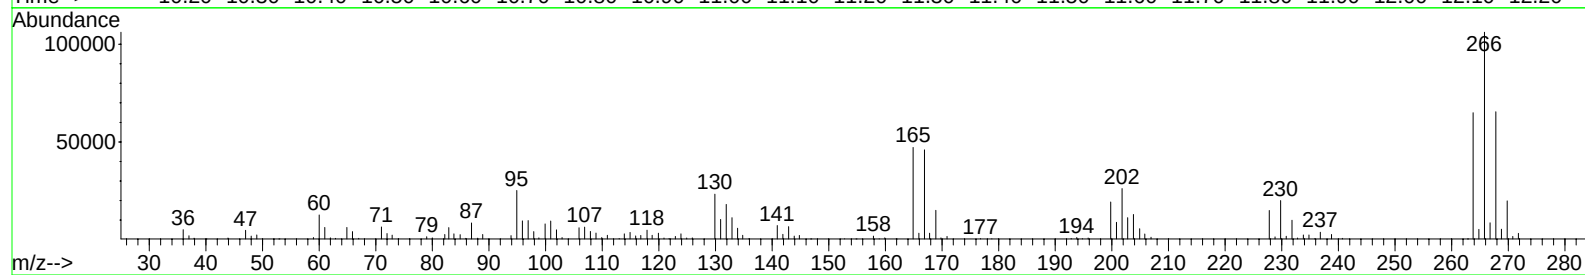


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF071420\
 Data File : BF120855.D
 Acq On : 14 Jul 2020 11:42
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 14 16:10:38 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF070220.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 13 14:16:14 2020
 Response via : Initial Calibration

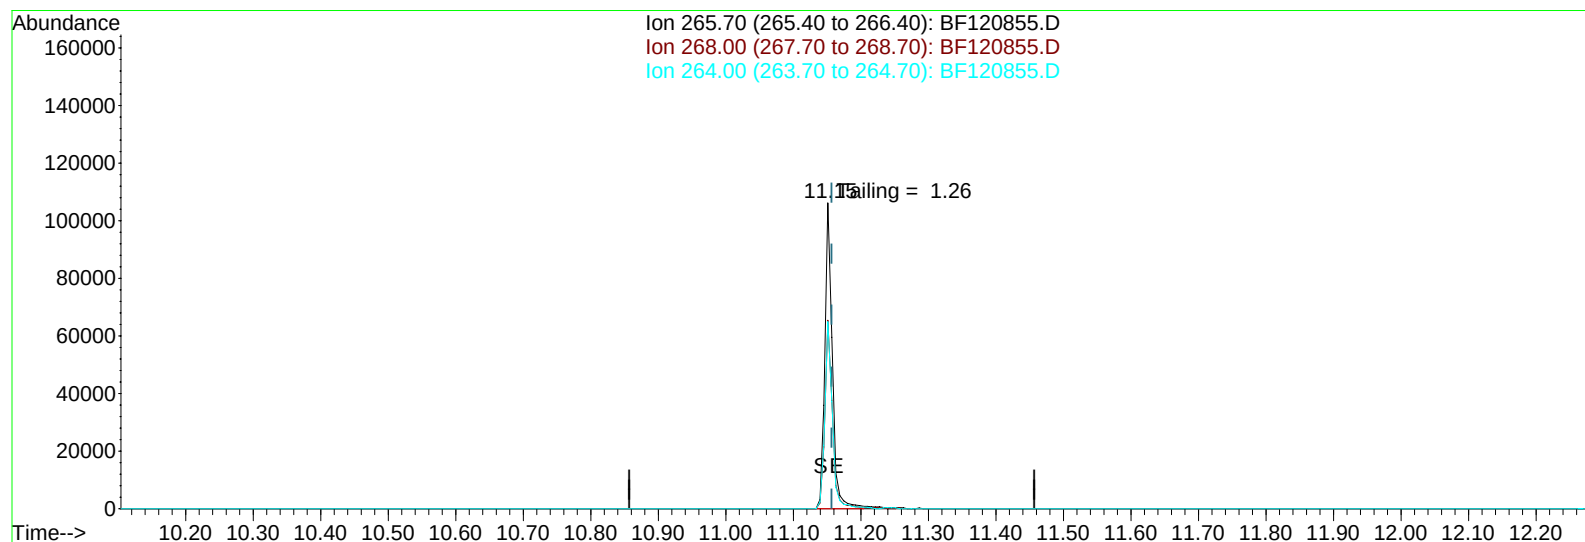

(70) Pentachlorophenol (C)




11.151min (-0.006) 34707.65ng

response 83421

Ion	Exp%	Act%
265.70	100	100
268.00	64.30	61.64
264.00	63.20	61.20
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF071420\
 Data File : BF120855.D
 Acq On : 14 Jul 2020 11:42
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 14 16:10:38 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF070220.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 13 14:16:14 2020
 Response via : Initial Calibration

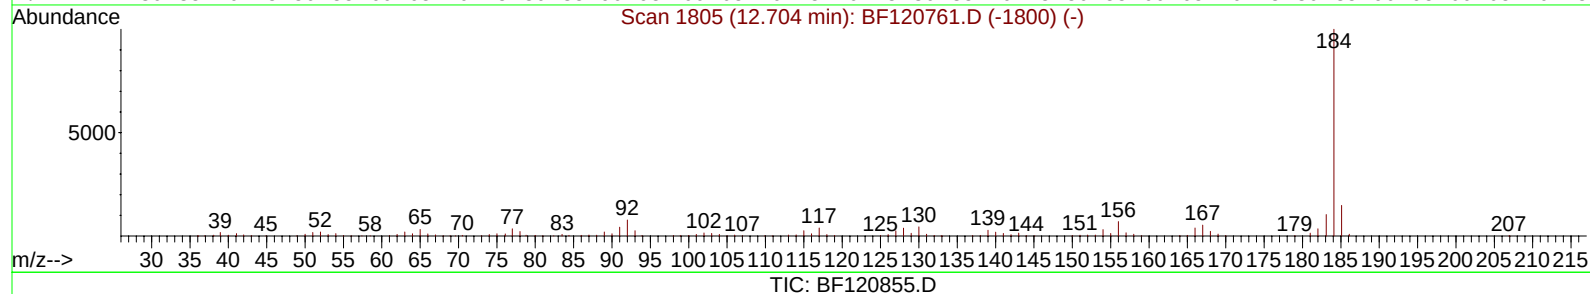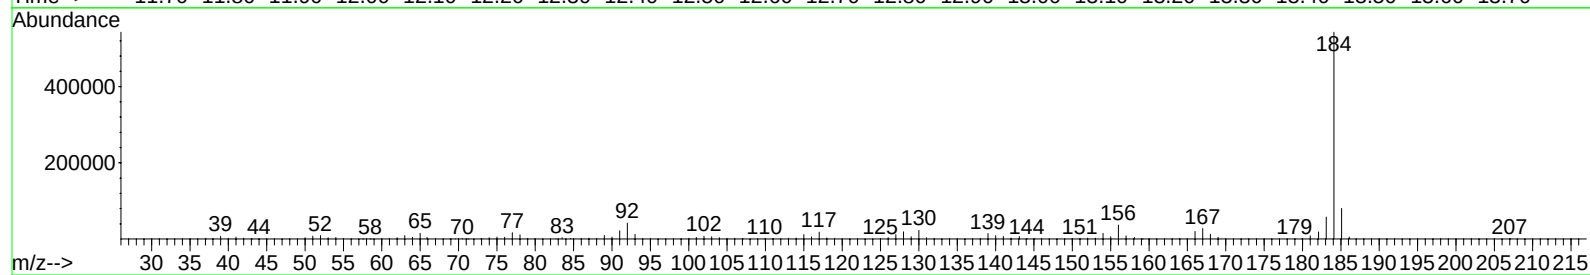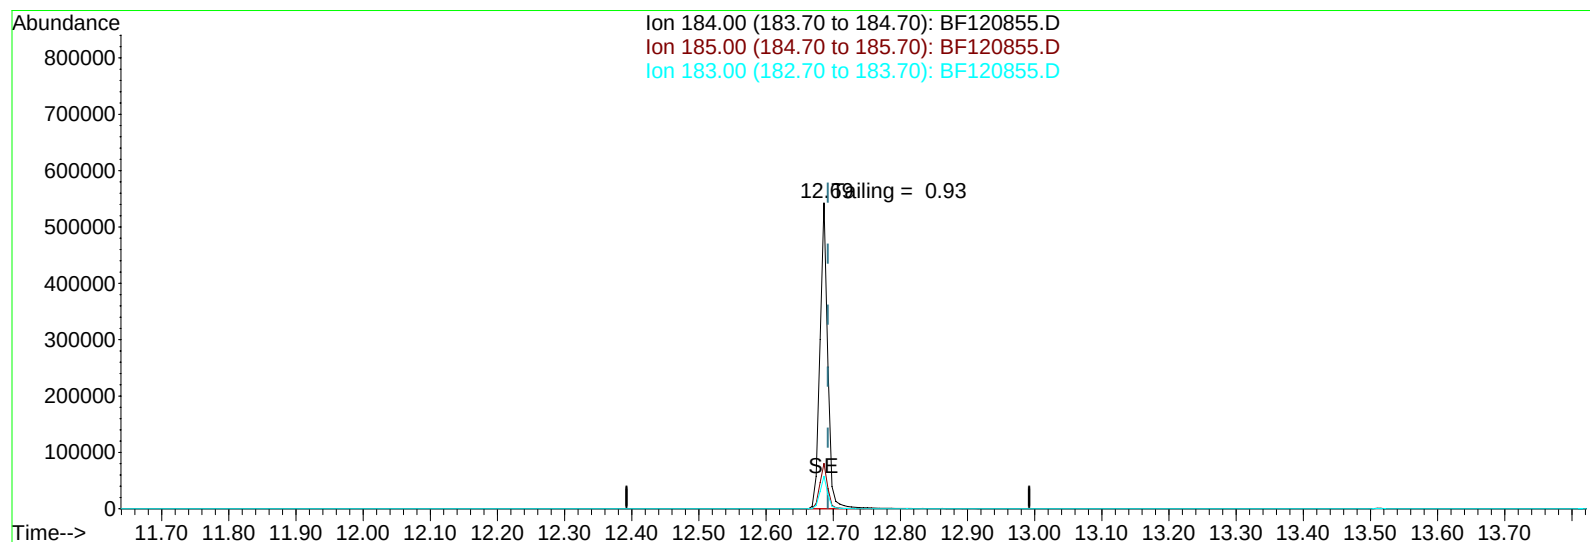

(77) Benzidine

12.686min (-0.006) 0.00ng

response 439940

Ion	Exp%	Act%
184.00	100	100
185.00	14.80	14.82
183.00	10.40	10.63
0.00	0.00	0.00