


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071420\
 Data File : BF120855.D
 Acq On : 14 Jul 2020 11:42
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070220.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jul 13 14:16:14 2020

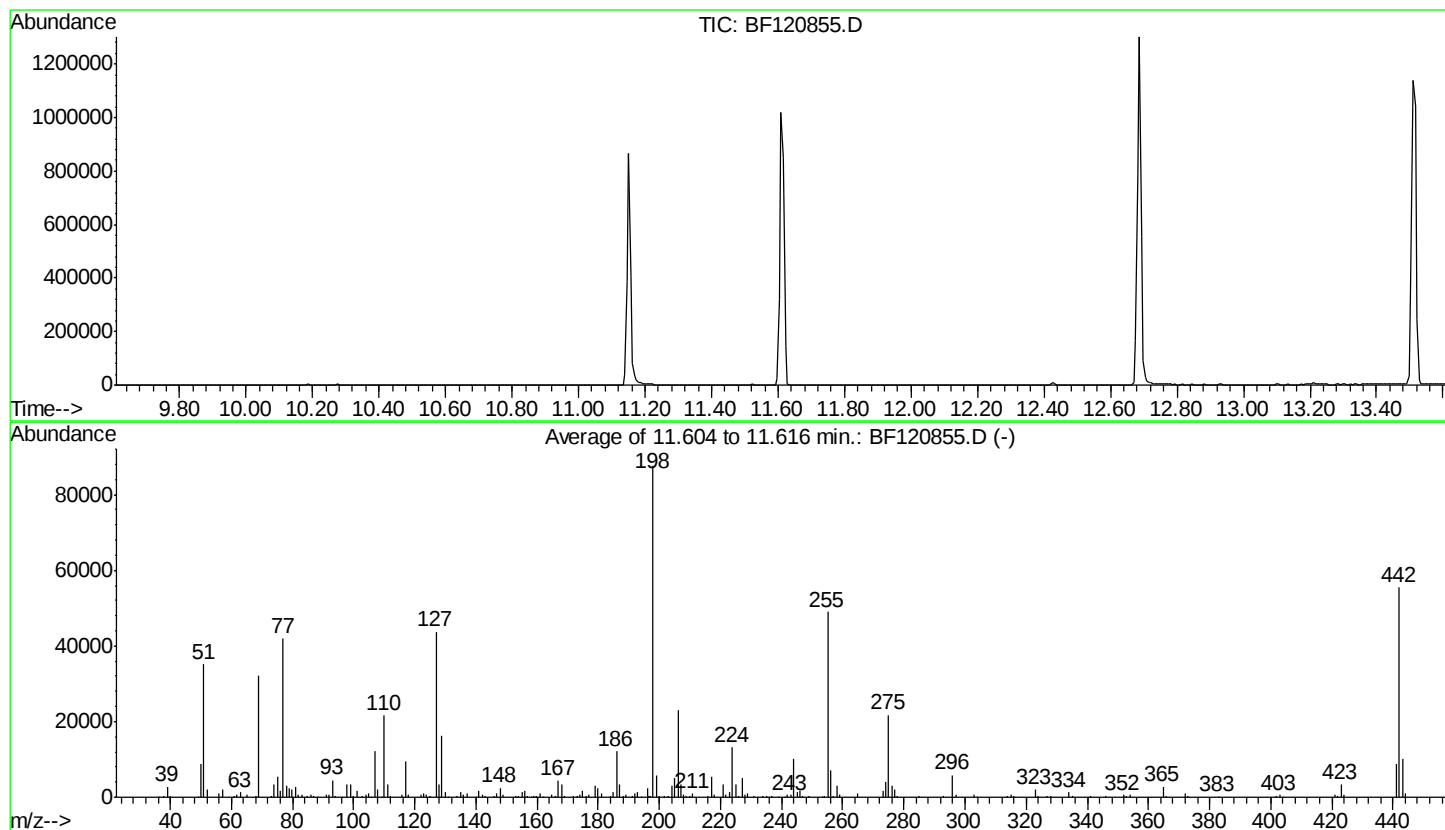

AutoFind: Scans 1618, 1619, 1620; Background Corrected with Scan 1614

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.1	35178	PASS
68	69	0.00	2	1.5	490	PASS
69	198	0.00	100	36.6	32112	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.8	43658	PASS
197	198	0.00	2	0.4	382	PASS
198	198	100	100	100.0	87666	PASS
199	198	5	9	6.7	5866	PASS
275	198	10	60	24.8	21773	PASS
365	198	1	100	3.2	2845	PASS
441	198	0.01	100	9.9	8676	PASS
442	198	50	100	63.3	55454	PASS
443	442	15	24	18.1	10018	PASS