

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071421\
 Data File : BF124563.D
 Acq On : 14 Jul 2021 14:19
 Operator : JU/CG
 Sample : PB137690BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB137690BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF124563.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.204	527	530	535	rBB	2310	3517	1.10%	0.202%
2	5.563	585	591	593	rBB	207156	222110	69.51%	12.782%
3	6.545	752	758	761	rBB	171238	227248	71.12%	13.078%
4	6.922	819	822	825	rBB	51749	44220	13.84%	2.545%
5	7.487	912	918	921	rBB	128526	148518	46.48%	8.547%
6	8.204	1036	1040	1043	rBB	67237	62435	19.54%	3.593%
7	9.286	1218	1224	1227	rBB	315089	299800	93.83%	17.253%
8	9.963	1335	1339	1342	rBB	84065	72211	22.60%	4.156%
9	10.757	1469	1474	1477	rBB	193403	173605	54.33%	9.991%
10	11.451	1588	1592	1595	rBV	94427	74870	23.43%	4.309%
11	13.045	1858	1863	1866	rBV	309420	319524	100.00%	18.388%
12	14.092	2037	2041	2044	rBB	65122	52453	16.42%	3.019%
13	15.586	2290	2295	2299	rBB	32206	37185	11.64%	2.140%




Sum of corrected areas: 1737696

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071421\
Data File : BF124563.D
Acq On : 14 Jul 2021 14:19
Operator : JU/CG
Sample : PB137690BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB137690BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

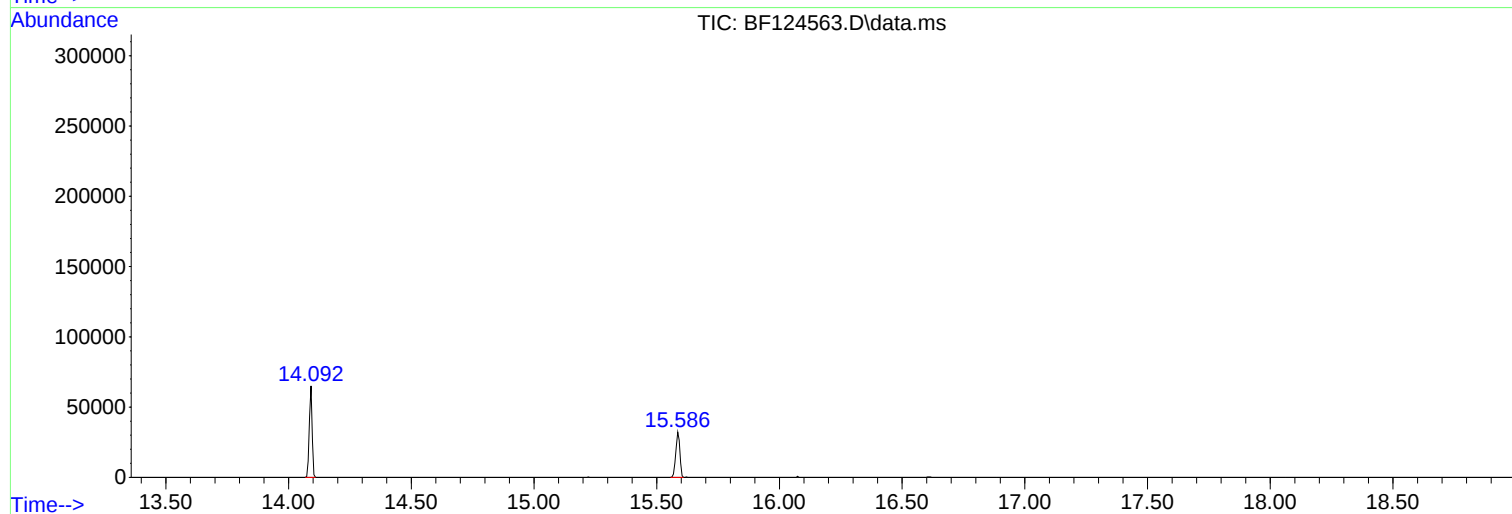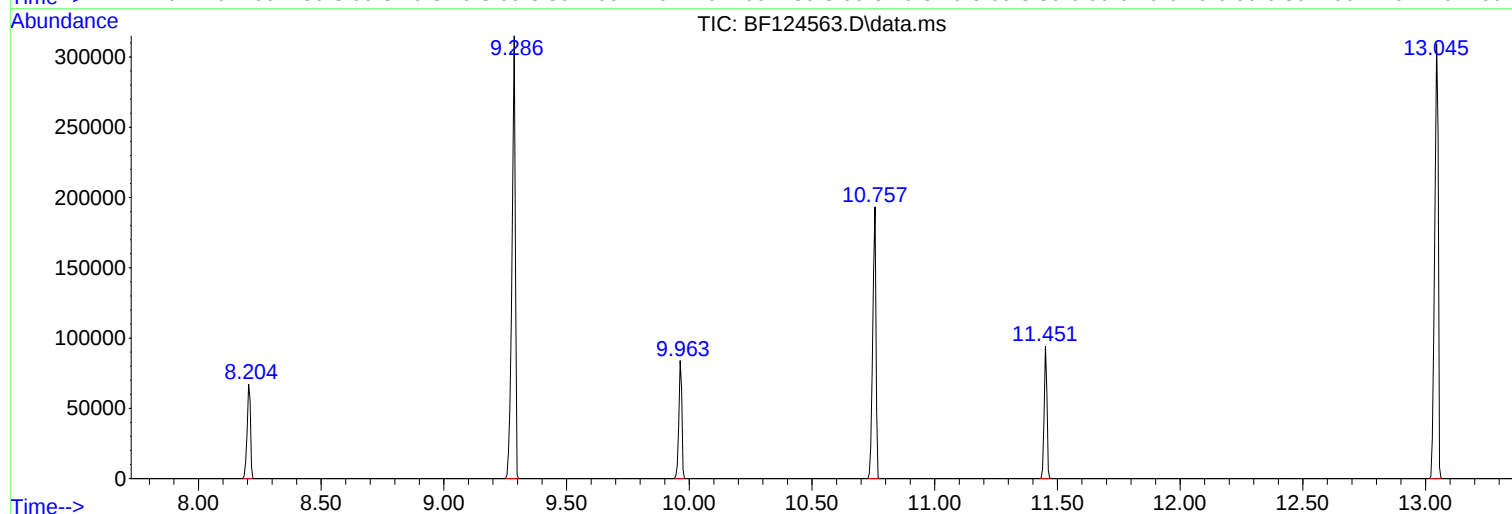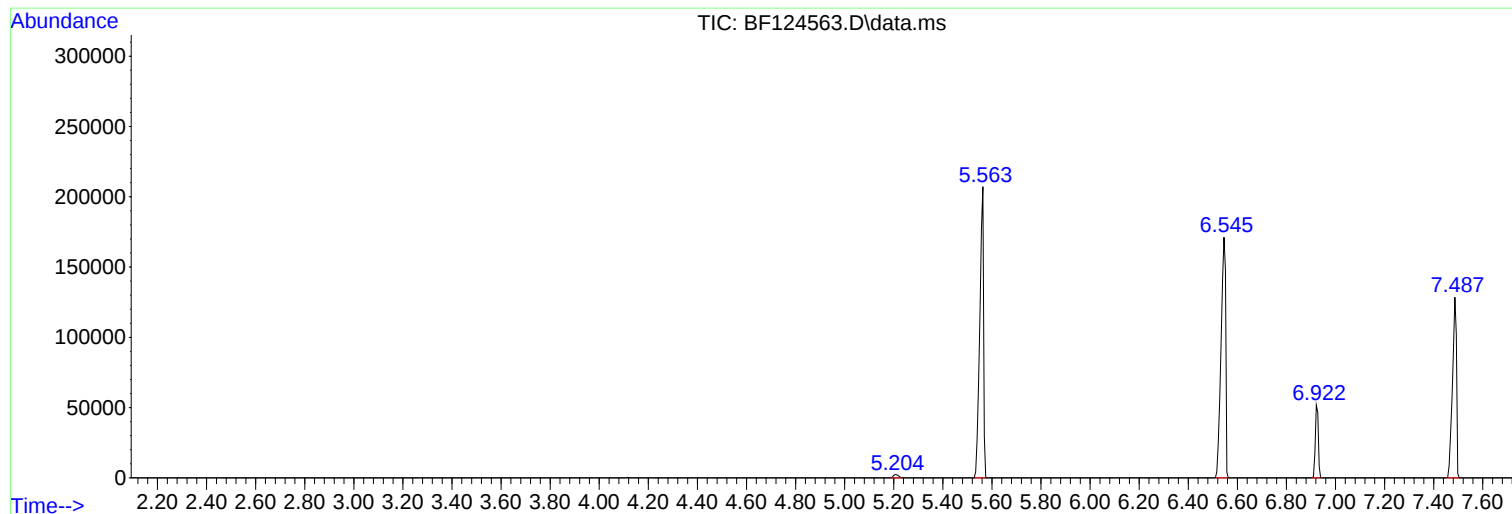

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071421\
Data File : BF124563.D
Acq On : 14 Jul 2021 14:19
Operator : JU/CG
Sample : PB137690BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB137690BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071421\
Data File : BF124563.D
Acq On : 14 Jul 2021 14:19
Operator : JU/CG
Sample : PB137690BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB137690BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------