
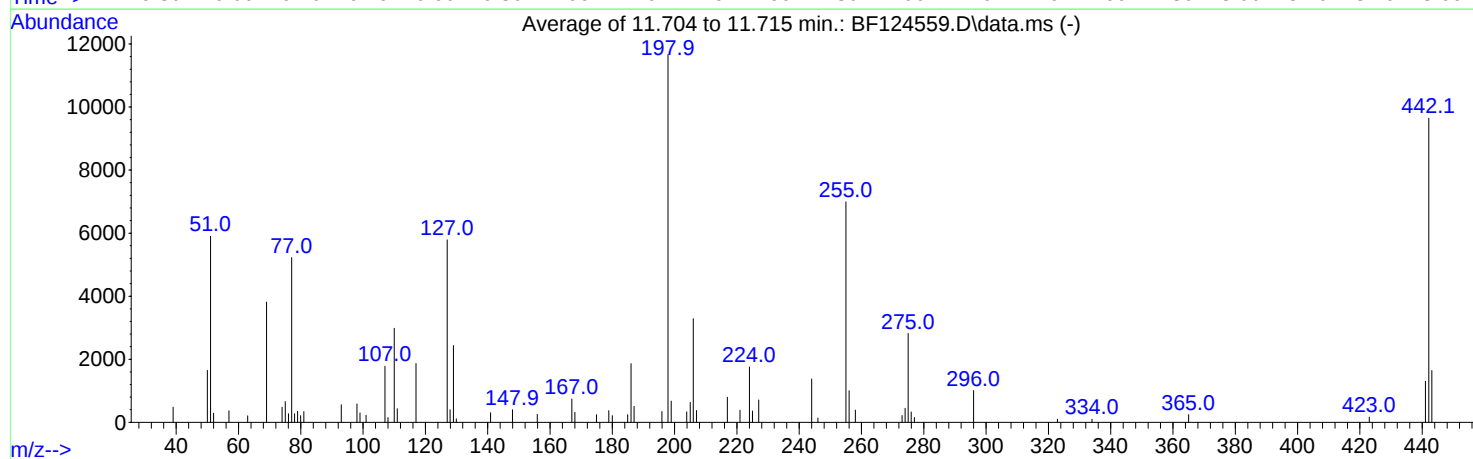


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071421\
 Data File : BF124559.D
 Acq On : 14 Jul 2021 11:50
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 08 07:49:42 2021

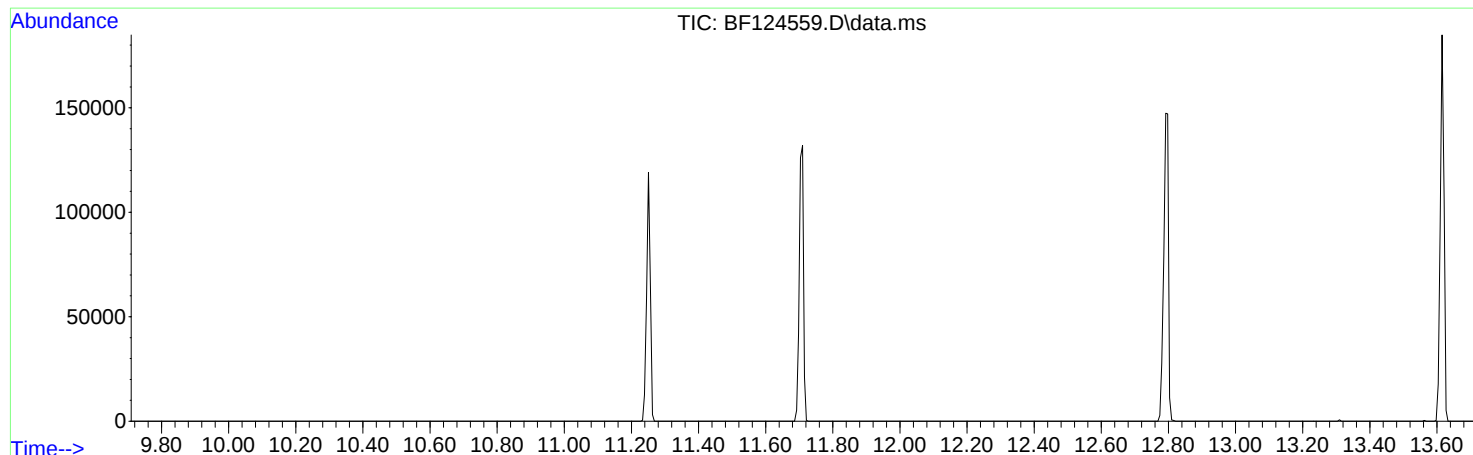




AutoFind: Scans 1635, 1636, 1637; Background Corrected with Scan 1630

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.6	5902	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	32.7	3818	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.6	5791	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	11666	PASS
199	198	5	9	5.8	675	PASS
275	198	10	60	24.2	2820	PASS
365	198	1	100	2.1	242	PASS
441	198	0.01	100	11.2	1306	PASS
442	442	50	100	100.0	9646	PASS
443	442	15	24	17.0	1643	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071421\
Data File : BF124559.D
Acq On : 14 Jul 2021 11:50
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 14 12:33:44 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 08 07:49:42 2021
Response via : Initial Calibration

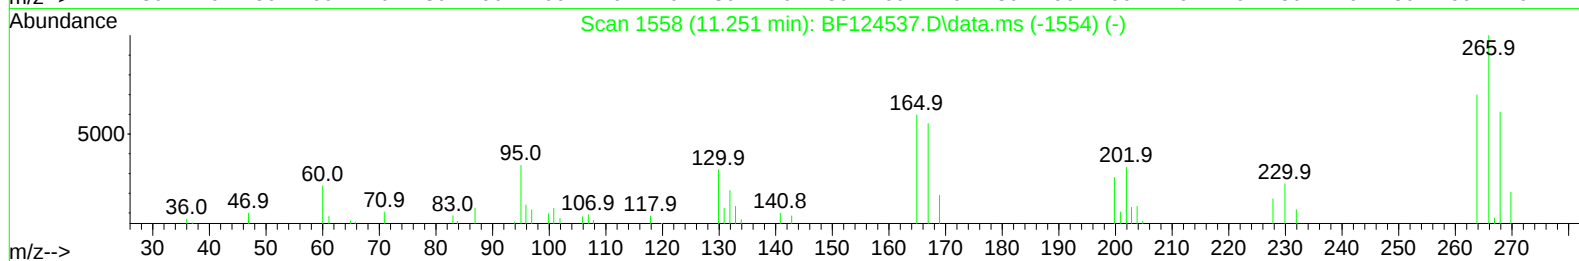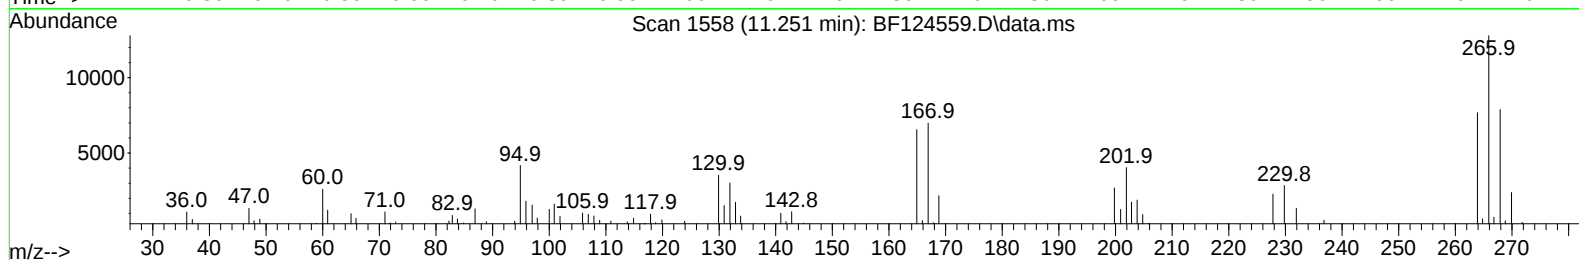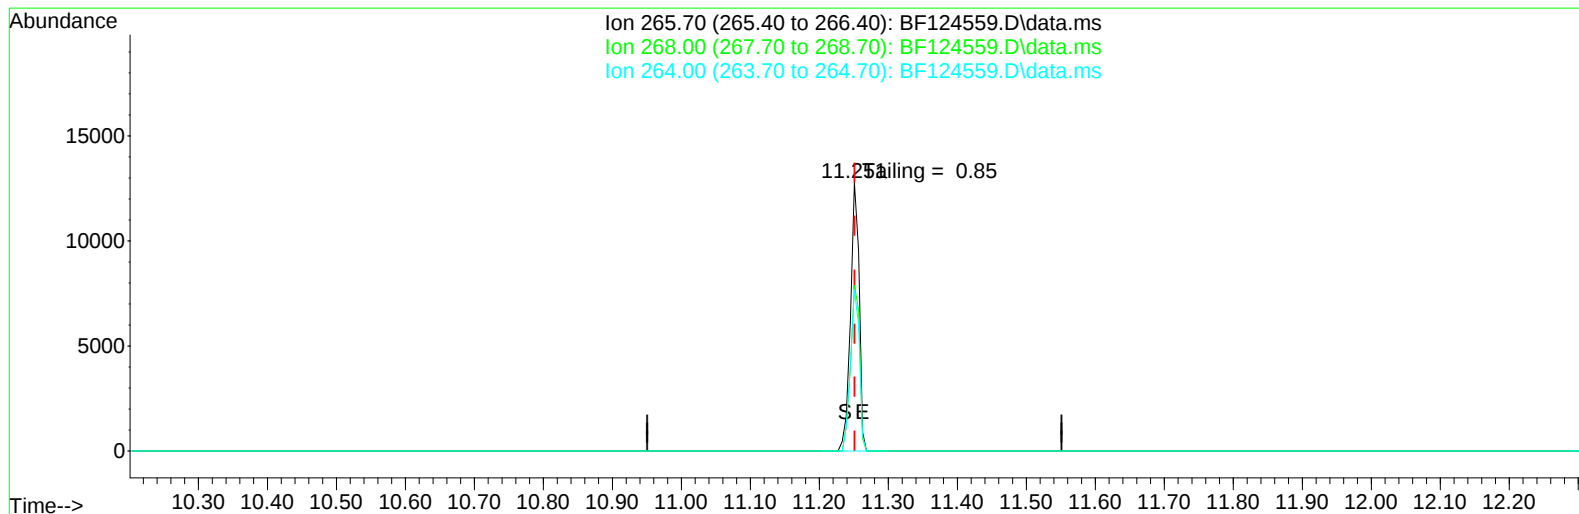

TIC: BF124559.D\data.ms

(70) Pentachlorophenol (C)

11.251min (-0.000) 0.00 ng




response 11143

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	61.70
264.00	69.90	60.07
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071421\
 Data File : BF124559.D
 Acq On : 14 Jul 2021 11:50
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jul 14 12:33:44 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 08 07:49:42 2021
 Response via : Initial Calibration

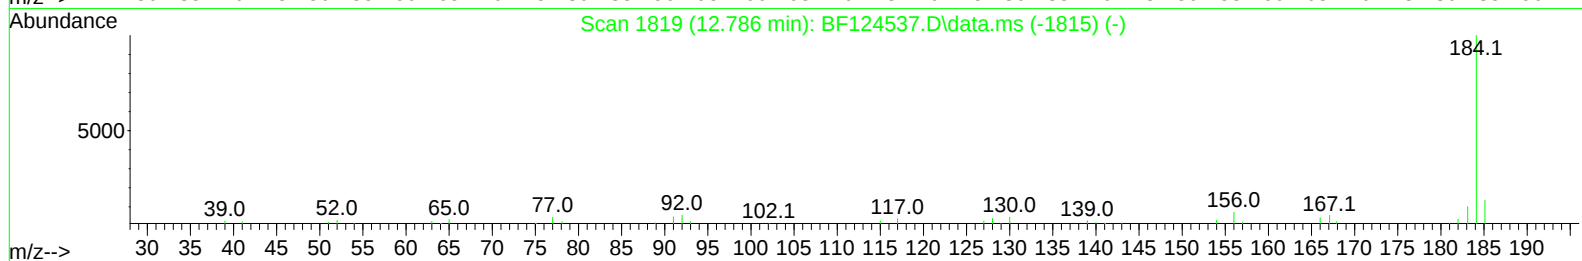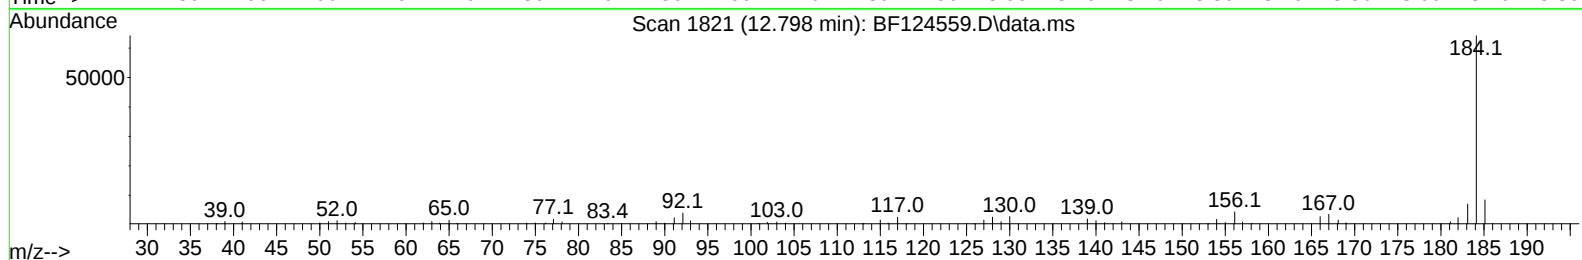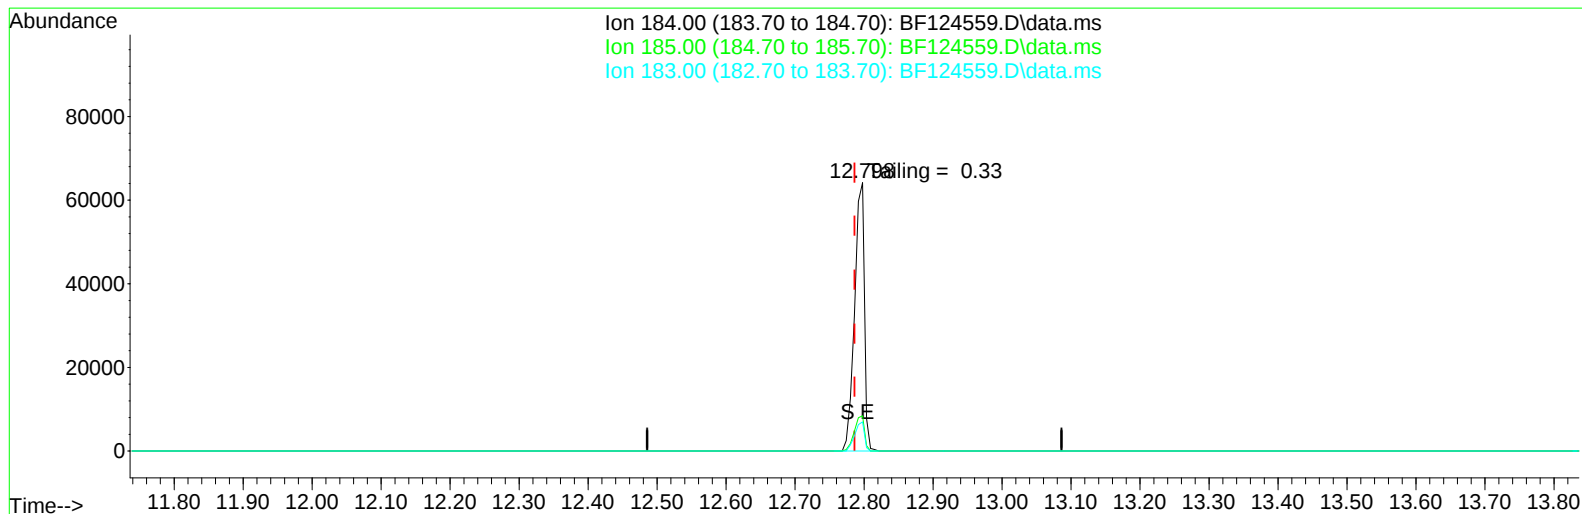

TIC: BF124559.D\data.ms

(77) Benzidine

12.798min (+ 0.012) 0.00 ng

response 63568

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	13.12
183.00	10.10	10.87
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/14/2021	BNA_F	<u>BF124559.D</u>
Compound Name	Response	Retention Time
DDT	27570	13.61
DDD	134	13.3
DDE	0	12.71
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
134	27704	0.48

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP