
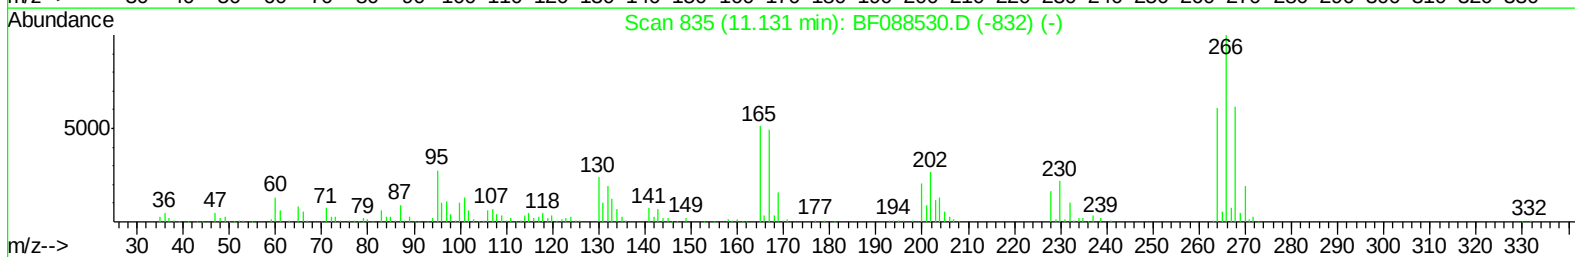
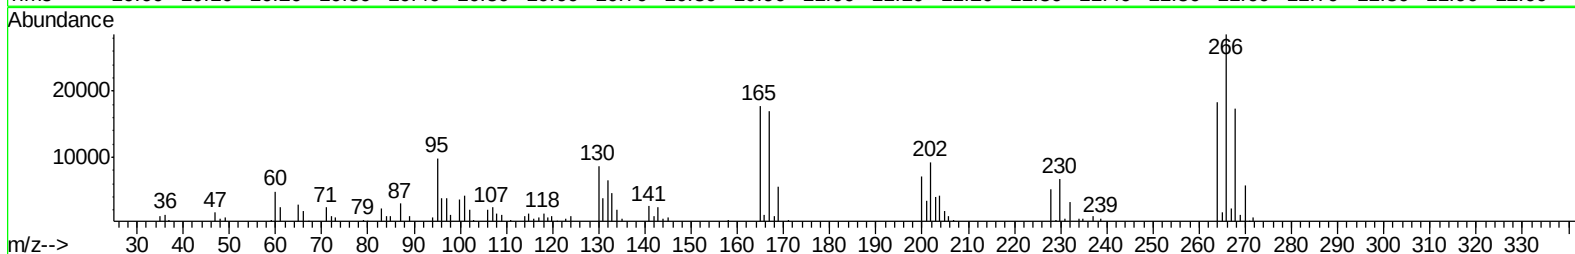


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF071516\
Data File : BF089013.D
Acq On : 15 Jul 2016 12:54
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 16 07:02:57 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 11 18:13:32 2016
Response via : Initial Calibration

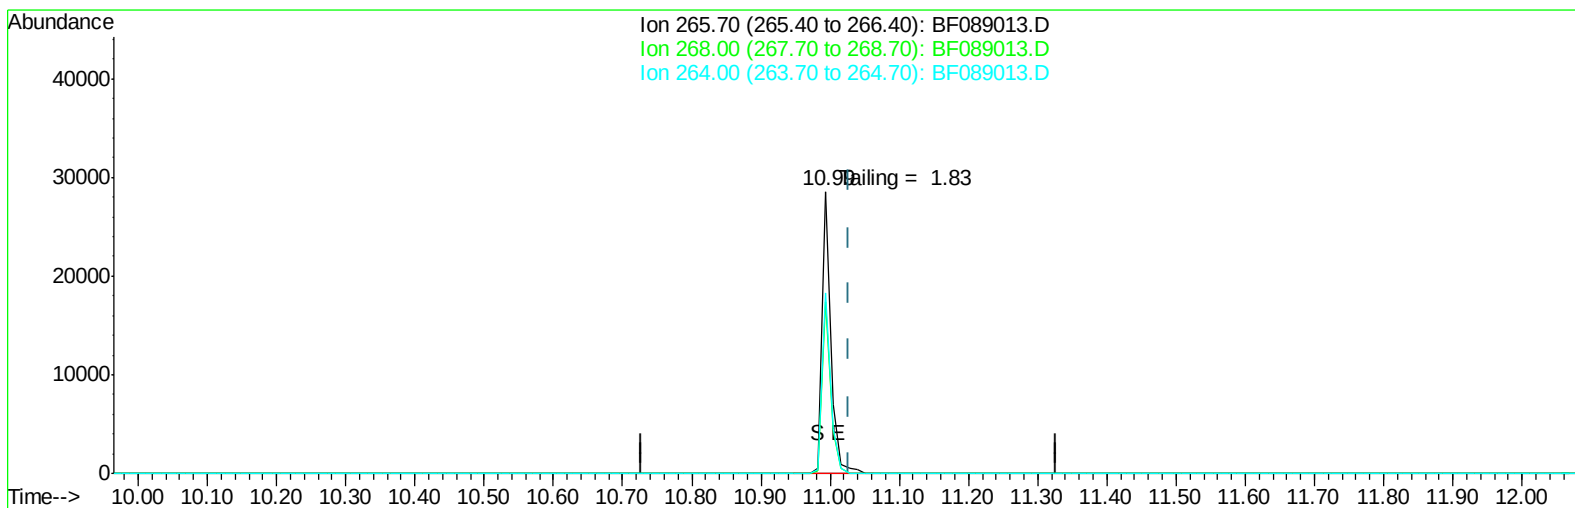

TIC: BF089013.D

(69) Pentachlorophenol (C)

10.993min (-0.034) 0.00ng

response 25922

Ion	Exp%	Act%
265.70	100	100
268.00	66.00	61.04
264.00	62.00	63.93
0.00	0.00	0.00