


Data Path : Z:\HPCHEM1\BNA F\DATA\BF071516\  
 Data File : BF089036.D  
 Acq On : 16 Jul 2016 2:34  
 Operator : UM/SJ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF063016.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Mon Jul 11 18:13:32 2016

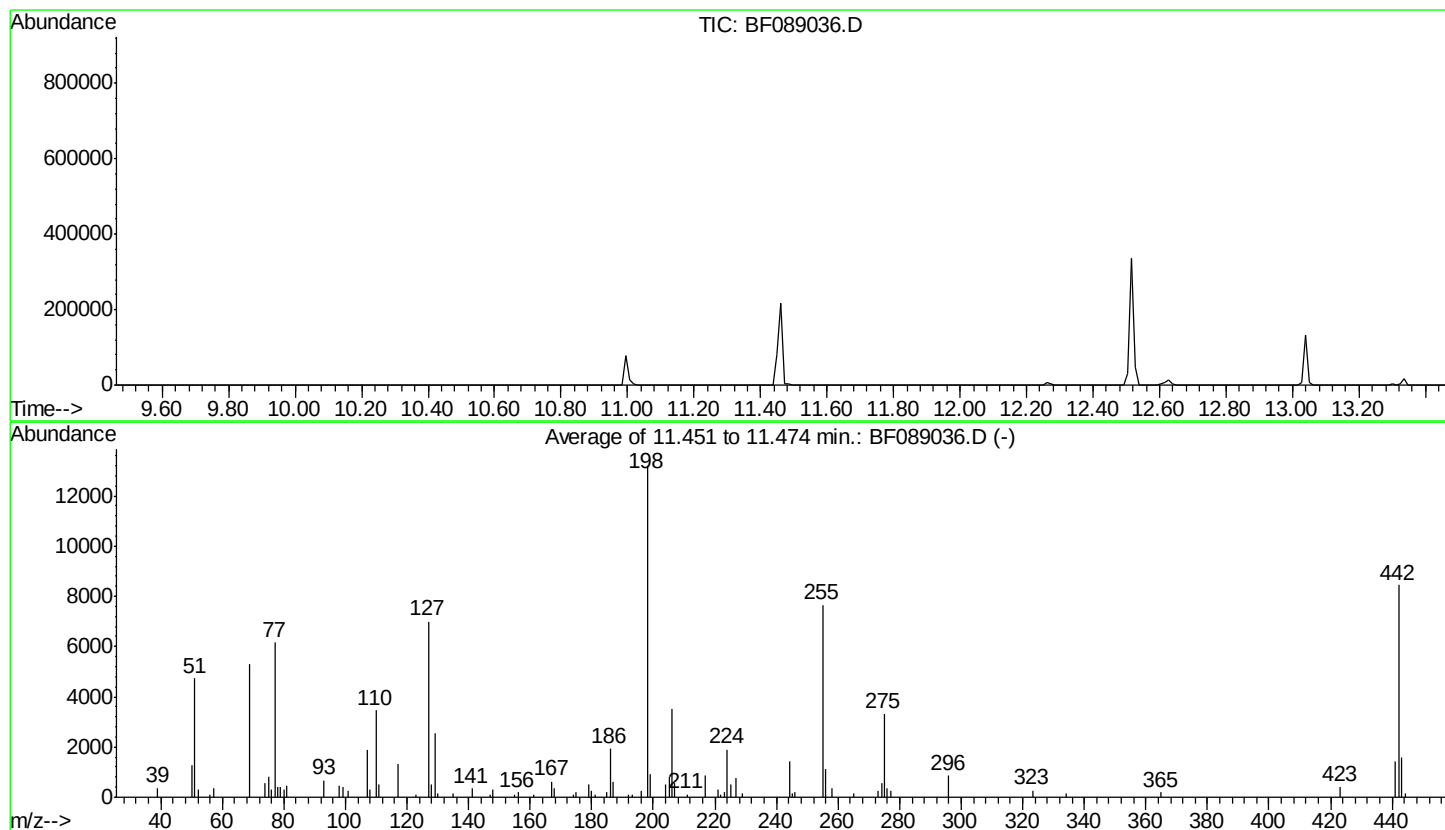

AutoFind: Scans 863, 864, 865; Background Corrected with Scan 860

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 35.8      | 4727    | PASS             |
| 68          | 69           | 0.00         | 2            | 0.0       | 0       | PASS             |
| 69          | 198          | 0.00         | 100          | 40.1      | 5290    | PASS             |
| 70          | 69           | 0.00         | 2            | 0.0       | 0       | PASS             |
| 127         | 198          | 10           | 80           | 52.9      | 6985    | PASS             |
| 197         | 198          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 13205   | PASS             |
| 199         | 198          | 5            | 9            | 7.0       | 924     | PASS             |
| 275         | 198          | 10           | 60           | 25.2      | 3332    | PASS             |
| 365         | 198          | 1            | 100          | 1.4       | 189     | PASS             |
| 441         | 442          | 0.01         | 24           | 16.8      | 1422    | PASS             |
| 442         | 198          | 50           | 100          | 63.9      | 8442    | PASS             |
| 443         | 442          | 15           | 24           | 18.7      | 1582    | PASS             |