

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071521\
 Data File : BF124570.D
 Acq On : 15 Jul 2021 12:27
 Operator : JU/CG
 Sample : PB137634BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB137634BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF124570.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.557	584	590	592	rBB	143135	154383	45.36%	8.585%
2	6.540	752	757	760	rBB	133207	154619	45.43%	8.598%
3	6.922	819	822	825	rBB	52589	44902	13.19%	2.497%
4	7.087	845	850	852	rBB	226447	214670	63.08%	11.937%
5	7.487	912	918	921	rBB	132424	161311	47.40%	8.970%
6	8.204	1036	1040	1043	rBB	62612	61128	17.96%	3.399%
7	9.286	1218	1224	1227	rBB	338563	326670	95.99%	18.165%
8	9.963	1335	1339	1342	rBB	86555	69580	20.45%	3.869%
9	10.751	1469	1473	1476	rBB	135968	117505	34.53%	6.534%
10	11.451	1588	1592	1595	rBB	87534	71406	20.98%	3.971%
11	13.045	1858	1863	1866	rBV	307403	340322	100.00%	18.924%
12	14.092	2037	2041	2044	rBB	65756	49848	14.65%	2.772%
13	15.586	2291	2295	2299	rBB	27268	32009	9.41%	1.780%




Sum of corrected areas: 1798353

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071521\
Data File : BF124570.D
Acq On : 15 Jul 2021 12:27
Operator : JU/CG
Sample : PB137634BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB137634BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

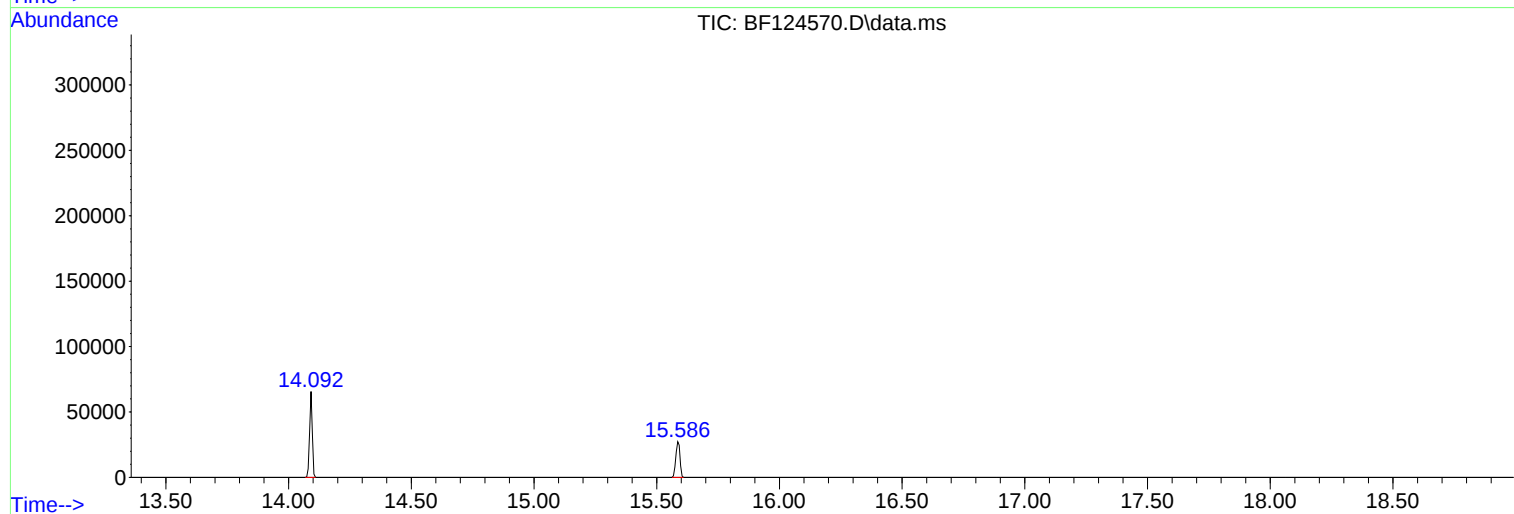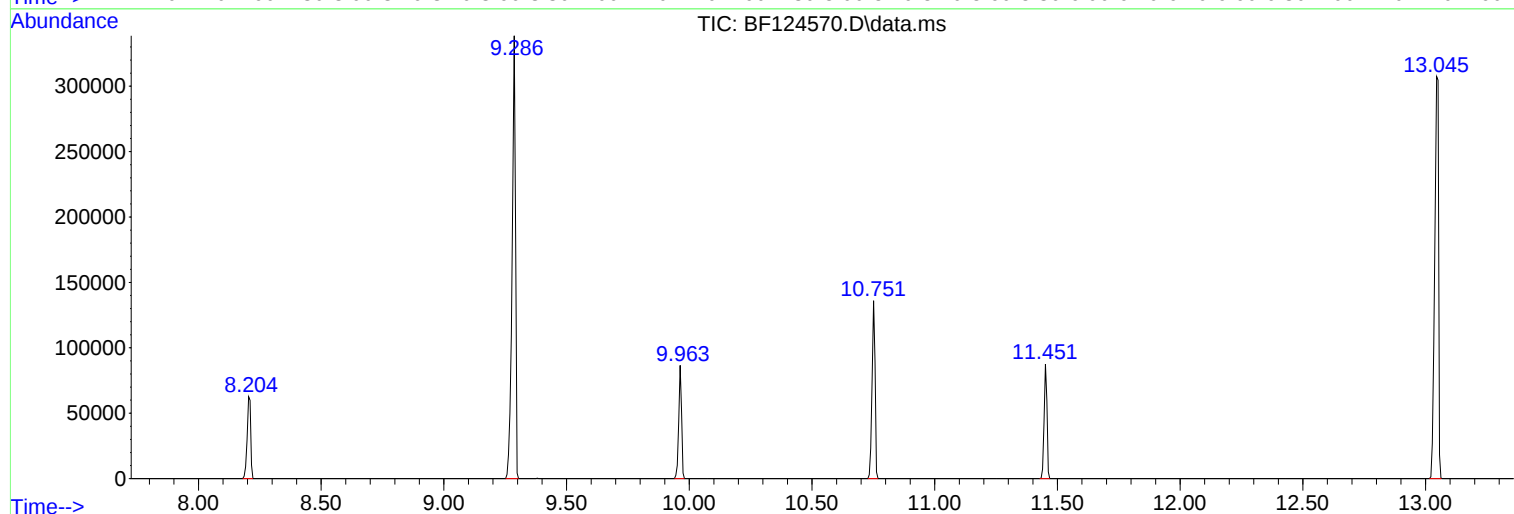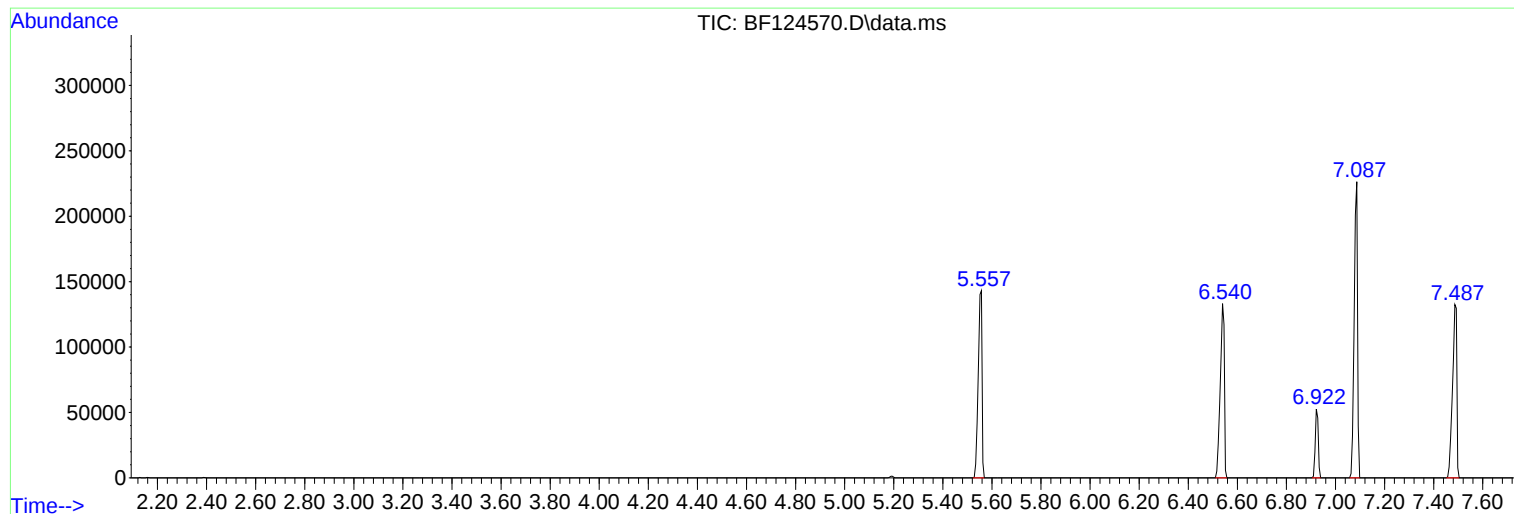

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071521\
Data File : BF124570.D
Acq On : 15 Jul 2021 12:27
Operator : JU/CG
Sample : PB137634BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB137634BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071521\
Data File : BF124570.D
Acq On : 15 Jul 2021 12:27
Operator : JU/CG
Sample : PB137634BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB137634BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------