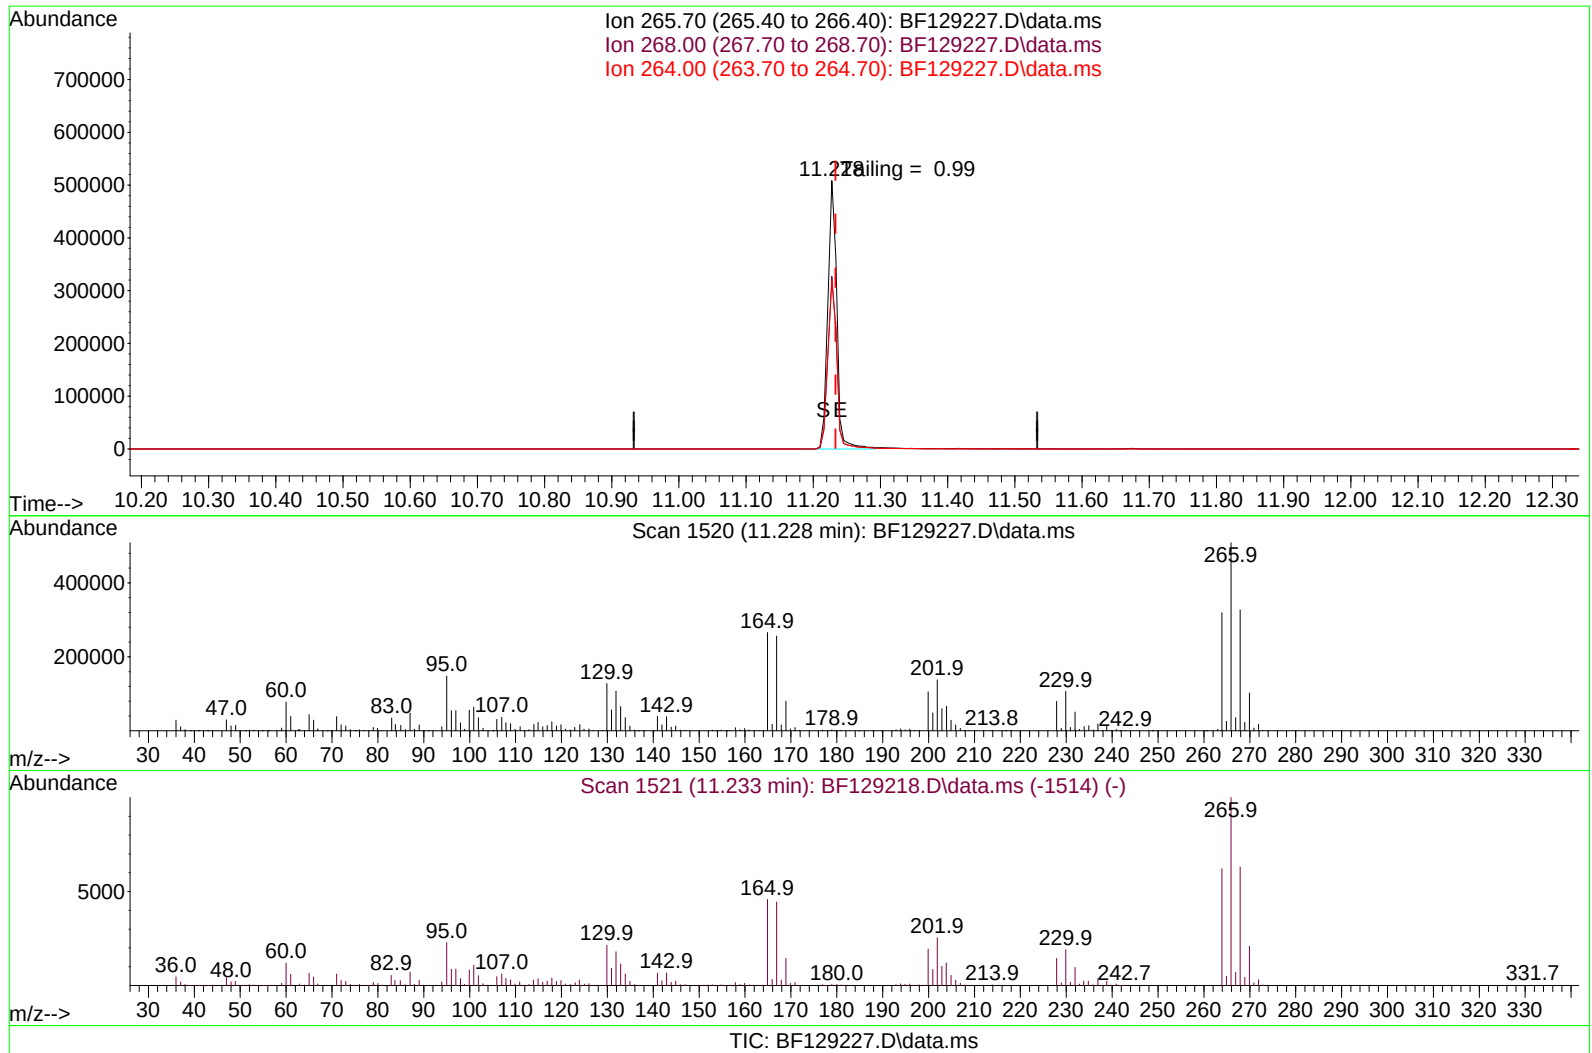


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071522\
Data File : BF129227.D
Acq On : 15 Jul 2022 08:19
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1




Quant Time: Jul 15 10:47:56 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 15 10:43:26 2022
Response via : Initial Calibration

**(70) Pentachlorophenol (C)****11.228min (-0.006) 159828.43 ng****response 475056**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	64.30
264.00	61.80	62.81
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071522\
Data File : BF129227.D
Acq On : 15 Jul 2022 08:19
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 15 10:47:56 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 15 10:43:26 2022
Response via : Initial Calibration

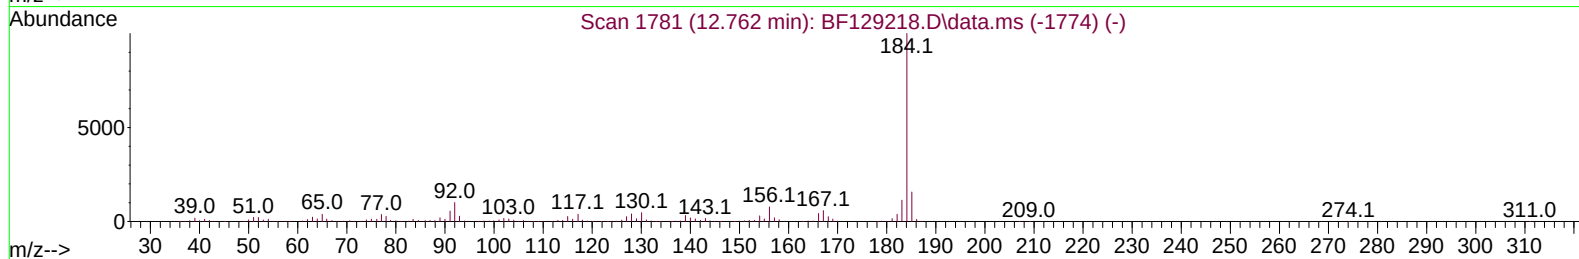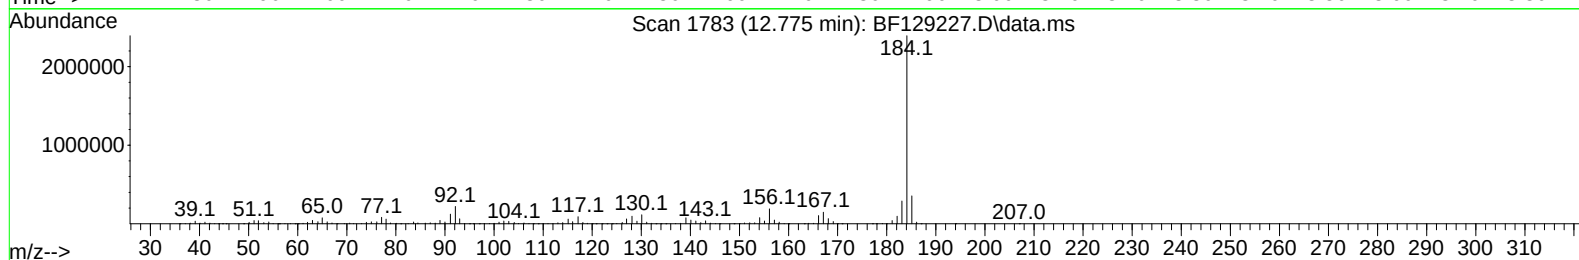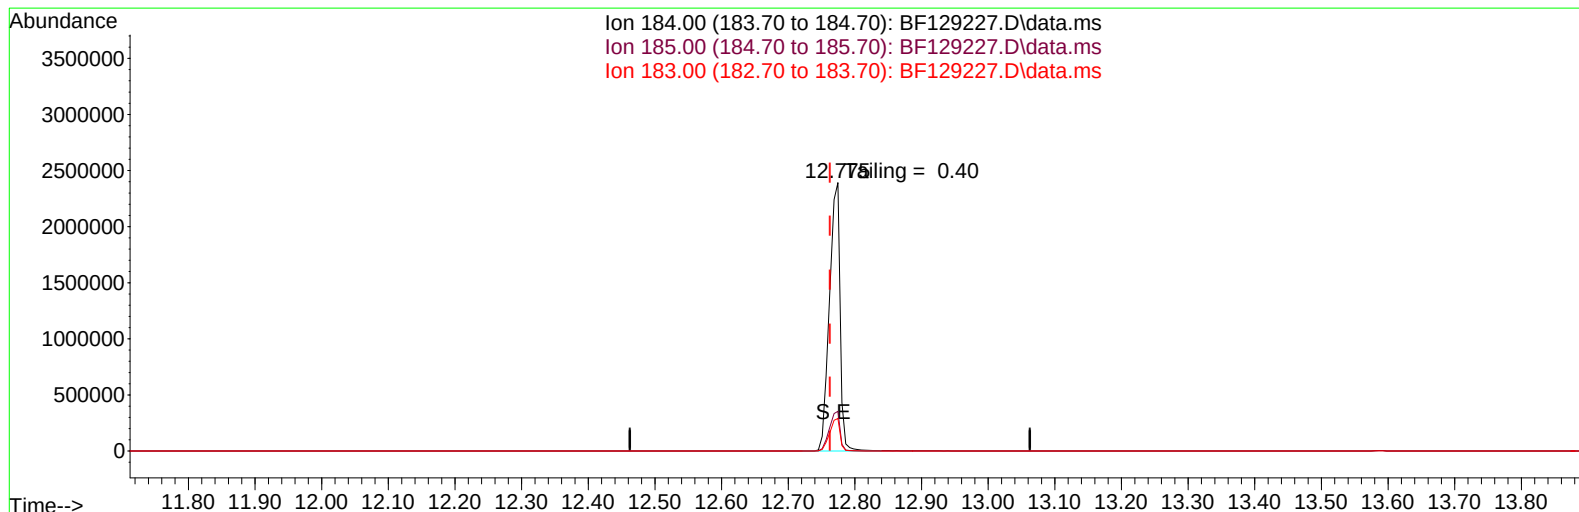

TIC: BF129227.D\data.ms

(77) Benzidine**12.775min (+ 0.012) 260974.32 ng****response 2657261**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.81
183.00	11.60	12.10
0.00	0.00	0.00