
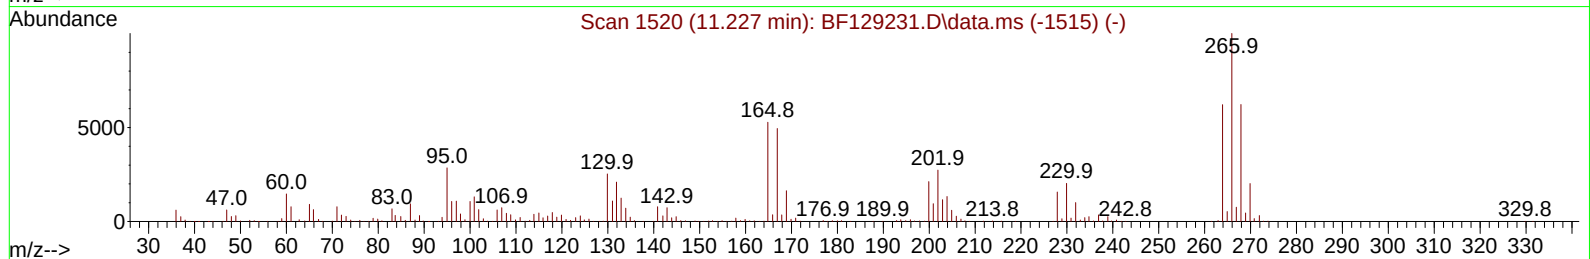
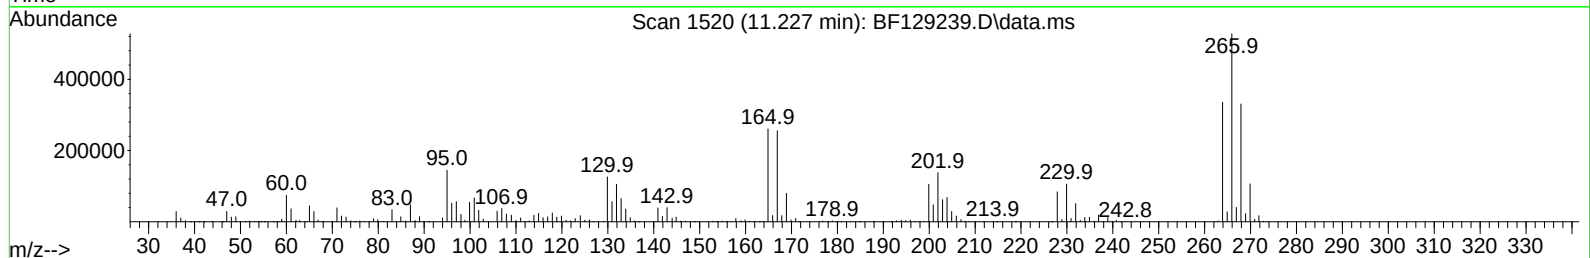


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071522\
Data File : BF129239.D
Acq On : 15 Jul 2022 15:33
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 16 03:15:08 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 15 12:55:49 2022
Response via : Initial Calibration

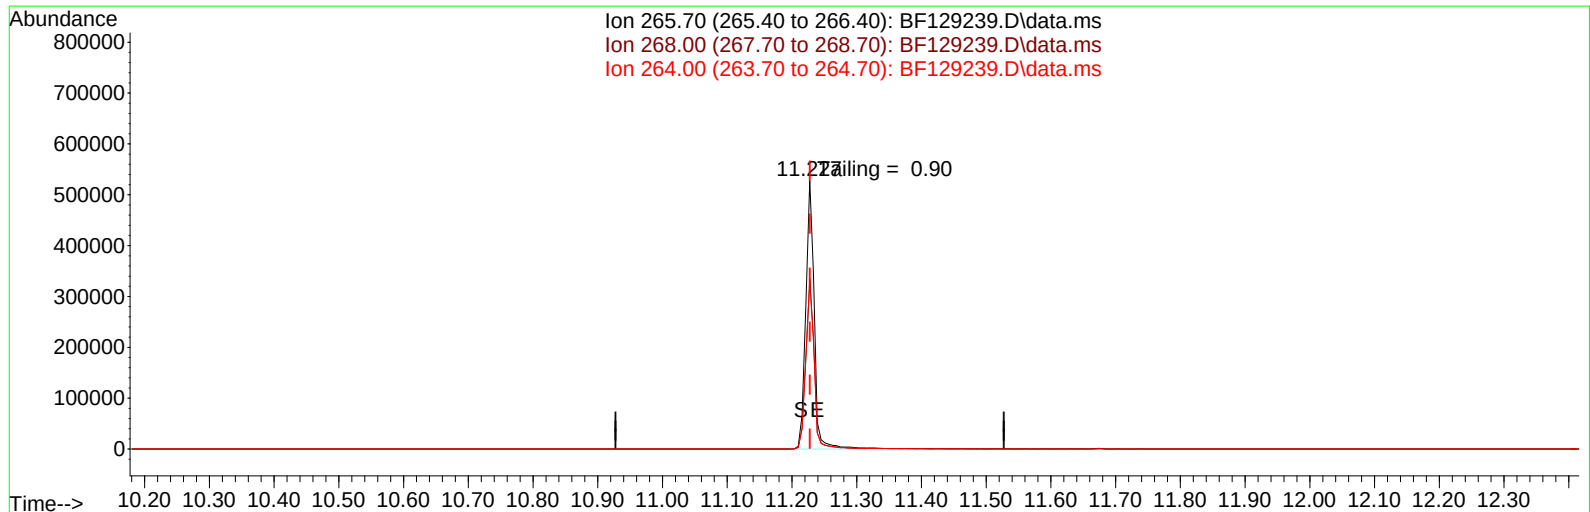

TIC: BF129239.D\data.ms




(70) Pentachlorophenol (C)

11.227min (-0.000) 109837.57 ng

response 487872

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	62.64
264.00	61.80	63.49
0.00	0.00	0.00

Quant Time: Jul 16 03:15:08 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 15 12:55:49 2022
Response via : Initial Calibration

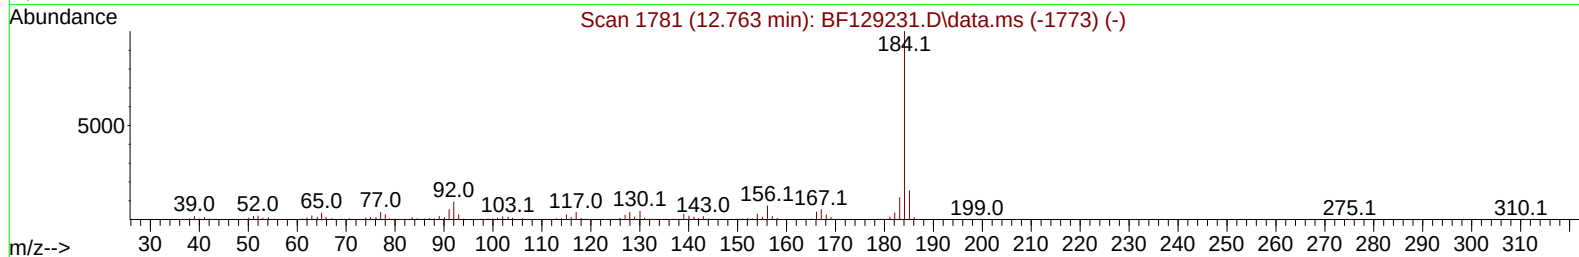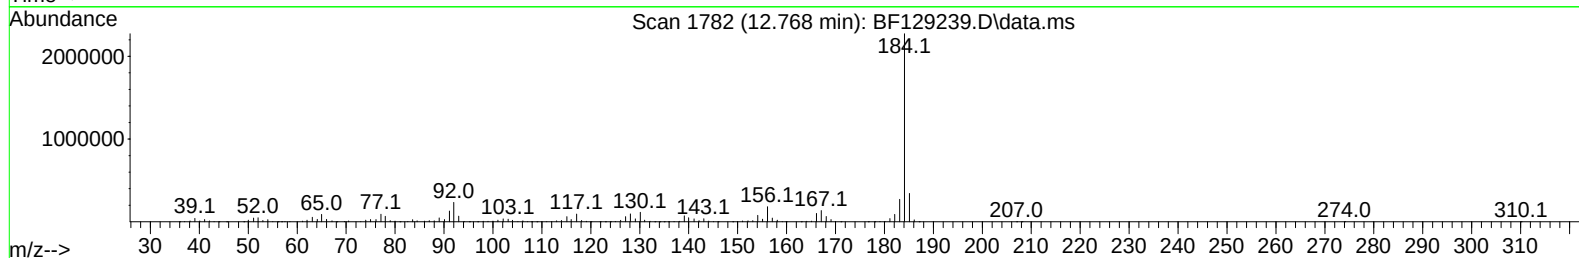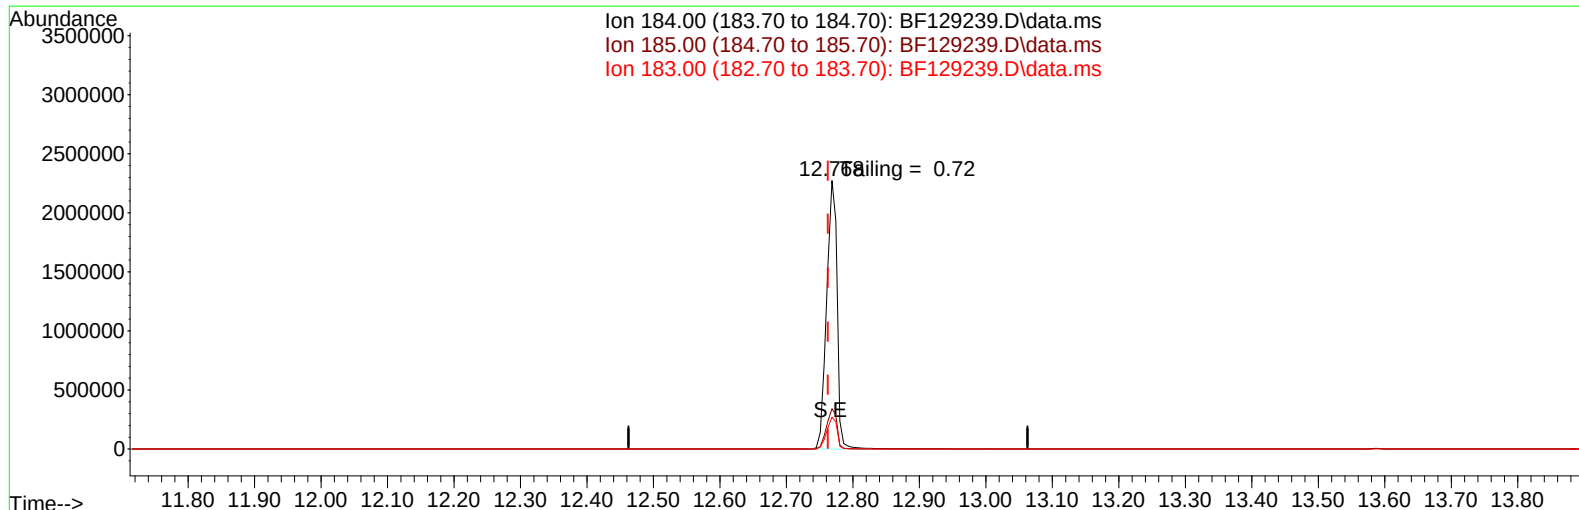

TIC: BF129239.D\data.ms

(77) Benzidine

12.768min (+ 0.006) 174762.39 ng

response **2485091**

Ion	Exp%	Act%
-----	------	------

184.00	100.00	100.00
--------	--------	--------

185.00	14.90	15.04
--------	-------	-------

183.00	11.60	11.91
--------	-------	-------

0.00 0.00 0.00