

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071522\
 Data File : BF129241.D
 Acq On : 15 Jul 2022 16:37
 Operator : CG\JU
 Sample : PB146243BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB146243BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF129241.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.040	289	298	303	rVB	128107	162601	1.65%	0.261%
2	5.528	545	551	554	rBV	7058931	7230915	73.40%	11.610%
3	6.522	714	720	723	rBV	6613349	7595885	77.10%	12.196%
4	6.892	779	783	787	rBV	2151000	1971286	20.01%	3.165%
5	7.457	873	879	882	rBV	4548630	5165882	52.44%	8.294%
6	8.181	996	1002	1005	rBV	2729137	2782566	28.24%	4.468%
7	9.257	1178	1185	1188	rBV	8756232	9432859	95.75%	15.145%
8	9.933	1294	1300	1304	rBV	3293996	3143467	31.91%	5.047%
9	10.727	1428	1435	1438	rBV	5922655	5986131	60.76%	9.611%
10	11.427	1547	1554	1557	rBV	3383241	3139347	31.87%	5.040%
11	13.016	1818	1824	1827	rBV	9307112	9851847	100.00%	15.818%
12	14.068	1998	2003	2006	rBV	2796203	2567954	26.07%	4.123%
13	14.157	2012	2018	2024	rBV	136486	149548	1.52%	0.240%
14	15.174	2187	2191	2198	rVB	108471	126887	1.29%	0.204%
15	15.557	2250	2256	2270	rBV	1760642	2289233	23.24%	3.676%
16	16.015	2328	2334	2343	rBV	139357	214613	2.18%	0.345%
17	16.533	2415	2422	2430	rBV	115060	213722	2.17%	0.343%
18	17.139	2519	2525	2535	rVB3	62881	139791	1.42%	0.224%
19	17.862	2642	2648	2660	rVB2	48279	118131	1.20%	0.190%




Sum of corrected areas: 62282665

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071522\
Data File : BF129241.D
Acq On : 15 Jul 2022 16:37
Operator : CG\JU
Sample : PB146243BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB146243BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

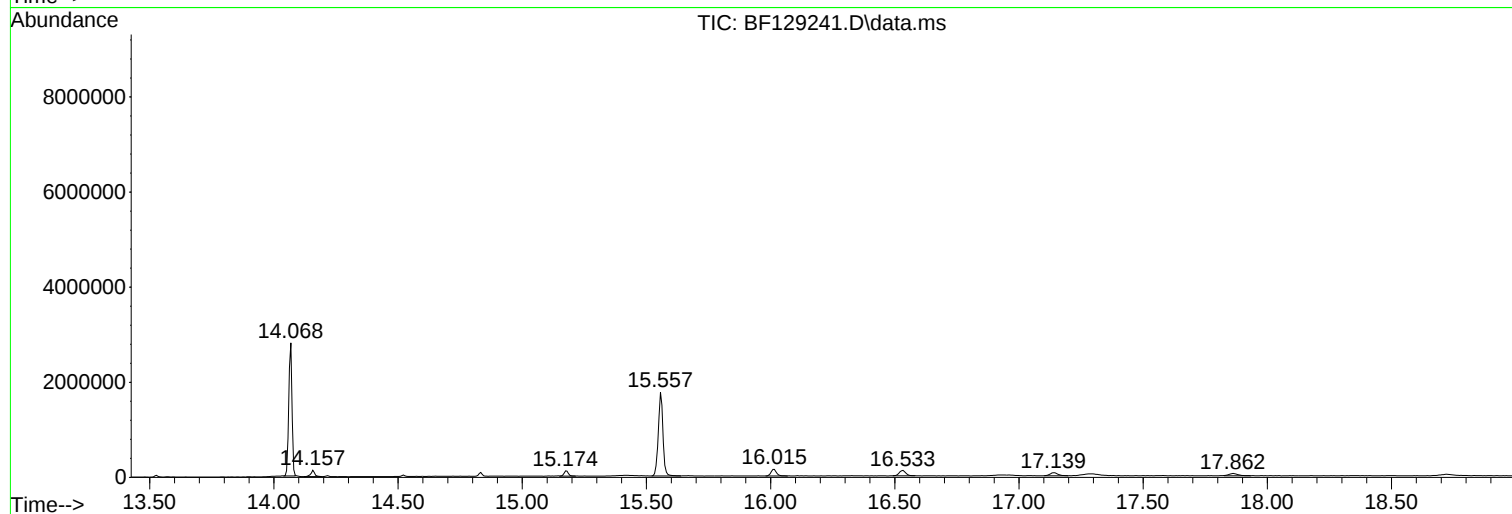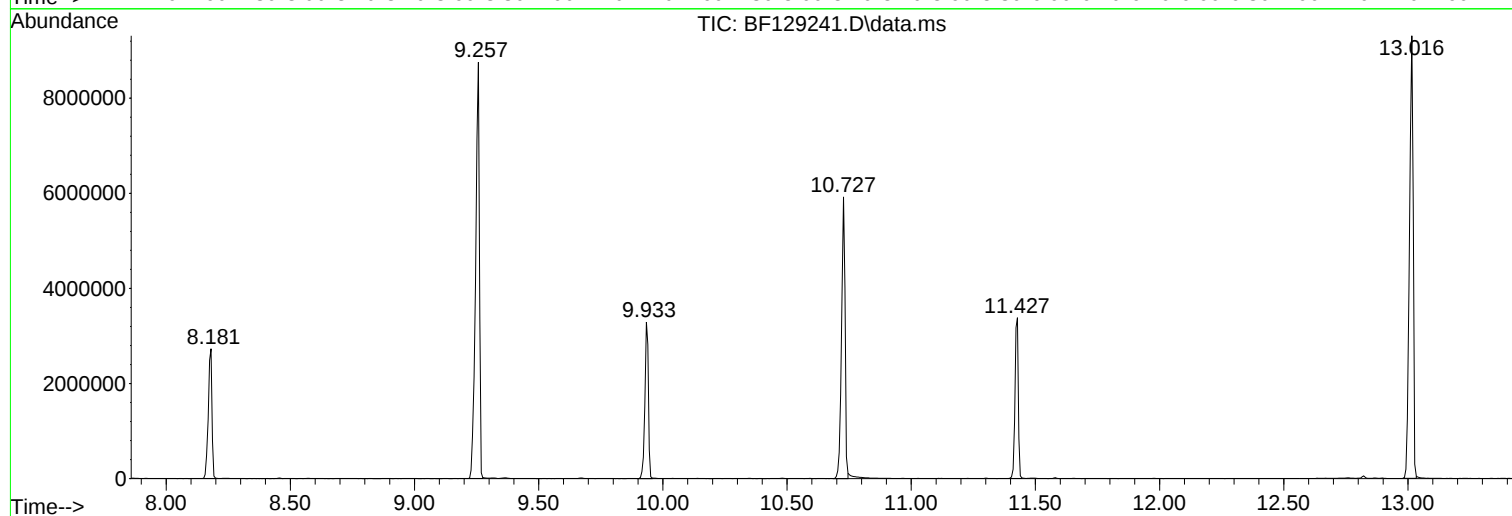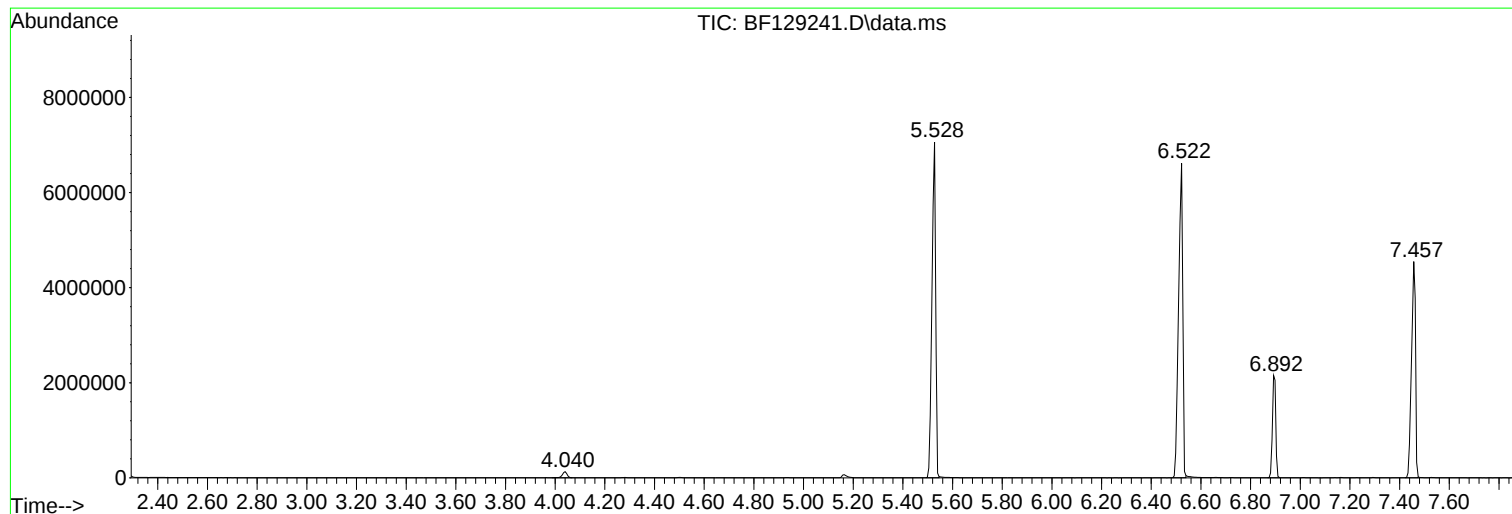

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071522\
Data File : BF129241.D
Acq On : 15 Jul 2022 16:37
Operator : CG\JU
Sample : PB146243BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB146243BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071522\
Data File : BF129241.D
Acq On : 15 Jul 2022 16:37
Operator : CG\JU
Sample : PB146243BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB146243BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------