
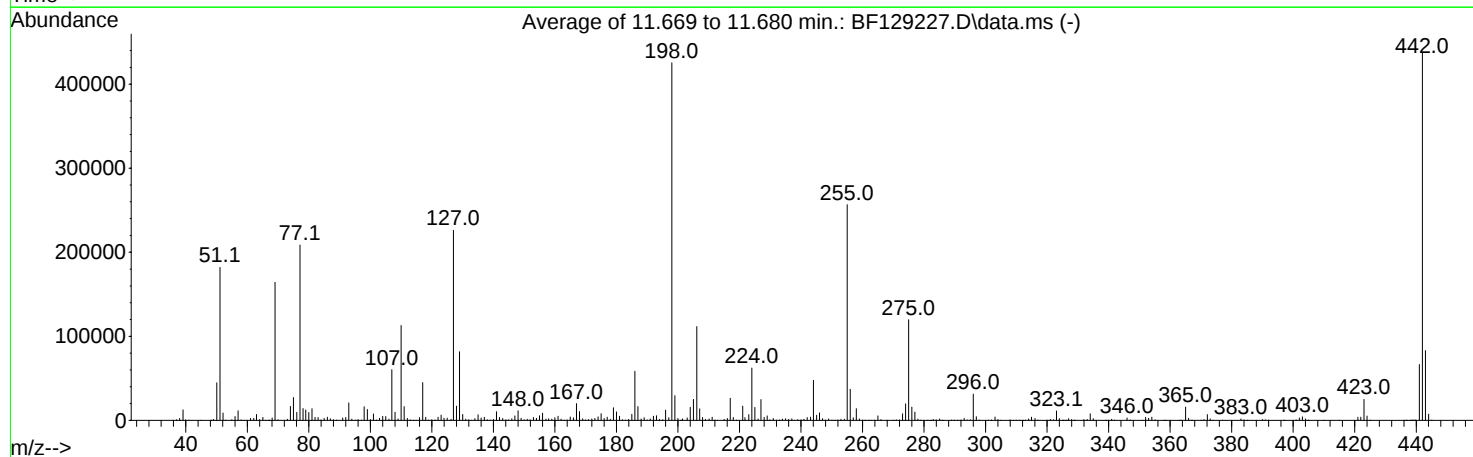


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071522\
 Data File : BF129227.D
 Acq On : 15 Jul 2022 08:19
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jul 15 12:55:49 2022

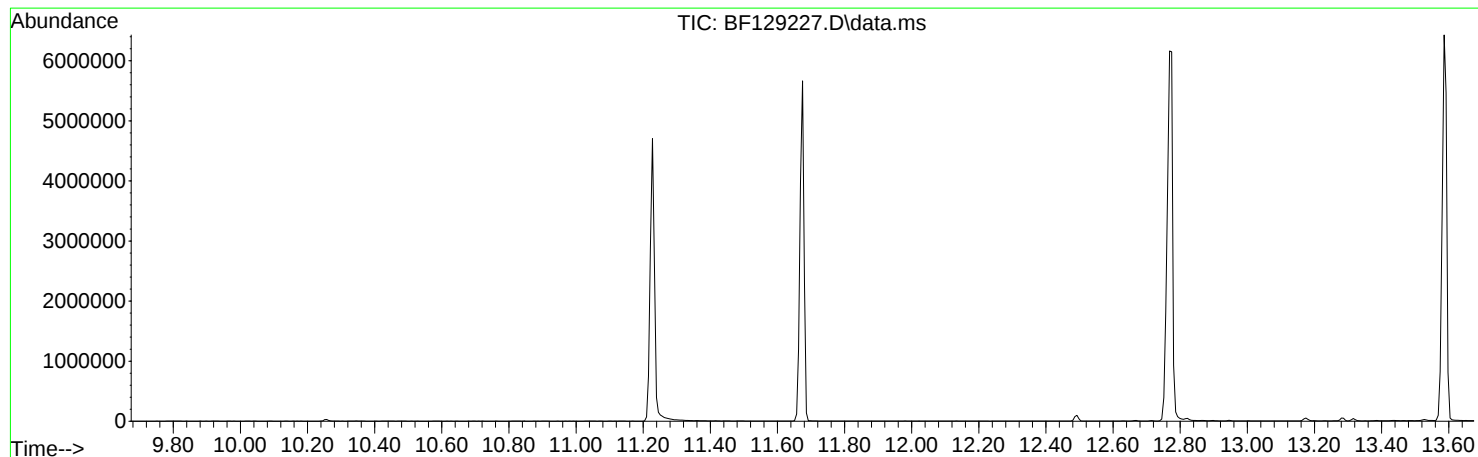




AutoFind: Scans 1595, 1596, 1597; Background Corrected with Scan 1589

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.8	182035	PASS
68	69	0.00	2	1.8	2890	PASS
69	198	0.00	100	38.6	164379	PASS
70	69	0.00	2	0.5	856	PASS
127	198	10	80	53.1	226112	PASS
197	198	0.00	2	0.8	3209	PASS
198	198	100	100	100.0	425515	PASS
199	198	5	9	6.9	29331	PASS
275	198	10	60	28.1	119699	PASS
365	198	1	100	3.7	15867	PASS
441	198	0.01	100	15.6	66368	PASS
442	442	50	100	100.0	437696	PASS
443	442	15	24	18.9	82933	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071522\
 Data File : BF129227.D
 Acq On : 15 Jul 2022 08:19
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jul 15 10:47:56 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 15 10:43:26 2022
 Response via : Initial Calibration

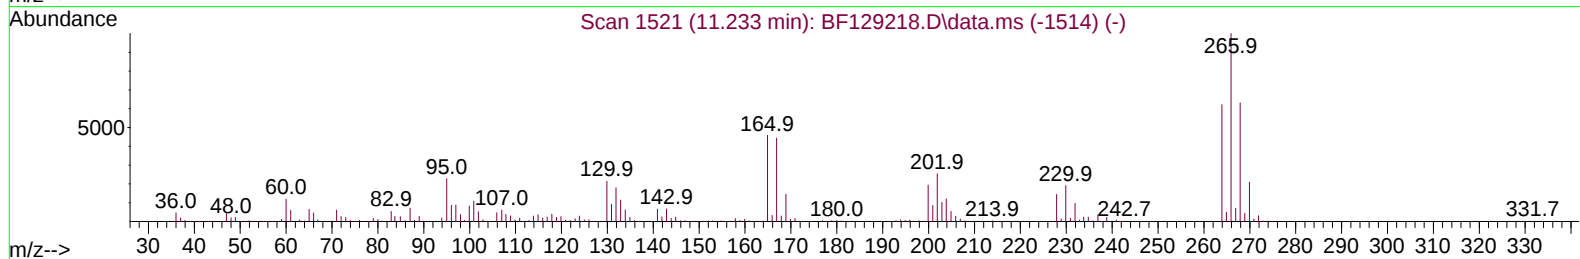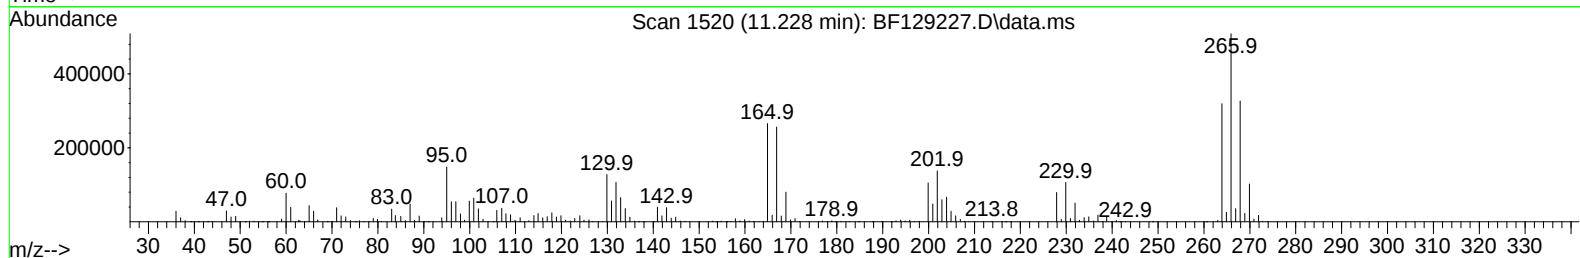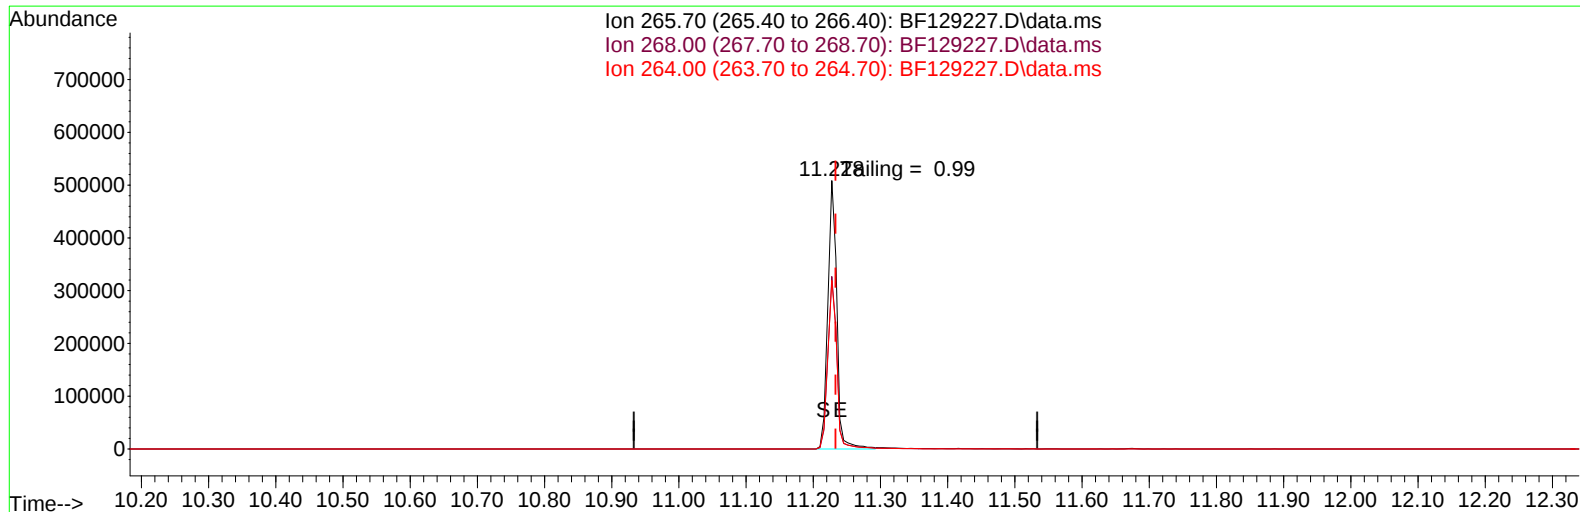

TIC: BF129227.D\data.ms

(70) Pentachlorophenol (C)

11.228min (-0.006) 159828.43 ng




response 475056

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	64.30
264.00	61.80	62.81
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071522\
 Data File : BF129227.D
 Acq On : 15 Jul 2022 08:19
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jul 15 10:47:56 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 15 10:43:26 2022
 Response via : Initial Calibration

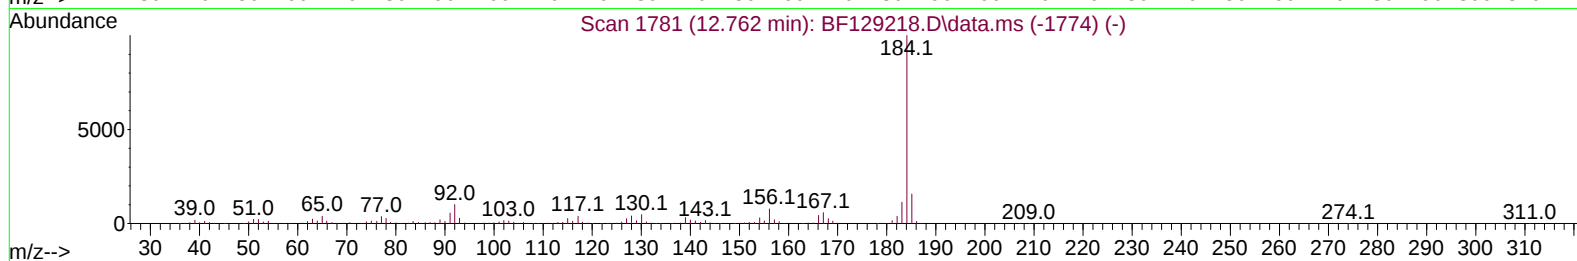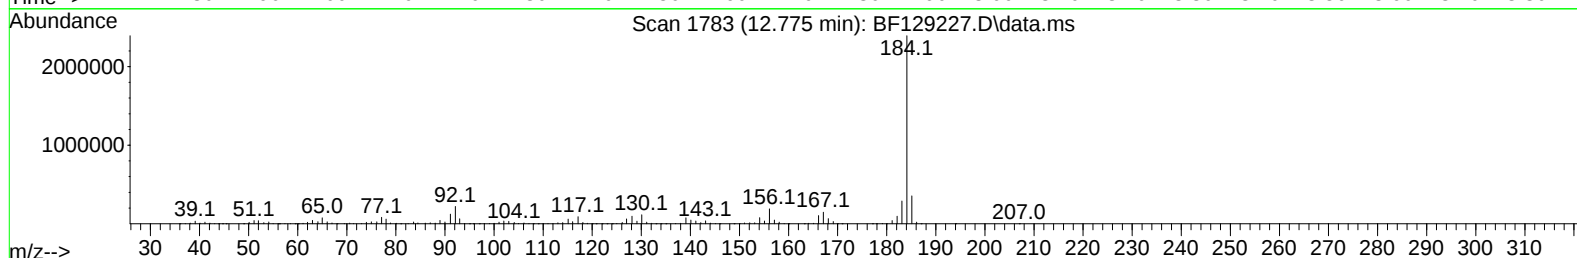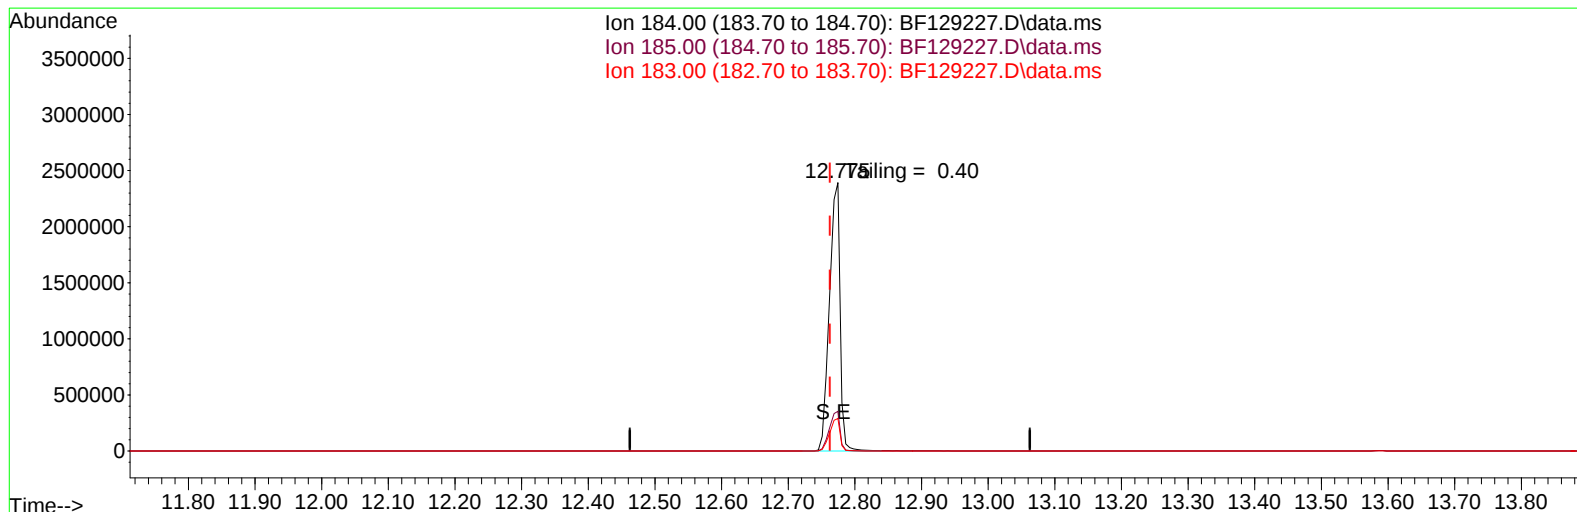

TIC: BF129227.D\data.ms

(77) Benzidine

12.775min (+ 0.012) 260974.32 ng

response 2657261

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.81
183.00	11.60	12.10
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/15/2022	BNA_F	<u>BF129227.D</u>
Compound Name	Response	Retention Time
DDT	1089772	13.56
DDD	8050	13.28
DDE	1129	12.94
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9179	1098951	0.84

Instrument :
BNA_F
ClientSampleId :
DFTPP