
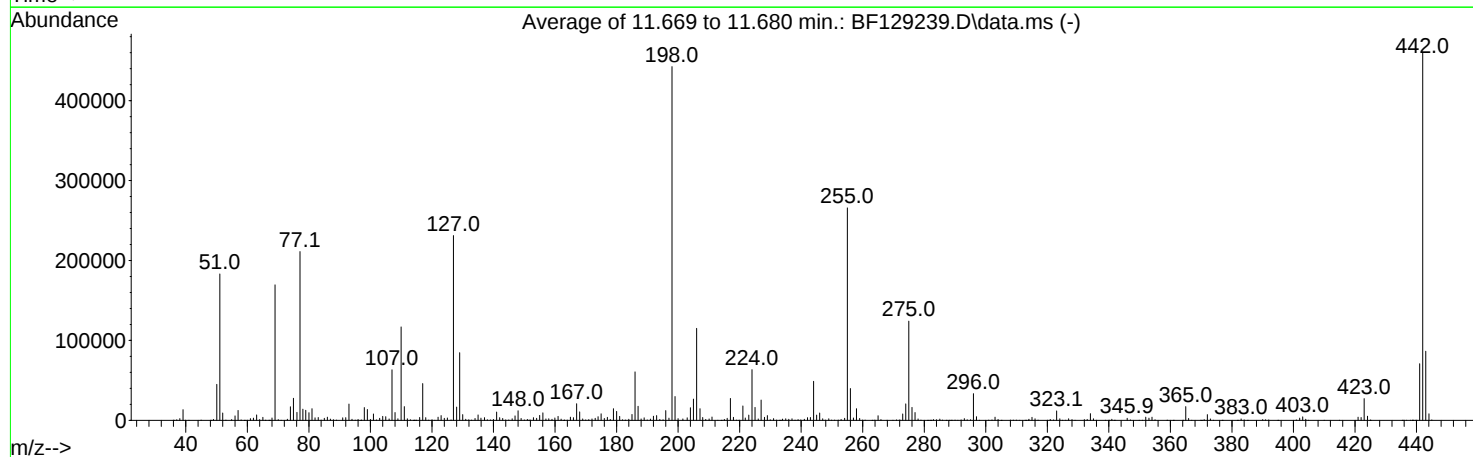


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071522\
 Data File : BF129239.D
 Acq On : 15 Jul 2022 15:33
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jul 15 12:55:49 2022

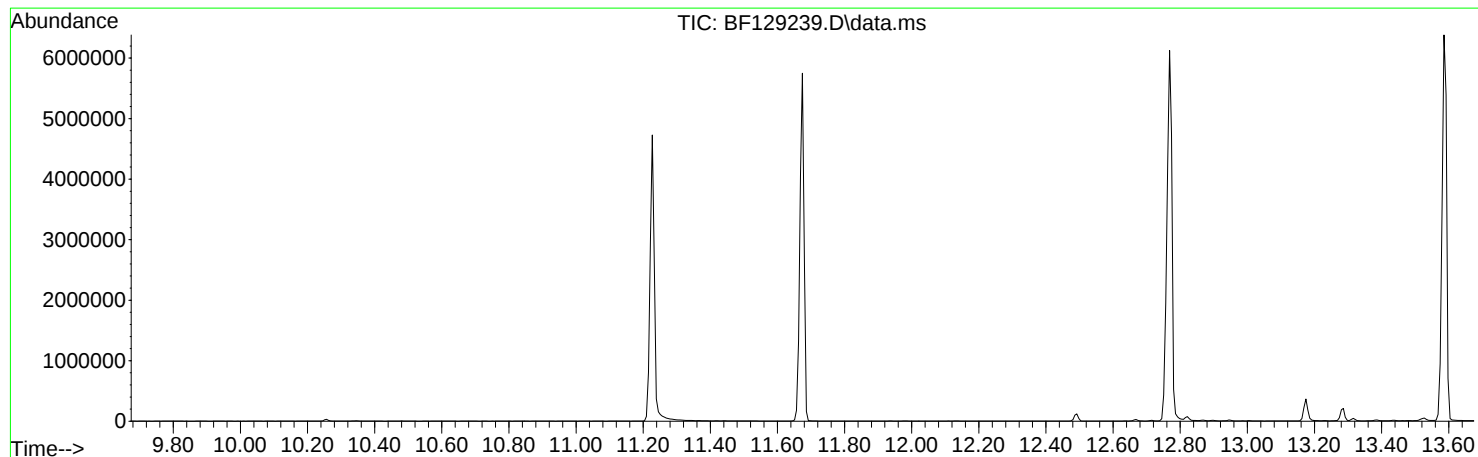




AutoFind: Scans 1595, 1596, 1597; Background Corrected with Scan 1589

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.4	183163	PASS
68	69	0.00	2	1.8	3098	PASS
69	198	0.00	100	38.3	169483	PASS
70	69	0.00	2	0.6	954	PASS
127	198	10	80	52.3	231296	PASS
197	198	0.00	2	0.7	2887	PASS
198	198	100	100	100.0	442645	PASS
199	198	5	9	6.7	29808	PASS
275	198	10	60	28.0	124128	PASS
365	198	1	100	3.9	17224	PASS
441	198	0.01	100	16.0	70832	PASS
442	442	50	100	100.0	460245	PASS
443	442	15	24	18.8	86547	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071522\
Data File : BF129239.D
Acq On : 15 Jul 2022 15:33
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 16 03:15:08 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 15 12:55:49 2022
Response via : Initial Calibration

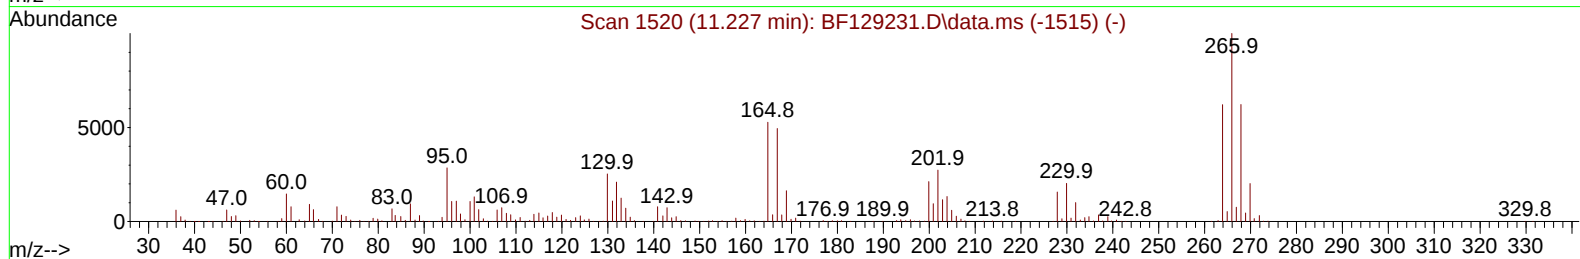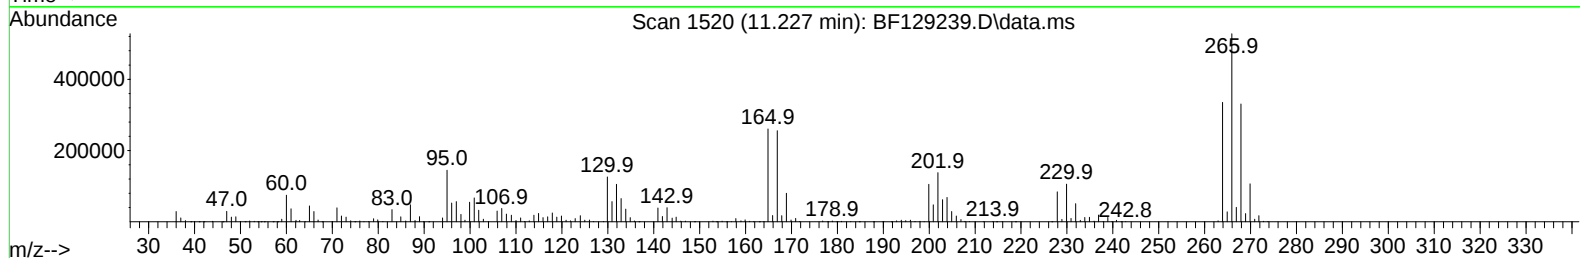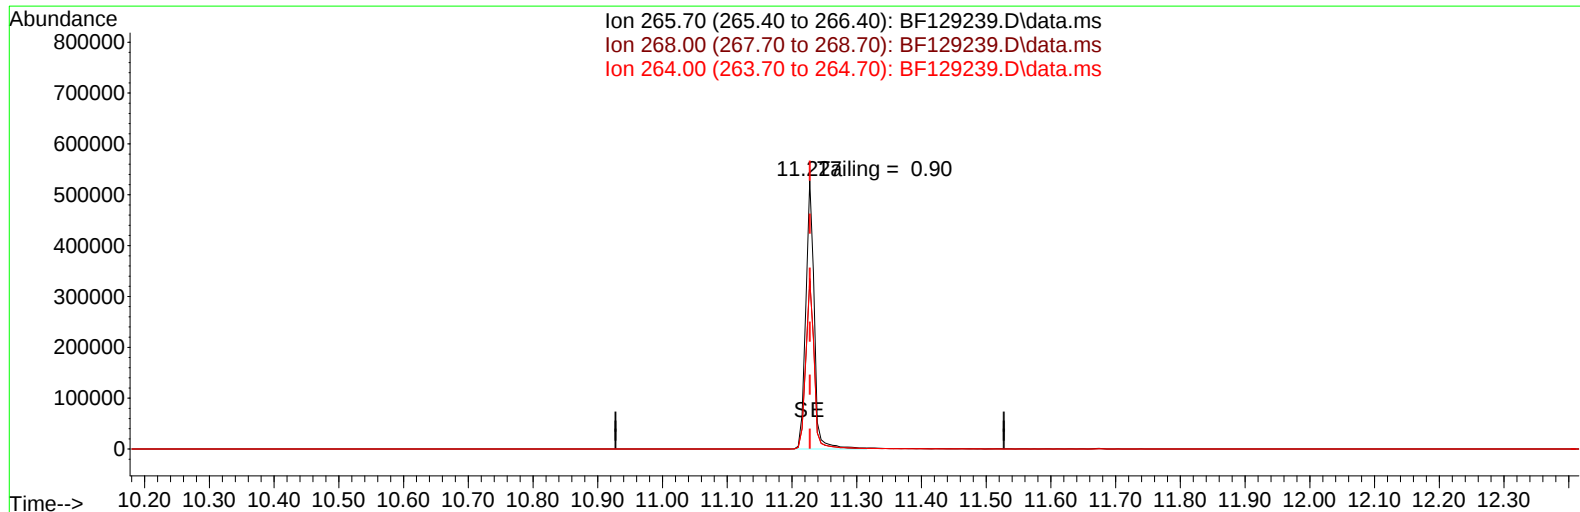

TIC: BF129239.D\data.ms

(70) Pentachlorophenol (C)

11.227min (-0.000) 109837.57 ng




response 487872

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	62.64
264.00	61.80	63.49
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071522\
Data File : BF129239.D
Acq On : 15 Jul 2022 15:33
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 16 03:15:08 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 15 12:55:49 2022
Response via : Initial Calibration

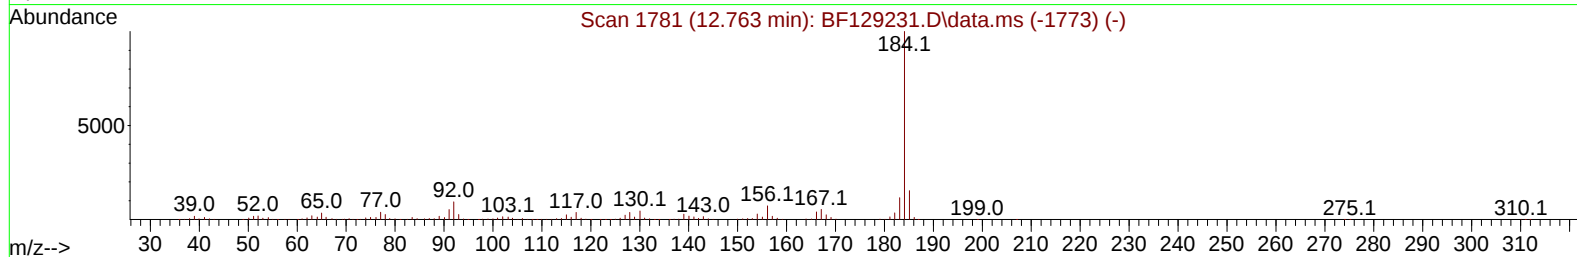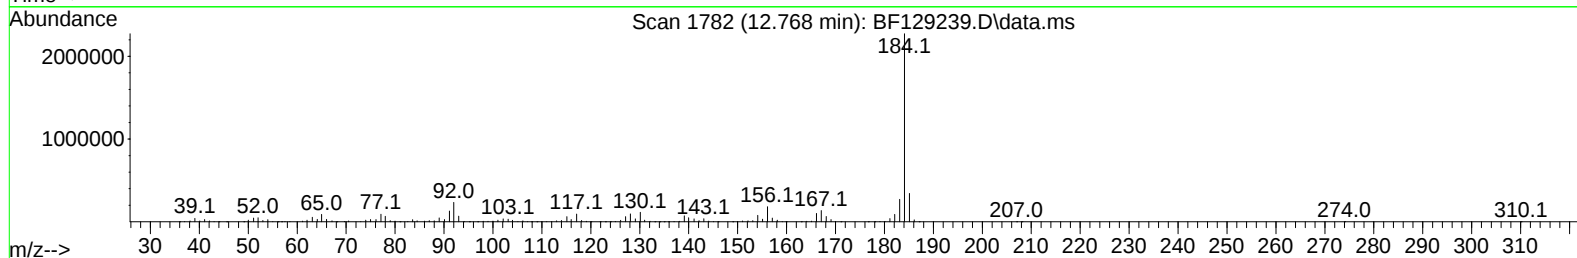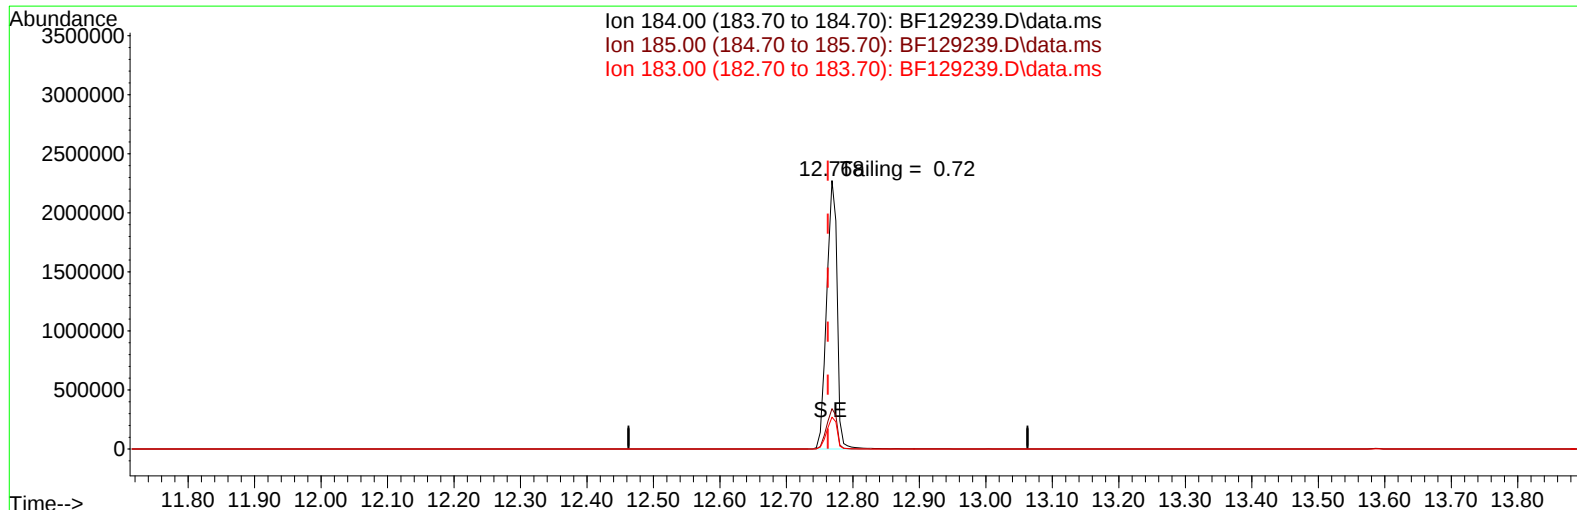

TIC: BF129239.D\data.ms

(77) Benzidine

12.768min (+ 0.006) 174762.39 ng

response 2485091

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	15.04
183.00	11.60	11.91
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/15/2022	BNA_F	<u>BF129239.D</u>
Compound Name	Response	Retention Time
DDT	1103117	13.586
DDD	40501	13.286
DDE	1488	12.945
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
41989	1145106	3.67

Instrument :
BNA_F
ClientSampleId :
DFTPP