


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF071615\
 Data File : BF080512.D
 Acq On : 16 Jul 2015 15:56
 Operator : TP/UM
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF071615.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 16 17:11:01 2015

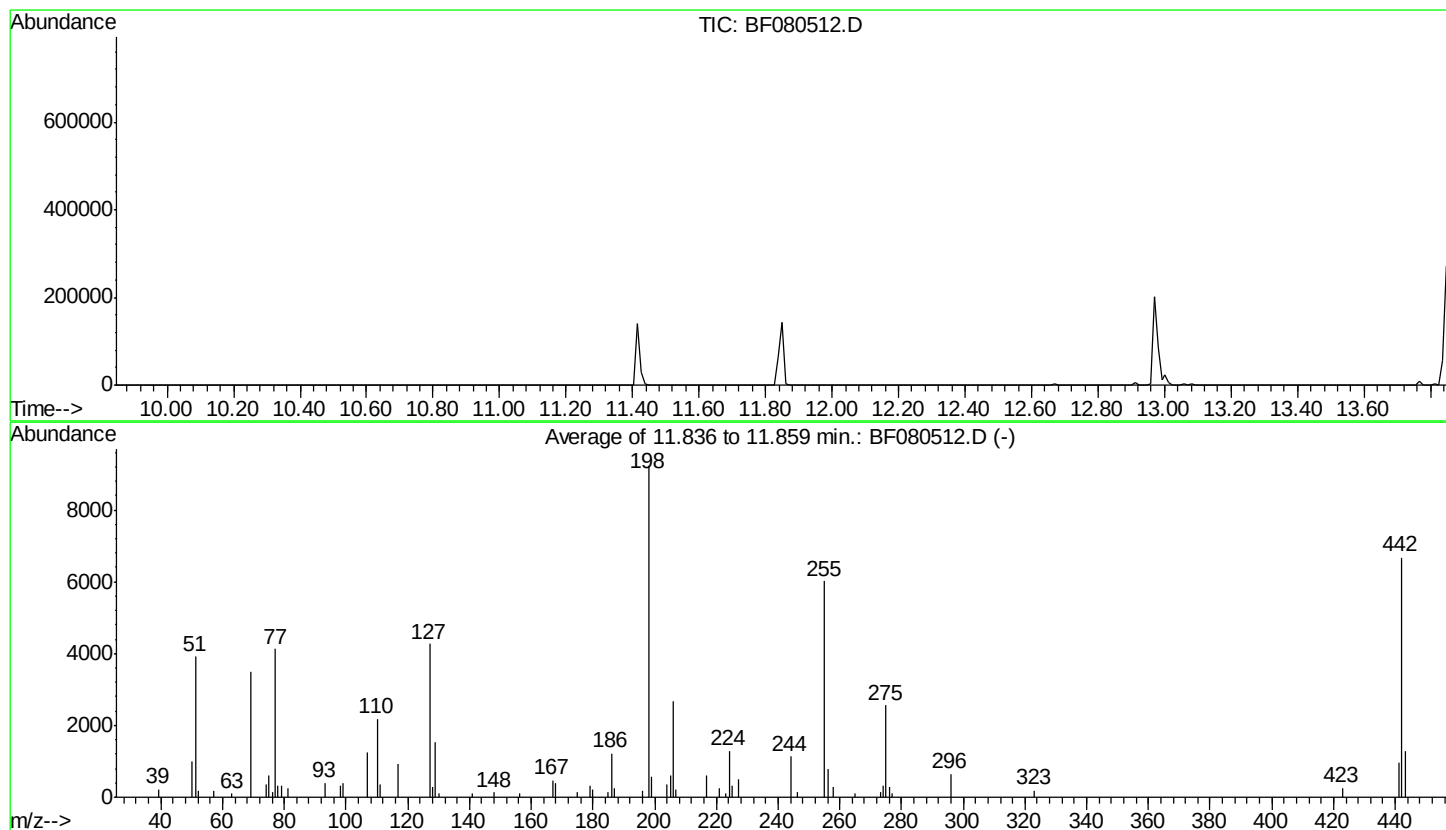

AutoFind: Scans 853, 854, 855; Background Corrected with Scan 850

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.4	3917	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	37.8	3492	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.2	4269	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	9234	PASS
199	198	5	9	6.3	578	PASS
275	198	10	60	27.7	2554	PASS
365	198	1	100	0.0	0	FAIL *
441	442	0.01	24	14.3	957	PASS
442	198	50	100	72.2	6670	PASS
443	442	15	24	19.4	1291	PASS