


Data Path : Z:\HPCHEM1\BNA\_F\DATA\BF071615\  
 Data File : BF080514.D  
 Acq On : 16 Jul 2015 17:12  
 Operator : TP/UM  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF071615.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Thu Jul 16 17:11:01 2015

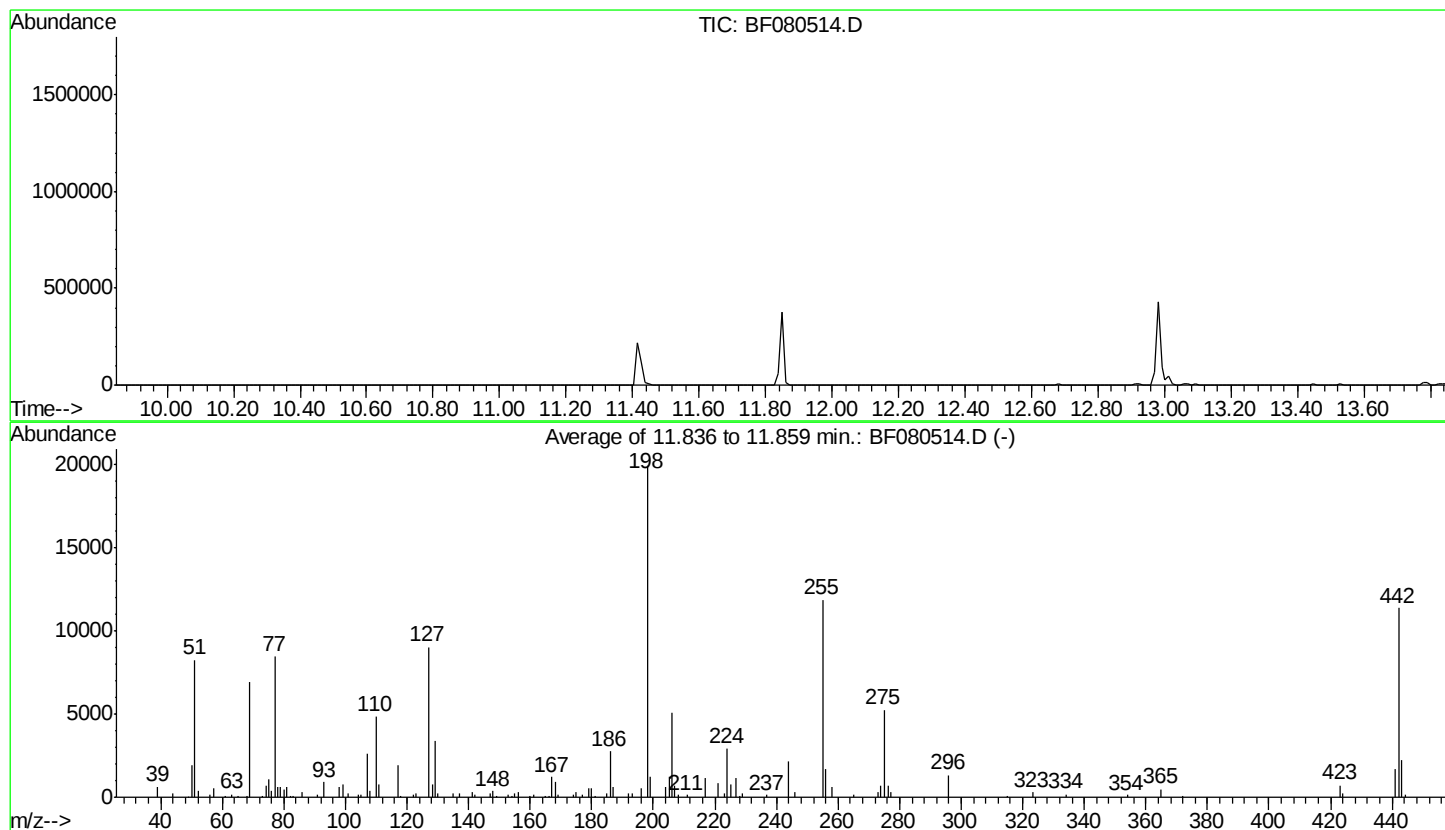

AutoFind: Scans 853, 854, 855; Background Corrected with Scan 850

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 41.5         | 8277       | PASS                |
| 68             | 69              | 0.00            | 2               | 1.5          | 107        | PASS                |
| 69             | 198             | 0.00            | 100             | 34.9         | 6952       | PASS                |
| 70             | 69              | 0.00            | 2               | 0.0          | 0          | PASS                |
| 127            | 198             | 10              | 80              | 45.4         | 9046       | PASS                |
| 197            | 198             | 0.00            | 2               | 0.0          | 0          | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 19944      | PASS                |
| 199            | 198             | 5               | 9               | 6.1          | 1214       | PASS                |
| 275            | 198             | 10              | 60              | 26.4         | 5259       | PASS                |
| 365            | 198             | 1               | 100             | 2.4          | 470        | PASS                |
| 441            | 442             | 0.01            | 24              | 15.2         | 1728       | PASS                |
| 442            | 198             | 50              | 100             | 57.0         | 11371      | PASS                |
| 443            | 442             | 15              | 24              | 20.0         | 2272       | PASS                |