

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF071616\
Data File : BF089052.D
Acq On : 16 Jul 2016 13:37
Operator : UM/SJ
Sample : H3951-15 10X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
LSS-SB-SB05(2-4ft)

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.770	14	16	51	rVB	1261238	2230075	100.00%	46.010%
2	5.256	319	321	323	rBV	38917	50943	2.28%	1.051%
3	6.307	411	413	416	rBV	67675	64364	2.89%	1.328%
4	6.433	422	424	426	rBV	57164	56703	2.54%	1.170%
5	6.662	442	444	446	rBB	443078	364709	16.35%	7.525%
6	6.810	456	457	459	rBB	45331	47538	2.13%	0.981%
7	7.222	491	493	495	rBB	38119	29080	1.30%	0.600%
8	7.942	554	556	559	rBV	331113	429300	19.25%	8.857%
9	9.028	649	651	653	rBB	80969	71721	3.22%	1.480%
10	9.702	707	710	712	rBV	474355	458511	20.56%	9.460%
11	11.176	836	839	841	rBV	481474	395114	17.72%	8.152%
12	12.754	976	977	979	rVB2	48366	47281	2.12%	0.975%
13	13.805	1066	1069	1071	rBV	280370	336875	15.11%	6.950%
14	15.165	1186	1188	1191	rBV	202372	264678	11.87%	5.461%




Sum of corrected areas: 4846892

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF071616\
Data File : BF089052.D
Acq On : 16 Jul 2016 13:37
Operator : UM/SJ
Sample : H3951-15 10X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
LSS-SB-SB05(2-4ft)

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

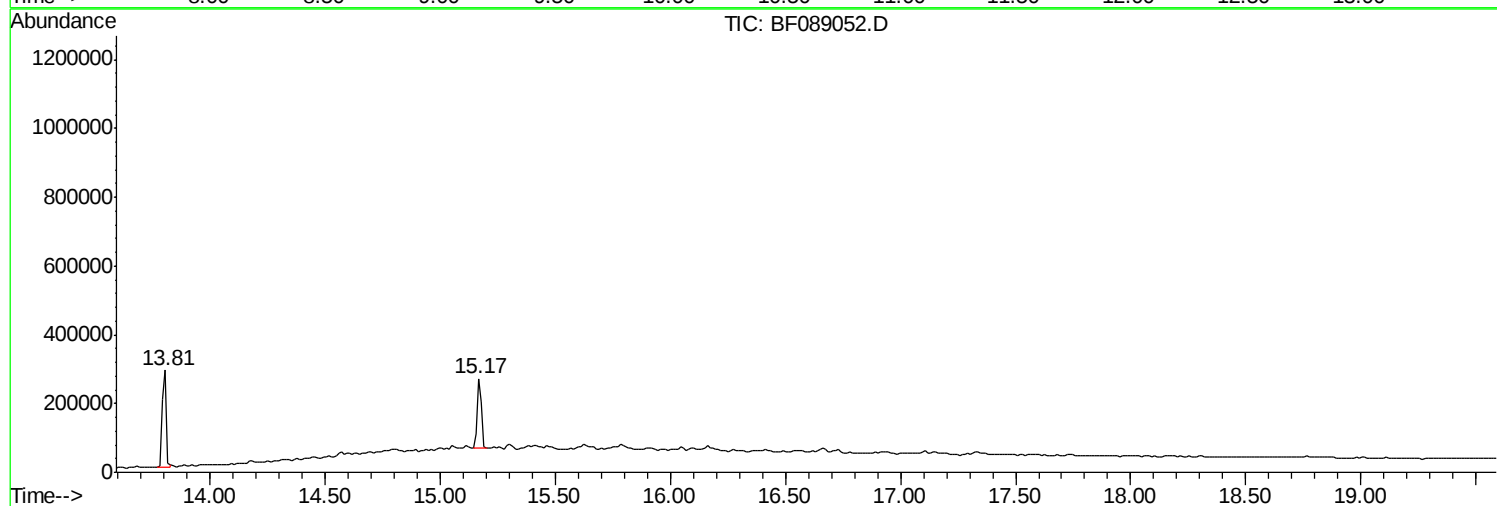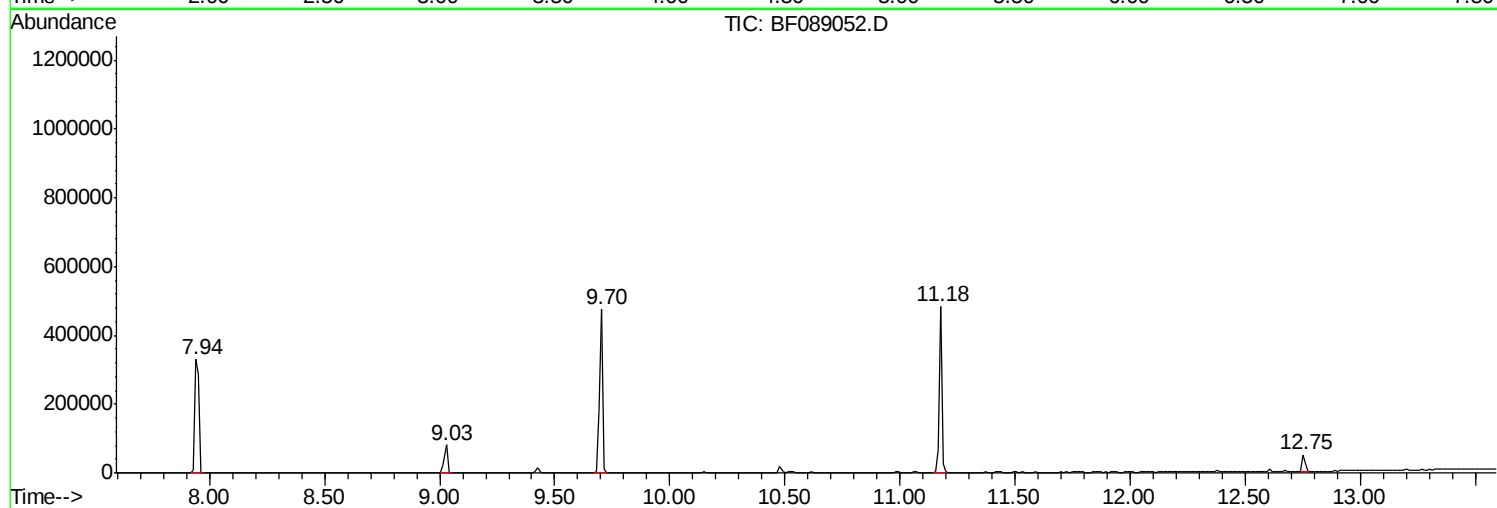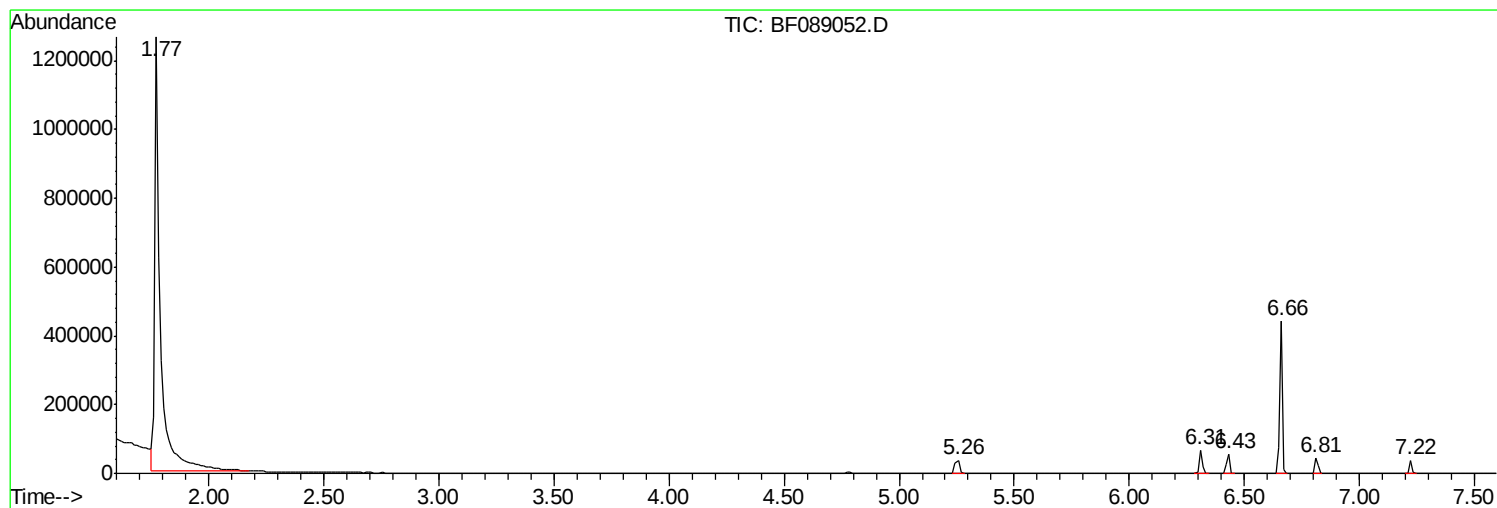

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF071616\
Data File : BF089052.D
Acq On : 16 Jul 2016 13:37
Operator : UM/SJ
Sample : H3951-15 10X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
LSS-SB-SB05(2-4ft)










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown6.43 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.43	3.11 ng	56703	1,4-Dichlorobenzene-d4	6.66

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	25
2			4-Chloro-2-fluoro-pyrimidine	132	C4H2ClFN2	051422-00-5	9
3			Xenon	132	Xe	007440-63-3	9
4			5-Aminoindole	132	C8H8N2	005192-03-0	9
5			4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	9

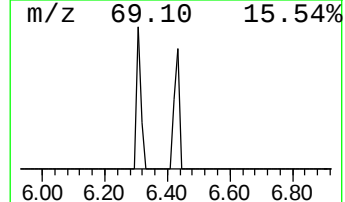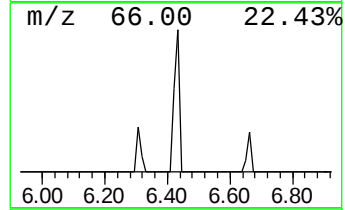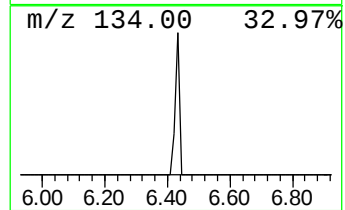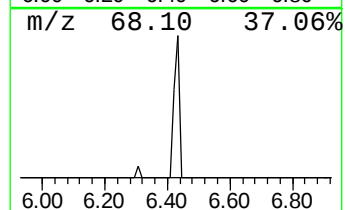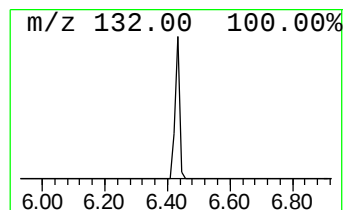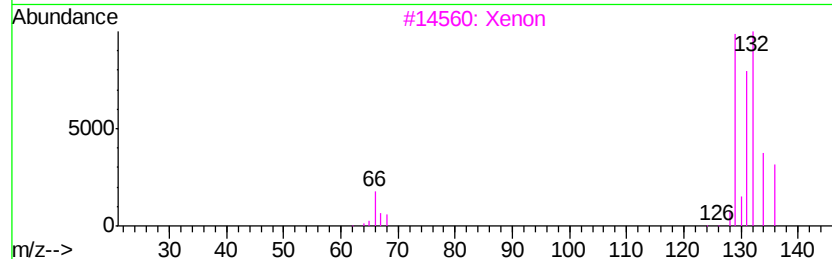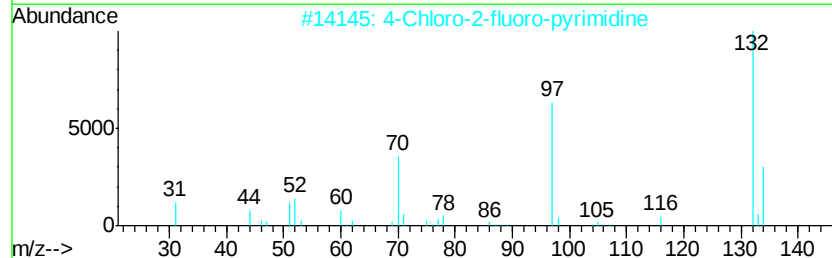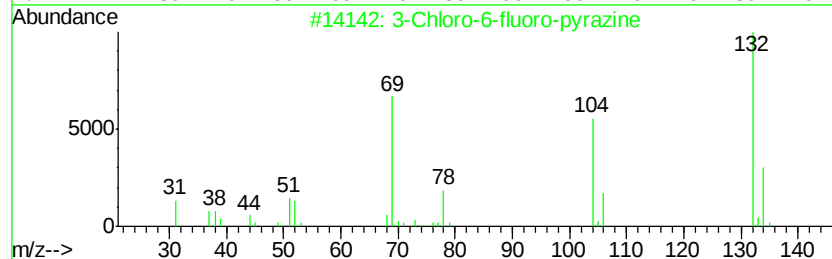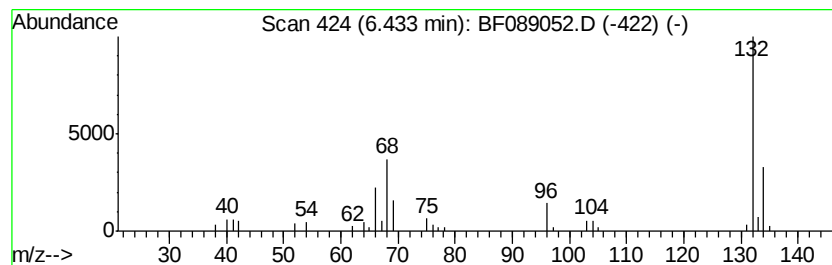

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF071616\
Data File : BF089052.D
Acq On : 16 Jul 2016 13:37
Operator : UM/SJ
Sample : H3951-15 10X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
LSS-SB-SB05(2-4ft)

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.43	6.43	3.1	ng	56703	1	6.66	364709	20.0