


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF071616\
 Data File : BF089046.D
 Acq On : 16 Jul 2016 10:05
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jul 11 18:13:32 2016

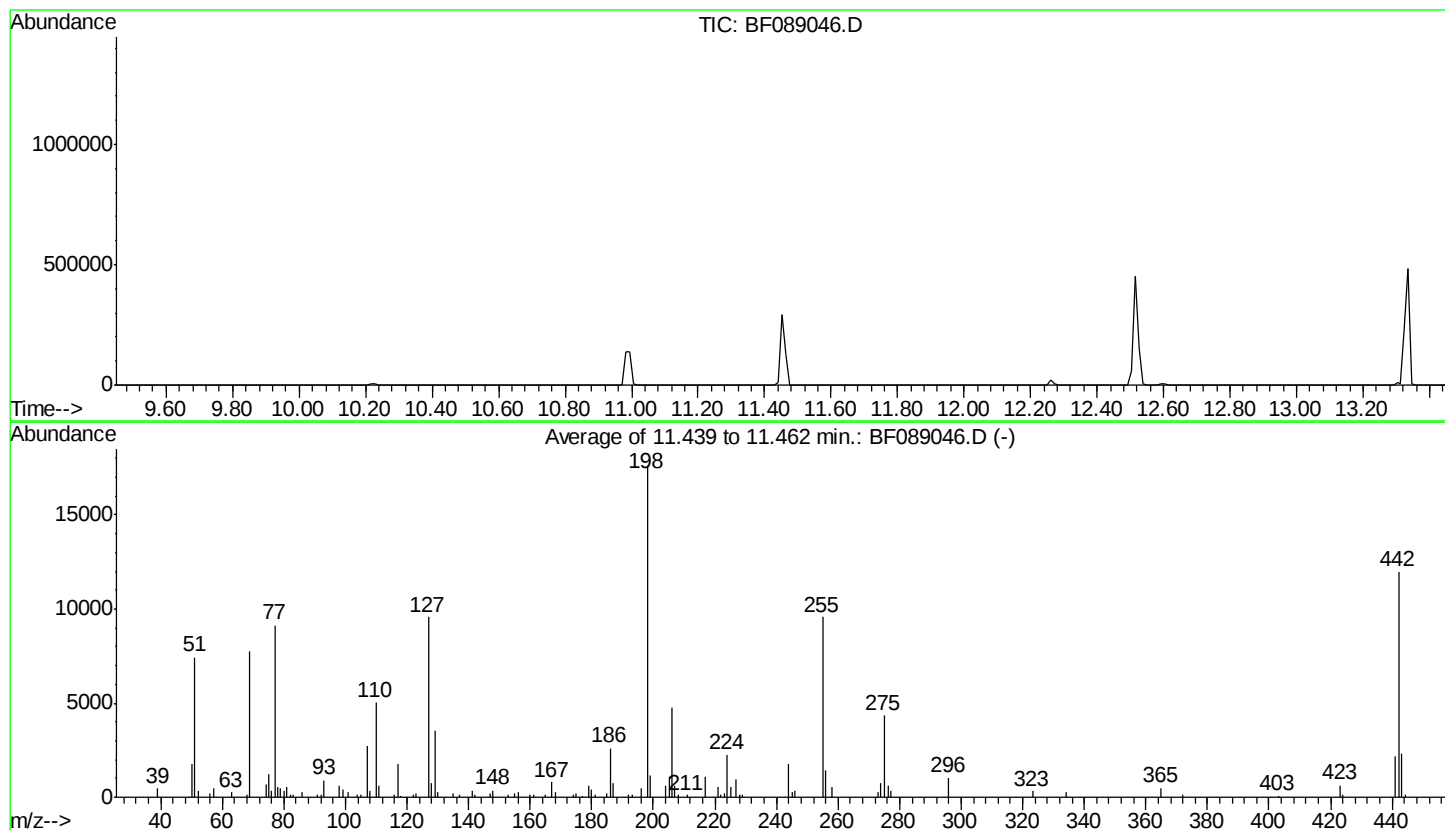

AutoFind: Scans 862, 863, 864; Background Corrected with Scan 859

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.2	7431	PASS
68	69	0.00	2	1.5	115	PASS
69	198	0.00	100	44.0	7752	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	54.3	9565	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	17616	PASS
199	198	5	9	6.7	1173	PASS
275	198	10	60	24.6	4327	PASS
365	198	1	100	2.7	479	PASS
441	442	0.01	24	17.9	2145	PASS
442	198	50	100	68.1	11992	PASS
443	442	15	24	19.5	2341	PASS