
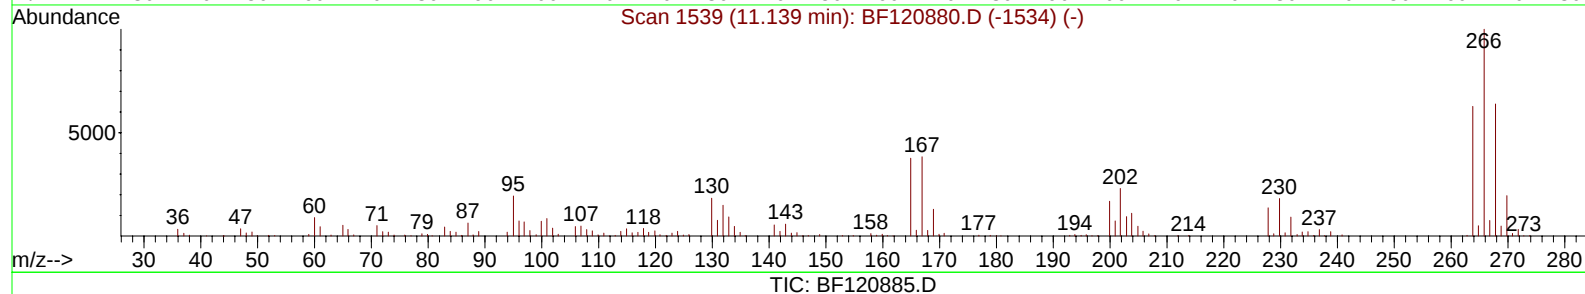
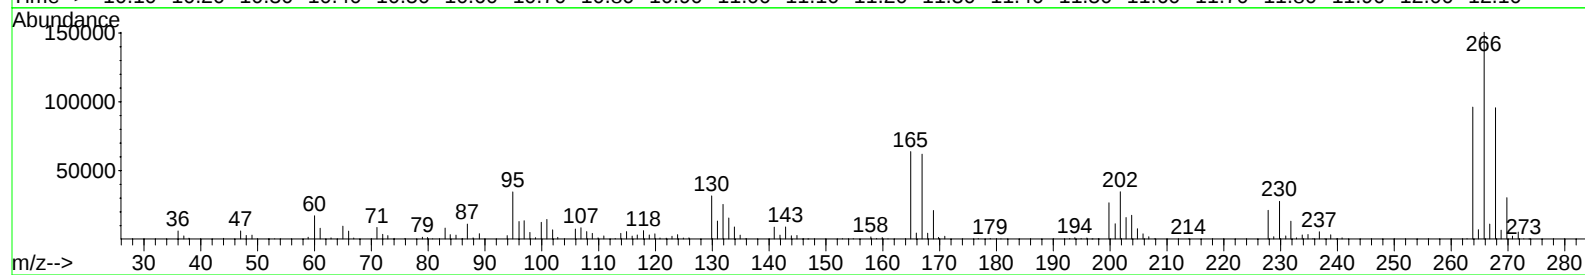


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF071620\
 Data File : BF120885.D
 Acq On : 16 Jul 2020 14:55
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 16 17:04:12 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071620.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 16 14:20:32 2020
 Response via : Initial Calibration

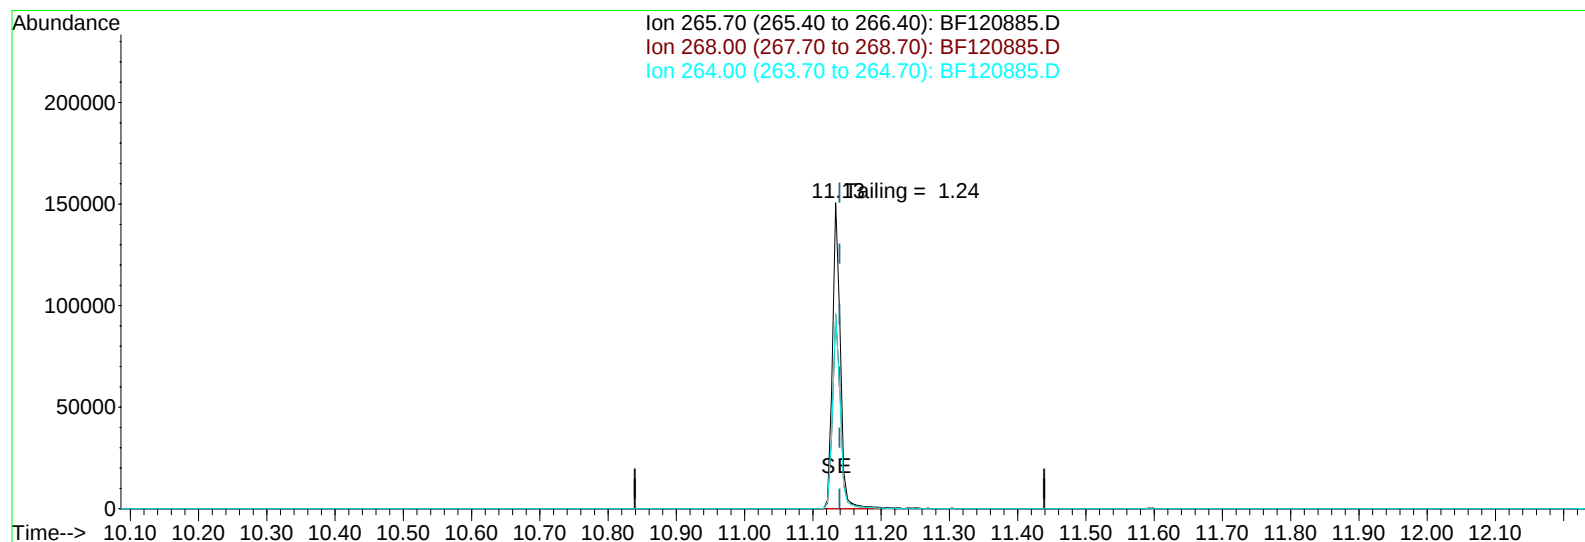

(70) Pentachlorophenol (C)




11.133min (-0.006) 37653.29ng

response 120453

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.57
264.00	62.70	63.84
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF071620\
 Data File : BF120885.D
 Acq On : 16 Jul 2020 14:55
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 16 17:04:12 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071620.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 16 14:20:32 2020
 Response via : Initial Calibration

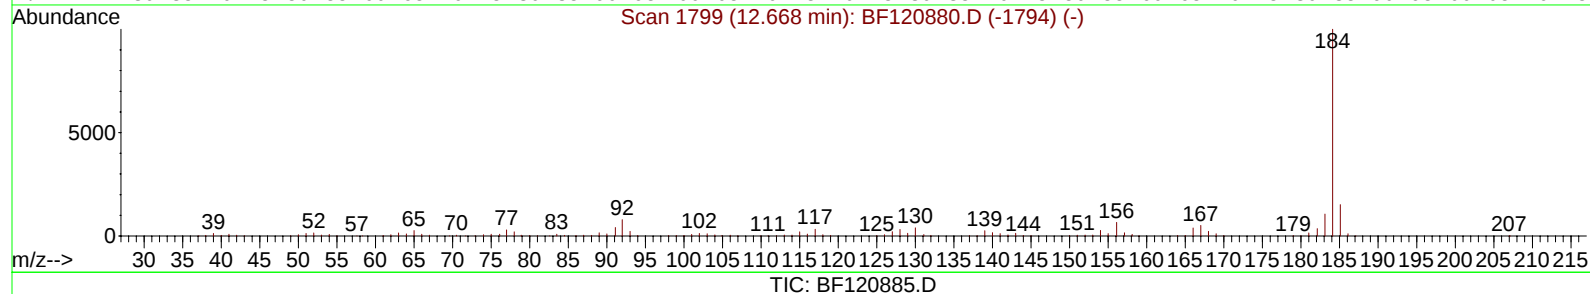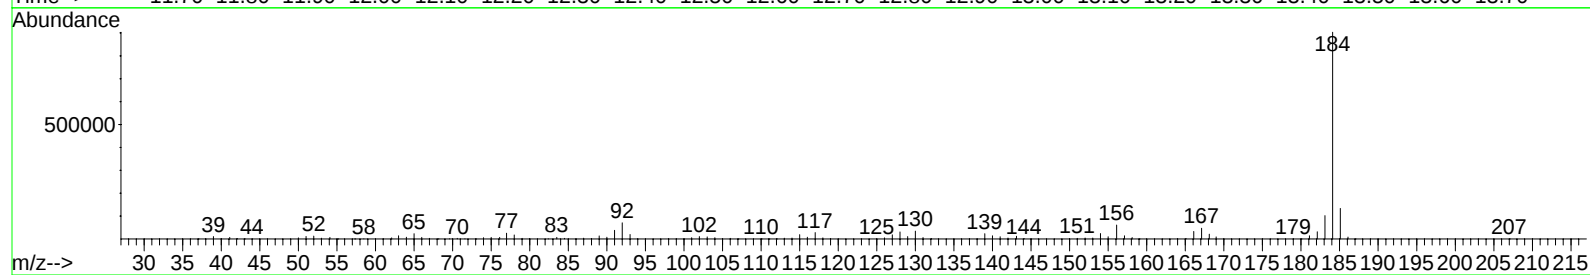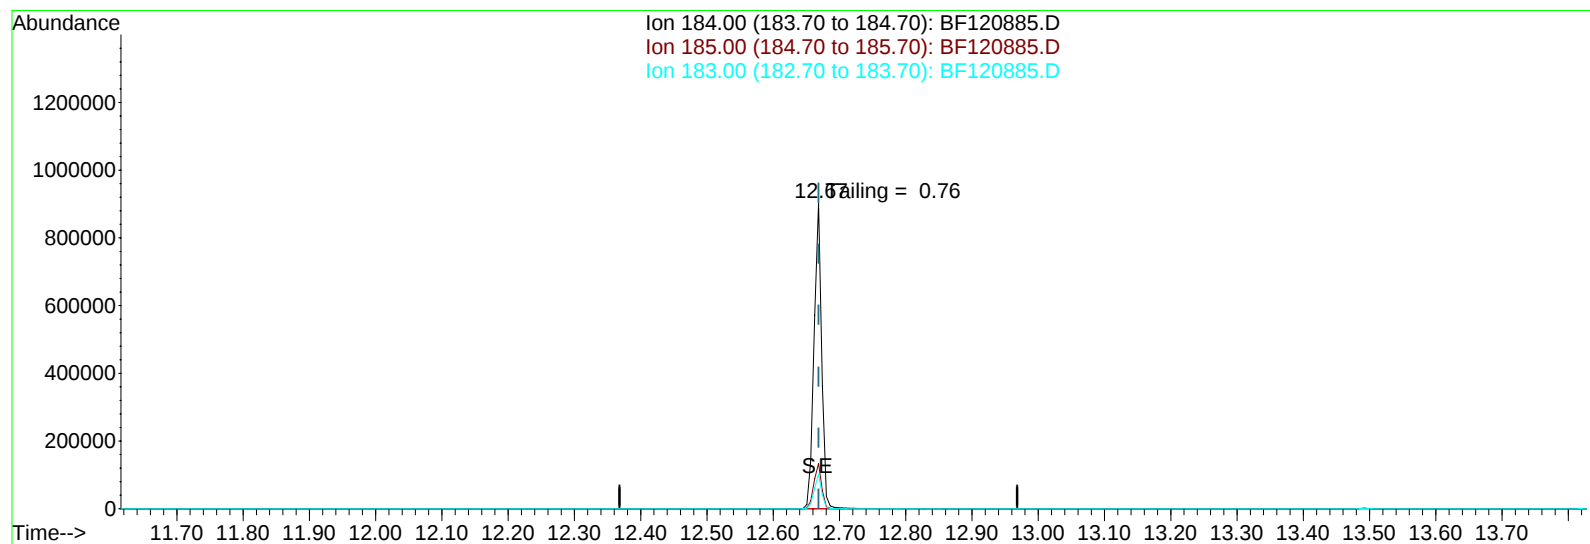

(77) Benzidine

12.668min (+0.000) 0.00ng

response 727718

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	14.83
183.00	10.60	11.32
0.00	0.00	0.00